

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030661.D
 Acq On : 19 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02360-17 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	80665	87257	6.35%	1.158%
2	1.536	148	154	164	rVB	81396	91134	6.63%	1.209%
3	2.066	310	319	333	rBV2	171837	259563	18.89%	3.443%
4	2.230	366	370	371	rBV3	2111	1352	0.10%	0.018%
5	2.638	495	497	500	rBV4	1207	657	0.05%	0.009%
6	2.687	510	512	514	rBV3	1981	954	0.07%	0.013%
7	2.876	569	571	574	rVB3	1982	1060	0.08%	0.014%
8	2.966	597	599	601	rBV2	1424	769	0.06%	0.010%
9	3.047	620	624	628	rBV5	1713	1483	0.11%	0.020%
10	3.076	630	633	637	rVB5	1176	743	0.05%	0.010%
11	3.095	637	639	642	rBV4	1182	874	0.06%	0.012%
12	3.240	680	684	687	rBV5	1410	1307	0.10%	0.017%
13	3.442	743	747	748	rBV4	1337	971	0.07%	0.013%
14	3.648	809	811	813	rBV3	2078	834	0.06%	0.011%
15	3.799	847	858	884	rBV2	58523	197896	14.40%	2.625%
16	4.259	989	1001	1026	rVB	120822	307079	22.35%	4.074%
17	4.613	1109	1111	1112	rBV2	1573	839	0.06%	0.011%
18	4.966	1205	1221	1242	rBV2	269348	722906	52.62%	9.590%
19	5.313	1326	1329	1331	rBV5	1620	935	0.07%	0.012%
20	5.387	1349	1352	1353	rBV3	1199	743	0.05%	0.010%
21	5.429	1363	1365	1366	rBV2	1618	812	0.06%	0.011%
22	5.484	1378	1382	1384	rBV4	1972	1559	0.11%	0.021%
23	5.542	1388	1400	1422	rVV	274000	564468	41.08%	7.488%
24	5.841	1479	1493	1515	rBV	691474	1373943	100.00%	18.227%
25	5.998	1532	1542	1562	rVB	167927	347251	25.27%	4.607%
26	6.391	1661	1664	1668	rBV5	1131	1228	0.09%	0.016%
27	6.465	1685	1687	1691	rVB5	2103	1520	0.11%	0.020%
28	6.487	1691	1694	1698	rBV6	1347	1273	0.09%	0.017%
29	6.571	1714	1720	1723	rBV7	2176	2292	0.17%	0.030%
30	6.600	1727	1729	1730	rBV2	2361	962	0.07%	0.013%
31	6.735	1768	1771	1773	rBV4	1895	1170	0.09%	0.016%
32	6.799	1789	1791	1793	rVB3	1891	822	0.06%	0.011%
33	6.815	1793	1796	1798	rBV4	1396	1064	0.08%	0.014%
34	6.831	1799	1801	1806	rBV6	1355	937	0.07%	0.012%
35	6.921	1818	1829	1846	rBV2	88149	164682	11.99%	2.185%
36	7.252	1921	1932	1955	rBV	298807	532587	38.76%	7.065%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041923\
 Data File : VW030661.D
 Acq On : 19 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02360-17 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.529	2015	2018	2019	rBV3	1728	985	0.07%	0.013%
38	7.561	2019	2028	2045	rVV	62655	114008	8.30%	1.512%
39	7.847	2115	2117	2119	rBV3	1204	687	0.05%	0.009%
40	7.860	2119	2121	2125	rVB5	1697	747	0.05%	0.010%
41	7.883	2125	2128	2129	rBV3	1451	722	0.05%	0.010%
42	7.940	2144	2146	2151	rBV4	1329	1214	0.09%	0.016%
43	8.034	2165	2175	2193	rBV	174114	327016	23.80%	4.338%
44	8.368	2276	2279	2282	rBV4	2362	1598	0.12%	0.021%
45	8.792	2400	2411	2437	rBV	415456	724231	52.71%	9.608%
46	9.088	2500	2503	2506	rVB5	1931	1182	0.09%	0.016%
47	9.165	2525	2527	2530	rBV3	1102	776	0.06%	0.010%
48	9.214	2540	2542	2544	rBV4	1613	862	0.06%	0.011%
49	9.419	2603	2606	2609	rBV5	1637	1310	0.10%	0.017%
50	9.509	2632	2634	2637	rBV4	1801	1442	0.10%	0.019%
51	9.551	2645	2647	2652	rVB5	1331	1070	0.08%	0.014%
52	9.593	2657	2660	2662	rBV4	1862	1209	0.09%	0.016%
53	9.683	2687	2688	2690	rBV2	1363	712	0.05%	0.009%
54	9.760	2709	2712	2715	rBV4	1636	1529	0.11%	0.020%
55	9.950	2768	2771	2773	rBV4	1498	898	0.07%	0.012%
56	10.091	2813	2815	2818	rBV4	1298	700	0.05%	0.009%
57	10.162	2827	2837	2854	rVB	240765	390080	28.39%	5.175%
58	10.275	2871	2872	2876	rVB4	1386	801	0.06%	0.011%
59	10.593	2969	2971	2974	rBV3	1031	708	0.05%	0.009%
60	10.693	2998	3002	3003	rBV4	1828	1161	0.08%	0.015%
61	10.757	3020	3022	3027	rVB6	1734	1202	0.09%	0.016%
62	10.789	3030	3032	3033	rBV2	1458	725	0.05%	0.010%
63	10.908	3068	3069	3071	rBV2	1283	664	0.05%	0.009%
64	11.011	3099	3101	3104	rVB4	1991	909	0.07%	0.012%
65	11.194	3147	3158	3178	rBV	403742	663214	48.27%	8.798%
66	11.570	3262	3275	3294	rBV	348448	577621	42.04%	7.663%
67	11.702	3314	3316	3319	rBV4	1428	887	0.06%	0.012%
68	11.786	3339	3342	3344	rBV4	1642	1173	0.09%	0.016%
69	11.892	3370	3375	3377	rBV6	1303	1079	0.08%	0.014%
70	11.918	3379	3383	3387	rVV7	1687	1393	0.10%	0.018%
71	11.998	3406	3408	3411	rBV4	1623	1155	0.08%	0.015%
72	12.169	3458	3461	3463	rBV4	2122	1426	0.10%	0.019%
73	12.214	3473	3475	3478	rBV4	1143	681	0.05%	0.009%
74	12.246	3482	3485	3489	rBV6	1643	1303	0.09%	0.017%
75	12.265	3489	3491	3494	rBV4	1071	852	0.06%	0.011%
76	12.332	3506	3512	3515	rBV7	1850	2180	0.16%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030661.D
 Acq On : 19 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02360-17 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.509	3563	3567	3569	rBV5	1878	1501	0.11%	0.020%
78	12.567	3582	3585	3588	rVB5	1337	686	0.05%	0.009%
79	12.583	3588	3590	3591	rVV2	1654	657	0.05%	0.009%
80	12.622	3600	3602	3606	rVB5	1910	1179	0.09%	0.016%
81	12.680	3617	3620	3621	rBV3	1102	702	0.05%	0.009%
82	12.689	3621	3623	3627	rVB5	1798	990	0.07%	0.013%
83	12.728	3632	3635	3637	rVV4	1684	942	0.07%	0.012%
84	12.776	3647	3650	3653	rBV5	1716	1343	0.10%	0.018%
85	12.898	3685	3688	3690	rBV4	1284	709	0.05%	0.009%
86	13.030	3727	3729	3732	rBV4	1651	1097	0.08%	0.015%
87	13.181	3771	3776	3777	rBV3	1844	1601	0.12%	0.021%
88	13.300	3811	3813	3819	rVB7	1381	981	0.07%	0.013%
89	13.426	3847	3852	3853	rBV5	1661	1377	0.10%	0.018%
90	13.545	3885	3889	3891	rBV4	1708	1151	0.08%	0.015%
91	13.693	3929	3935	3939	rBV10	3425	3875	0.28%	0.051%
92	13.767	3954	3958	3959	rBV3	1375	972	0.07%	0.013%
93	13.866	3987	3989	3992	rBV4	1569	855	0.06%	0.011%
94	14.165	4081	4082	4086	rBV4	1219	770	0.06%	0.010%
95	14.471	4174	4177	4179	rBV4	1250	846	0.06%	0.011%
96	14.484	4179	4181	4185	rBV5	1999	1614	0.12%	0.021%
97	14.535	4193	4197	4198	rBV4	1727	1208	0.09%	0.016%
98	14.673	4237	4240	4242	rBV4	1464	972	0.07%	0.013%
99	14.783	4270	4274	4280	rBV7	2441	3059	0.22%	0.041%
100	15.146	4384	4387	4388	rBV3	1966	964	0.07%	0.013%




Sum of corrected areas: 7538089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030661.D
Acq On : 19 Apr 2023 13:48
Operator : SY/MD
Sample : 02360-17 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

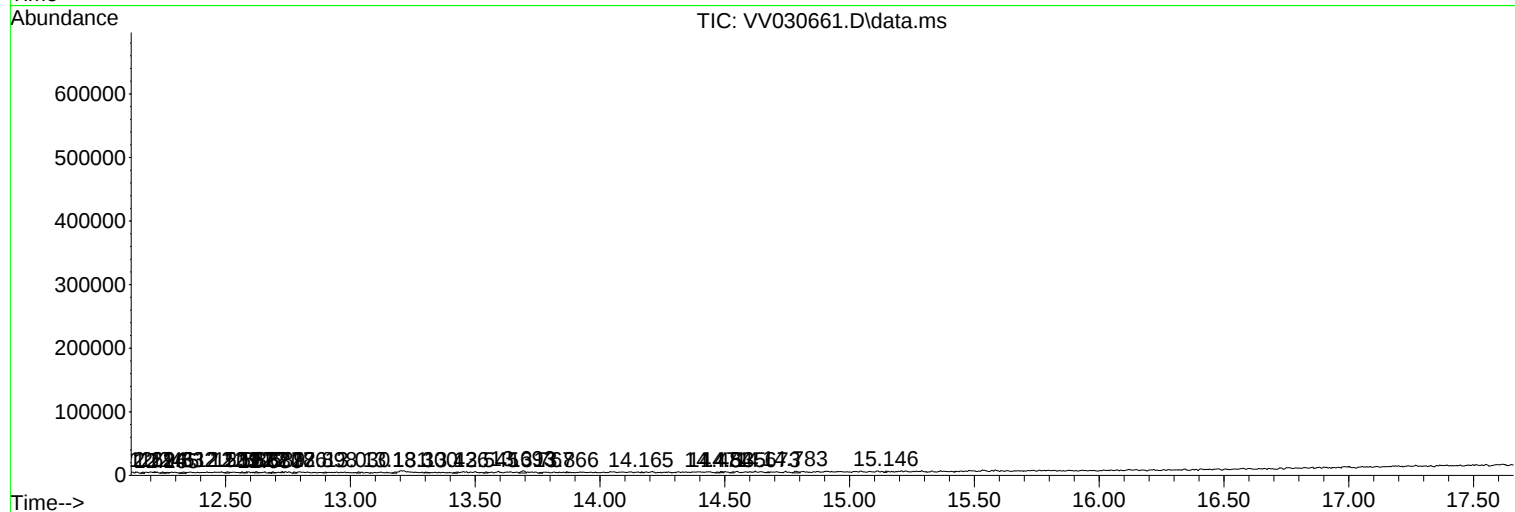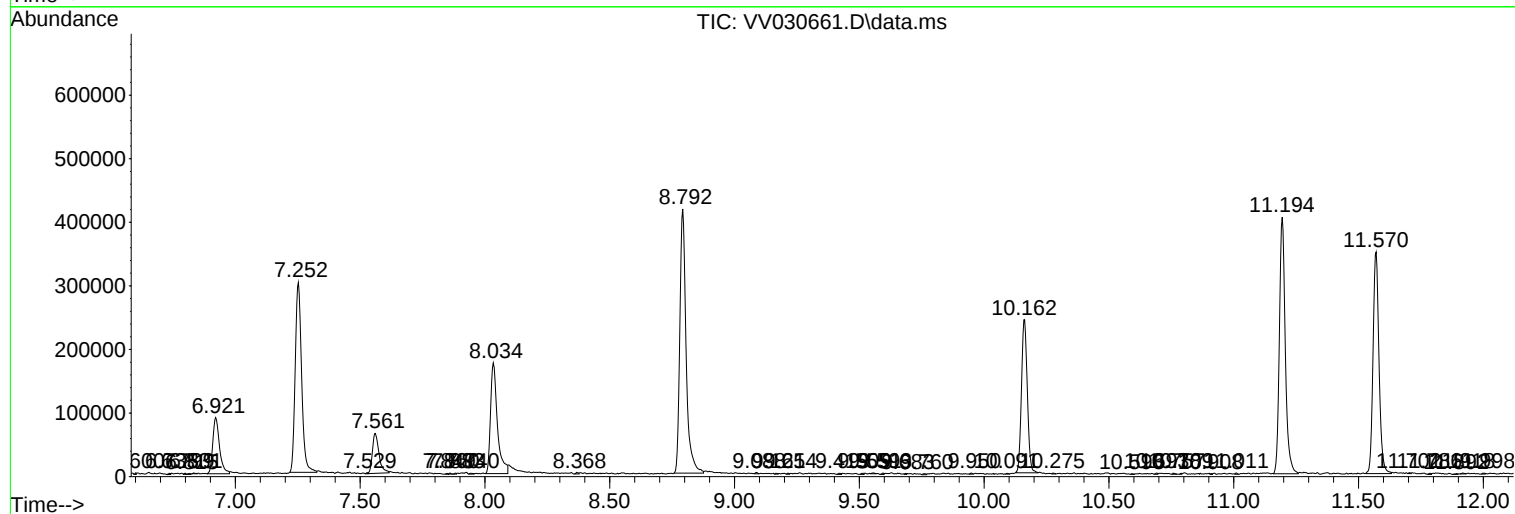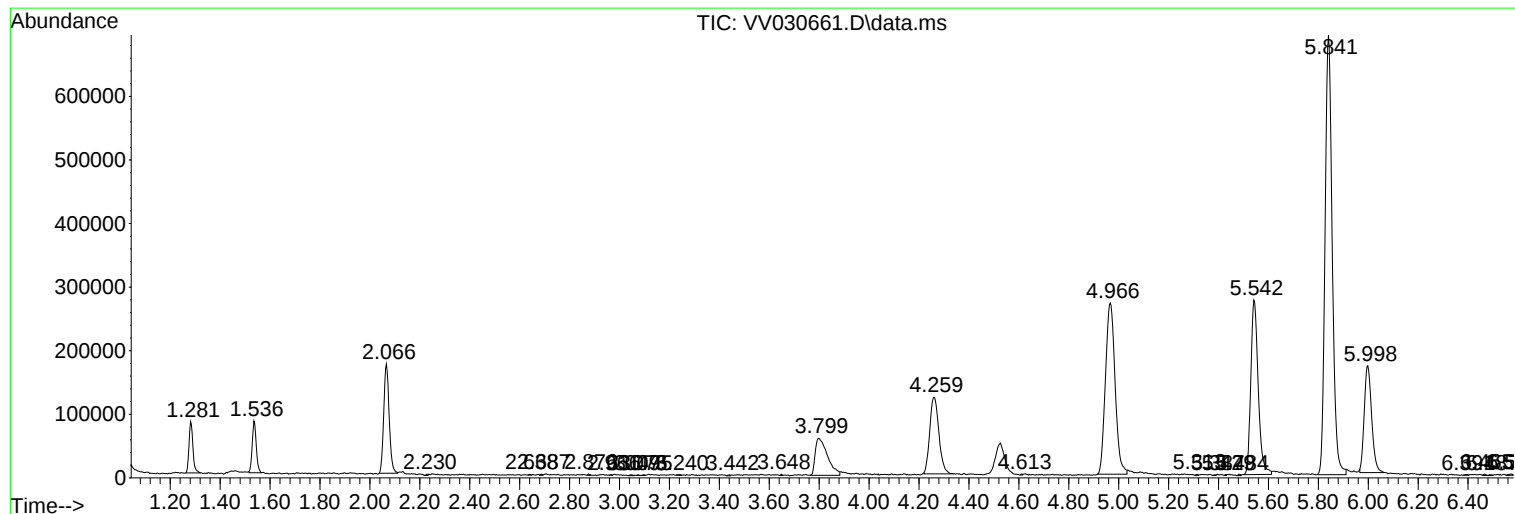

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030661.D
Acq On : 19 Apr 2023 13:48
Operator : SY/MD
Sample : 02360-17 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030661.D
Acq On : 19 Apr 2023 13:48
Operator : SY/MD
Sample : 02360-17 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc