

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030665.D
 Acq On : 19 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02360-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	81044	85666	2.90%	0.947%
2	1.536	148	154	168	rVB	78884	93423	3.16%	1.033%
3	2.066	311	319	334	rVB2	170019	256625	8.69%	2.837%
4	2.400	419	423	424	rBV3	1104	603	0.02%	0.007%
5	2.539	464	466	468	rBV3	1600	861	0.03%	0.010%
6	2.581	477	479	481	rBV3	795	337	0.01%	0.004%
7	2.790	540	544	545	rBV4	1432	728	0.02%	0.008%
8	2.799	545	547	548	rBV2	1155	504	0.02%	0.006%
9	2.979	600	603	605	rBV4	821	473	0.02%	0.005%
10	3.018	611	615	617	rBV4	1953	1303	0.04%	0.014%
11	3.169	658	662	663	rBV4	1731	713	0.02%	0.008%
12	3.201	671	672	675	rVB3	1458	492	0.02%	0.005%
13	3.265	689	692	693	rBV3	1248	626	0.02%	0.007%
14	3.291	699	700	704	rVB4	1932	884	0.03%	0.010%
15	3.310	704	706	708	rBV3	1668	966	0.03%	0.011%
16	3.343	713	716	717	rBV3	1068	556	0.02%	0.006%
17	3.365	721	723	726	rVV4	1475	783	0.03%	0.009%
18	3.394	729	732	733	rBV3	1172	597	0.02%	0.007%
19	3.420	739	740	741	rBV	1199	379	0.01%	0.004%
20	3.458	748	752	756	rVB7	2006	1922	0.07%	0.021%
21	3.484	756	760	762	rBV5	1753	1171	0.04%	0.013%
22	3.529	771	774	777	rBV5	1410	1102	0.04%	0.012%
23	3.687	820	823	824	rBV3	1106	508	0.02%	0.006%
24	3.761	845	846	849	rBV3	941	570	0.02%	0.006%
25	3.822	849	865	887	rBV3	91793	313677	10.62%	3.467%
26	4.259	989	1001	1025	rVB	120154	301190	10.20%	3.329%
27	4.754	1154	1155	1158	rBV3	1152	547	0.02%	0.006%
28	4.966	1202	1221	1246	rBV3	264161	718039	24.32%	7.937%
29	5.465	1374	1376	1377	rBV2	798	316	0.01%	0.003%
30	5.478	1377	1380	1382	rBV3	1601	1081	0.04%	0.012%
31	5.542	1387	1400	1422	rBV	267152	556955	18.86%	6.156%
32	5.841	1478	1493	1514	rBV	1518940	2952418	100.00%	32.635%
33	5.998	1532	1542	1562	rVB	162189	332874	11.27%	3.680%
34	6.500	1696	1698	1700	rBV4	1645	850	0.03%	0.009%
35	6.651	1743	1745	1748	rVB4	1307	787	0.03%	0.009%
36	6.844	1803	1805	1809	rBV4	1289	1094	0.04%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030665.D
 Acq On : 19 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02360-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.876	1813	1815	1816	rBV2	1582	696	0.02%	0.008%
38	6.921	1819	1829	1848	rVV	81718	155364	5.26%	1.717%
39	7.162	1899	1904	1906	rBV5	2120	1928	0.07%	0.021%
40	7.194	1911	1914	1917	rVB5	1252	734	0.02%	0.008%
41	7.252	1920	1932	1949	rBV	280805	506096	17.14%	5.594%
42	7.465	1996	1998	2003	rBV6	1574	960	0.03%	0.011%
43	7.561	2020	2028	2040	rBV	56165	94936	3.22%	1.049%
44	7.757	2086	2089	2090	rBV3	1535	835	0.03%	0.009%
45	7.847	2113	2117	2118	rBV3	1035	648	0.02%	0.007%
46	7.857	2118	2120	2122	rBV3	940	402	0.01%	0.004%
47	7.886	2123	2129	2131	rBV7	3939	4418	0.15%	0.049%
48	7.928	2140	2142	2145	rVB4	1344	539	0.02%	0.006%
49	8.034	2165	2175	2206	rBV	160086	324051	10.98%	3.582%
50	8.329	2265	2267	2271	rBV5	1648	932	0.03%	0.010%
51	8.741	2392	2395	2397	rBV4	1018	617	0.02%	0.007%
52	8.792	2400	2411	2433	rVV	397994	700597	23.73%	7.744%
53	9.111	2506	2510	2515	rVB7	1619	1612	0.05%	0.018%
54	9.137	2515	2518	2519	rBV3	1383	844	0.03%	0.009%
55	9.400	2595	2600	2604	rBV7	2549	2932	0.10%	0.032%
56	9.426	2604	2608	2610	rVV3	1813	1235	0.04%	0.014%
57	9.481	2623	2625	2627	rBV2	784	333	0.01%	0.004%
58	9.628	2669	2671	2673	rVB2	1635	699	0.02%	0.008%
59	9.718	2694	2699	2700	rBV4	1460	1239	0.04%	0.014%
60	9.969	2776	2777	2780	rVB3	1354	526	0.02%	0.006%
61	10.001	2784	2787	2790	rBV5	1942	1269	0.04%	0.014%
62	10.085	2811	2813	2815	rBV4	1173	569	0.02%	0.006%
63	10.159	2825	2836	2856	rBV	232138	384900	13.04%	4.255%
64	10.336	2883	2891	2898	rBV5	5686	8464	0.29%	0.094%
65	10.429	2916	2920	2921	rBV4	2087	1138	0.04%	0.013%
66	10.471	2929	2933	2936	rBV6	2034	2168	0.07%	0.024%
67	10.500	2939	2942	2945	rVB5	1447	998	0.03%	0.011%
68	10.599	2970	2973	2976	rBV5	1211	1090	0.04%	0.012%
69	10.622	2978	2980	2984	rVB5	1514	775	0.03%	0.009%
70	10.706	3003	3006	3008	rBV3	1197	798	0.03%	0.009%
71	10.735	3013	3015	3018	rVB3	1189	584	0.02%	0.006%
72	10.773	3025	3027	3028	rBV2	1509	449	0.02%	0.005%
73	10.796	3028	3034	3037	rVB8	2093	2223	0.08%	0.025%
74	10.818	3037	3041	3043	rBV6	1717	1600	0.05%	0.018%
75	10.899	3063	3066	3068	rBV4	1398	875	0.03%	0.010%
76	11.091	3122	3126	3128	rBV5	1983	1667	0.06%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030665.D
 Acq On : 19 Apr 2023 15:22
 Operator : SY/MD
 Sample : 02360-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3147	3158	3180	rBV	387765	637448	21.59%	7.046%
78	11.423	3228	3229	3231	rBV2	1031	543	0.02%	0.006%
79	11.571	3264	3275	3294	rVB	328275	546521	18.51%	6.041%
80	11.972	3399	3400	3403	rVB3	1886	736	0.02%	0.008%
81	12.117	3443	3445	3447	rBV3	2828	1427	0.05%	0.016%
82	12.802	3656	3658	3660	rBV3	1980	1078	0.04%	0.012%
83	12.918	3692	3694	3696	rVB3	904	364	0.01%	0.004%
84	12.927	3696	3697	3700	rBV3	1140	494	0.02%	0.005%
85	13.117	3752	3756	3759	rBV6	1472	1398	0.05%	0.015%
86	13.181	3774	3776	3777	rBV2	1010	348	0.01%	0.004%
87	13.194	3778	3780	3781	rBV2	1814	781	0.03%	0.009%
88	13.400	3842	3844	3845	rBV2	1143	417	0.01%	0.005%
89	13.490	3869	3872	3874	rBV4	1126	781	0.03%	0.009%
90	13.525	3880	3883	3884	rBV3	1355	869	0.03%	0.010%
91	13.670	3926	3928	3931	rBV4	1287	976	0.03%	0.011%
92	13.731	3944	3947	3949	rBV3	1015	646	0.02%	0.007%
93	13.786	3962	3964	3965	rBV2	1022	453	0.02%	0.005%
94	13.879	3990	3993	3994	rBV2	1327	649	0.02%	0.007%
95	14.030	4039	4040	4043	rBV3	905	510	0.02%	0.006%
96	14.104	4061	4063	4065	rBV3	1314	762	0.03%	0.008%
97	14.130	4068	4071	4073	rBV4	1954	1413	0.05%	0.016%
98	14.188	4086	4089	4090	rBV2	922	570	0.02%	0.006%
99	14.564	4202	4206	4212	rBV7	2119	2200	0.07%	0.024%
100	14.744	4260	4262	4265	rBV4	1674	944	0.03%	0.010%




Sum of corrected areas: 9046688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030665.D
Acq On : 19 Apr 2023 15:22
Operator : SY/MD
Sample : 02360-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

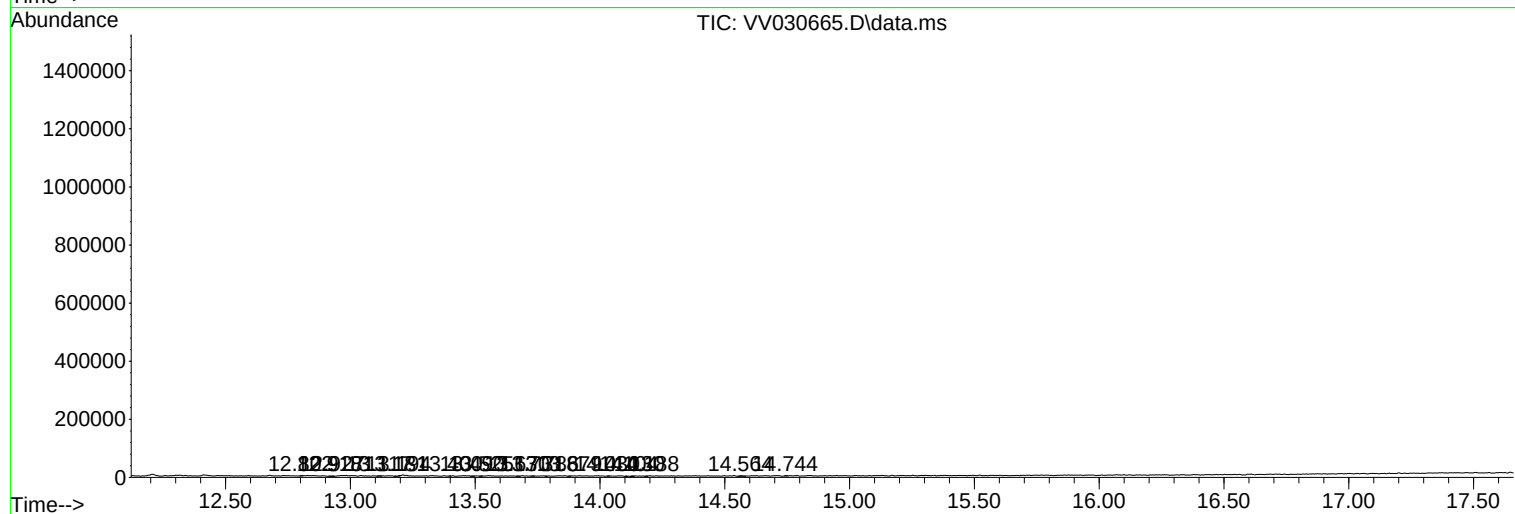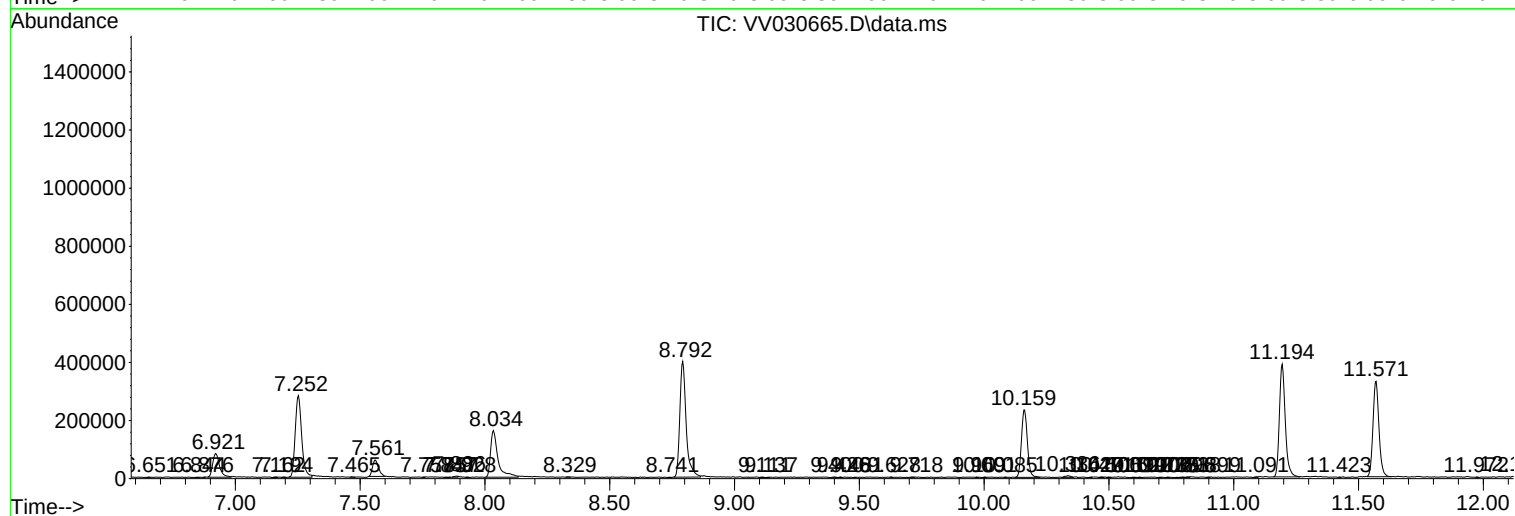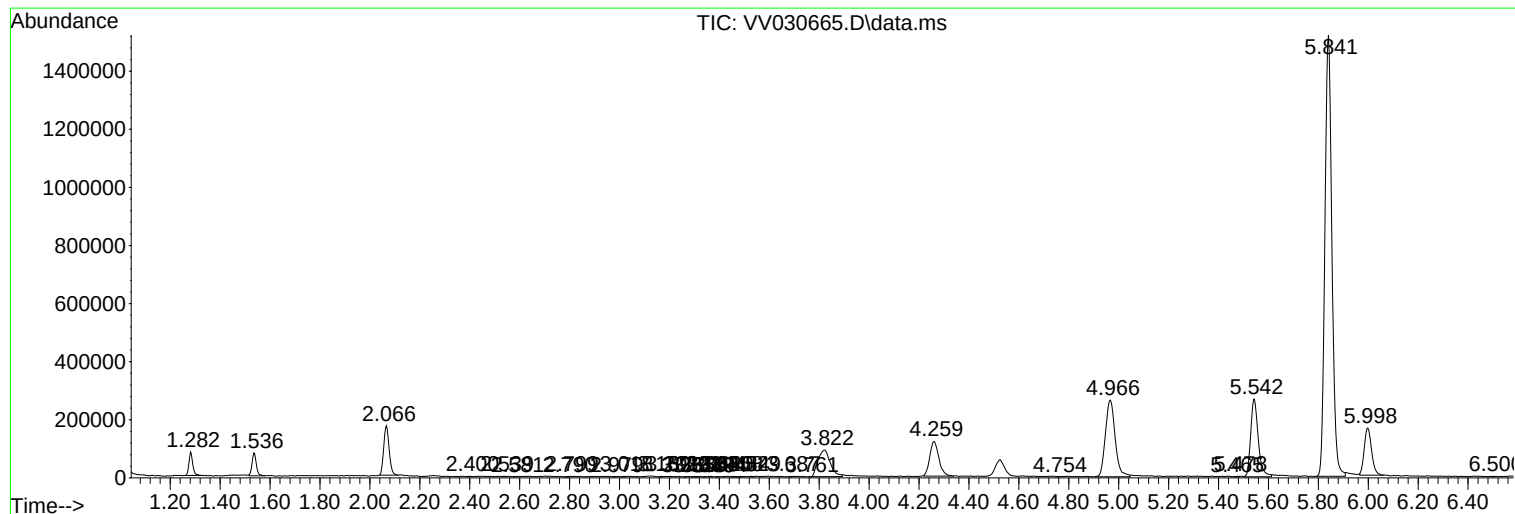

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030665.D
Acq On : 19 Apr 2023 15:22
Operator : SY/MD
Sample : 02360-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030665.D
Acq On : 19 Apr 2023 15:22
Operator : SY/MD
Sample : 02360-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------