

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030667.D
 Acq On : 19 Apr 2023 16:09
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	70	76	88	rVB	69754	76532	11.09%	1.332%
2	1.536	148	154	167	rVB	72526	86924	12.59%	1.513%
3	2.066	310	319	331	rBV	140483	202056	29.28%	3.517%
4	2.420	427	429	431	rBV3	1018	623	0.09%	0.011%
5	2.503	451	455	456	rBV3	1332	864	0.13%	0.015%
6	2.706	513	518	520	rBV6	1828	1578	0.23%	0.027%
7	2.786	539	543	546	rBV6	1223	919	0.13%	0.016%
8	2.806	547	549	553	rVB4	1830	956	0.14%	0.017%
9	2.925	584	586	589	rBV4	1268	884	0.13%	0.015%
10	2.950	591	594	596	rVB5	998	583	0.08%	0.010%
11	3.040	620	622	625	rBV4	1511	997	0.14%	0.017%
12	3.108	639	643	646	rBV5	1812	1721	0.25%	0.030%
13	3.214	673	676	677	rBV3	1611	933	0.14%	0.016%
14	3.224	677	679	683	rVV4	1597	1103	0.16%	0.019%
15	3.285	696	698	700	rVB3	1535	640	0.09%	0.011%
16	3.304	701	704	707	rVB4	1415	911	0.13%	0.016%
17	3.368	721	724	725	rBV3	1125	609	0.09%	0.011%
18	3.429	736	743	745	rBV8	1673	2012	0.29%	0.035%
19	3.478	755	758	761	rVB5	1360	887	0.13%	0.015%
20	3.516	766	770	772	rBV5	2162	1413	0.20%	0.025%
21	3.535	772	776	778	rBV5	1358	1153	0.17%	0.020%
22	3.600	794	796	801	rVB4	2377	1732	0.25%	0.030%
23	3.664	810	816	817	rBV5	1392	1190	0.17%	0.021%
24	3.757	840	845	846	rBV5	1259	904	0.13%	0.016%
25	3.796	847	857	883	rVV2	67660	194080	28.12%	3.378%
26	4.259	988	1001	1021	rVB2	117346	297220	43.07%	5.173%
27	4.580	1096	1101	1103	rBV6	2257	1863	0.27%	0.032%
28	4.670	1126	1129	1131	rBV3	1320	1035	0.15%	0.018%
29	4.783	1162	1164	1166	rVB3	1707	787	0.11%	0.014%
30	4.966	1206	1221	1244	rBV2	258302	690147	100.00%	12.013%
31	5.478	1378	1380	1383	rBV4	1425	787	0.11%	0.014%
32	5.542	1389	1400	1422	rBV	243804	506996	73.46%	8.825%
33	5.728	1456	1458	1460	rBV2	1702	885	0.13%	0.015%
34	5.998	1531	1542	1561	rBV	165424	327737	47.49%	5.705%
35	6.326	1642	1644	1647	rBV3	1497	896	0.13%	0.016%
36	6.921	1820	1829	1851	rBV	82269	148109	21.46%	2.578%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030667.D
 Acq On : 19 Apr 2023 16:09
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.043	1865	1867	1869	rBV3	1484	767	0.11%	0.013%
38	7.130	1891	1894	1895	rBV3	1332	761	0.11%	0.013%
39	7.252	1922	1932	1951	rBV	268519	471417	68.31%	8.206%
40	7.561	2020	2028	2041	rBV	57520	97665	14.15%	1.700%
41	7.696	2068	2070	2072	rBV2	1167	568	0.08%	0.010%
42	8.034	2162	2175	2207	rBV	179589	363961	52.74%	6.335%
43	8.545	2332	2334	2339	rVB6	1541	936	0.14%	0.016%
44	8.603	2349	2352	2354	rBV4	1053	654	0.09%	0.011%
45	8.728	2389	2391	2394	rBV3	1277	754	0.11%	0.013%
46	8.792	2400	2411	2435	rVV	380086	665232	96.39%	11.579%
47	9.284	2559	2564	2567	rBV6	1534	1548	0.22%	0.027%
48	9.365	2585	2589	2591	rBV5	1541	1141	0.17%	0.020%
49	9.423	2604	2607	2611	rVV5	1433	998	0.14%	0.017%
50	9.455	2615	2617	2619	rVV3	1371	574	0.08%	0.010%
51	9.571	2652	2653	2657	rVB4	1714	792	0.11%	0.014%
52	9.616	2665	2667	2671	rVB4	2554	1287	0.19%	0.022%
53	9.645	2671	2676	2679	rBV7	1719	1630	0.24%	0.028%
54	9.760	2709	2712	2715	rBV5	1602	1382	0.20%	0.024%
55	9.847	2735	2739	2740	rBV4	1423	851	0.12%	0.015%
56	9.956	2771	2773	2780	rVB8	1281	965	0.14%	0.017%
57	10.005	2784	2788	2790	rBV4	1284	907	0.13%	0.016%
58	10.159	2823	2836	2855	rBV	252681	413190	59.87%	7.192%
59	10.445	2923	2925	2927	rBV3	1138	705	0.10%	0.012%
60	10.587	2965	2969	2971	rVV4	1410	931	0.13%	0.016%
61	10.767	3023	3025	3027	rVB3	1665	738	0.11%	0.013%
62	10.834	3044	3046	3049	rBV4	974	678	0.10%	0.012%
63	11.034	3106	3108	3112	rBV5	1082	660	0.10%	0.011%
64	11.104	3128	3130	3132	rBV3	1212	693	0.10%	0.012%
65	11.194	3147	3158	3178	rBV	355277	588282	85.24%	10.240%
66	11.374	3209	3214	3216	rBV7	1569	1216	0.18%	0.021%
67	11.571	3264	3275	3294	rVB	321311	527736	76.47%	9.186%
68	11.831	3354	3356	3358	rBV3	1340	608	0.09%	0.011%
69	11.895	3373	3376	3377	rBV2	1321	687	0.10%	0.012%
70	12.053	3423	3425	3428	rBV4	1529	1055	0.15%	0.018%
71	12.146	3451	3454	3456	rBV4	1432	977	0.14%	0.017%
72	12.169	3456	3461	3466	rVB7	1326	1479	0.21%	0.026%
73	12.204	3466	3472	3475	rVB8	1858	2317	0.34%	0.040%
74	12.374	3520	3525	3529	rBV7	1958	1902	0.28%	0.033%
75	12.538	3573	3576	3577	rBV3	944	695	0.10%	0.012%
76	12.593	3591	3593	3597	rVB5	2067	1222	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030667.D
 Acq On : 19 Apr 2023 16:09
 Operator : SY/MD
 Sample : VIBLK202
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK202

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.667	3614	3616	3619	rVB4	1272	583	0.08%	0.010%
78	12.689	3619	3623	3625	rBV5	1144	731	0.11%	0.013%
79	12.751	3640	3642	3645	rBV4	1300	649	0.09%	0.011%
80	12.779	3649	3651	3656	rBV6	1223	881	0.13%	0.015%
81	13.111	3748	3754	3757	rBV7	1448	1963	0.28%	0.034%
82	13.188	3774	3778	3781	rBV6	1555	1464	0.21%	0.025%
83	13.210	3781	3785	3788	rBV6	3330	2922	0.42%	0.051%
84	13.271	3800	3804	3807	rBV6	1323	963	0.14%	0.017%
85	13.365	3829	3833	3834	rBV3	1274	791	0.11%	0.014%
86	13.442	3855	3857	3859	rBV2	1561	775	0.11%	0.013%
87	13.609	3906	3909	3912	rBV5	1267	1126	0.16%	0.020%
88	13.628	3912	3915	3916	rBV3	1371	674	0.10%	0.012%
89	13.641	3916	3919	3922	rVV5	1341	811	0.12%	0.014%
90	13.725	3944	3945	3948	rBV4	1195	579	0.08%	0.010%
91	13.837	3978	3980	3984	rVB5	1219	780	0.11%	0.014%
92	14.165	4080	4082	4087	rBV5	1264	767	0.11%	0.013%
93	14.233	4100	4103	4105	rVB3	1425	709	0.10%	0.012%
94	14.284	4114	4119	4120	rBV4	1226	858	0.12%	0.015%
95	14.294	4120	4122	4124	rBV2	1797	755	0.11%	0.013%
96	14.513	4187	4190	4195	rBV6	1304	1284	0.19%	0.022%
97	14.667	4235	4238	4243	rBV7	1661	1659	0.24%	0.029%
98	14.741	4259	4261	4270	rBV9	1515	2323	0.34%	0.040%
99	14.995	4337	4340	4342	rBV4	1705	958	0.14%	0.017%
100	15.185	4397	4399	4402	rBV4	1541	851	0.12%	0.015%




Sum of corrected areas: 5745083

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030667.D
Acq On : 19 Apr 2023 16:09
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

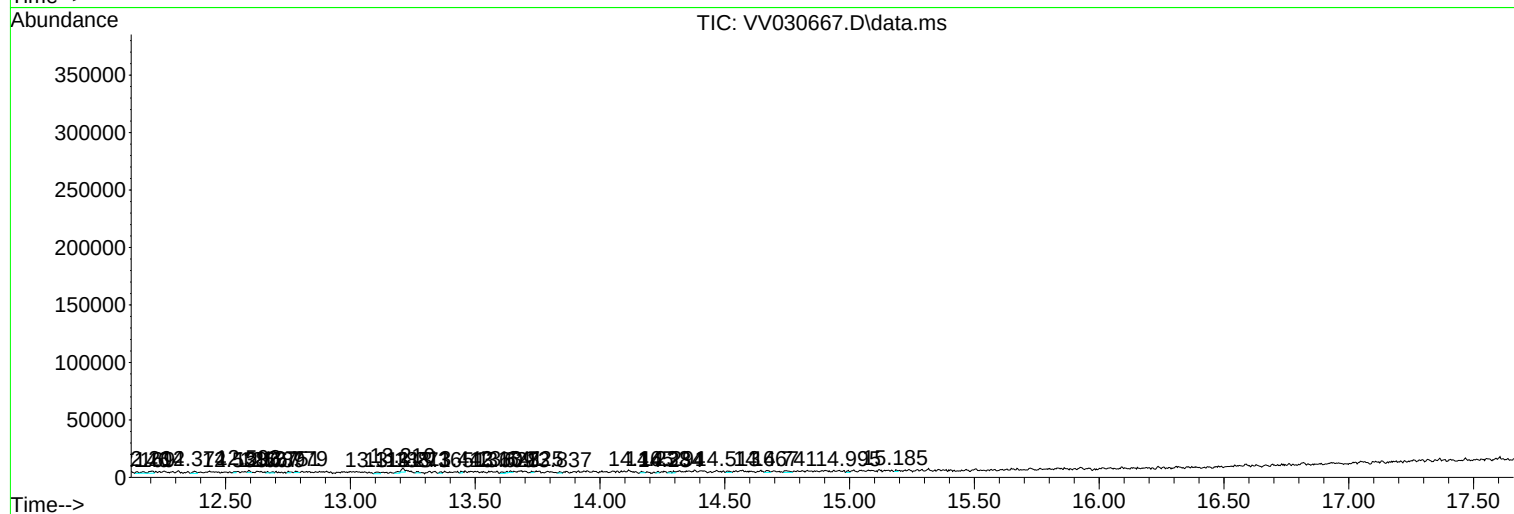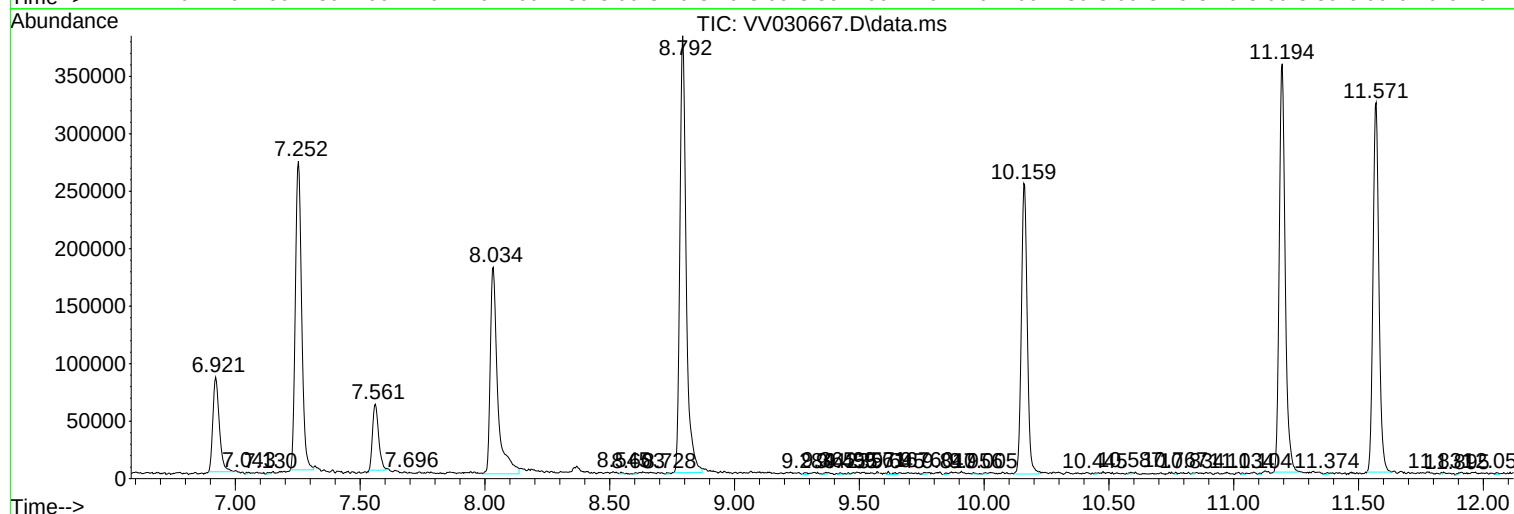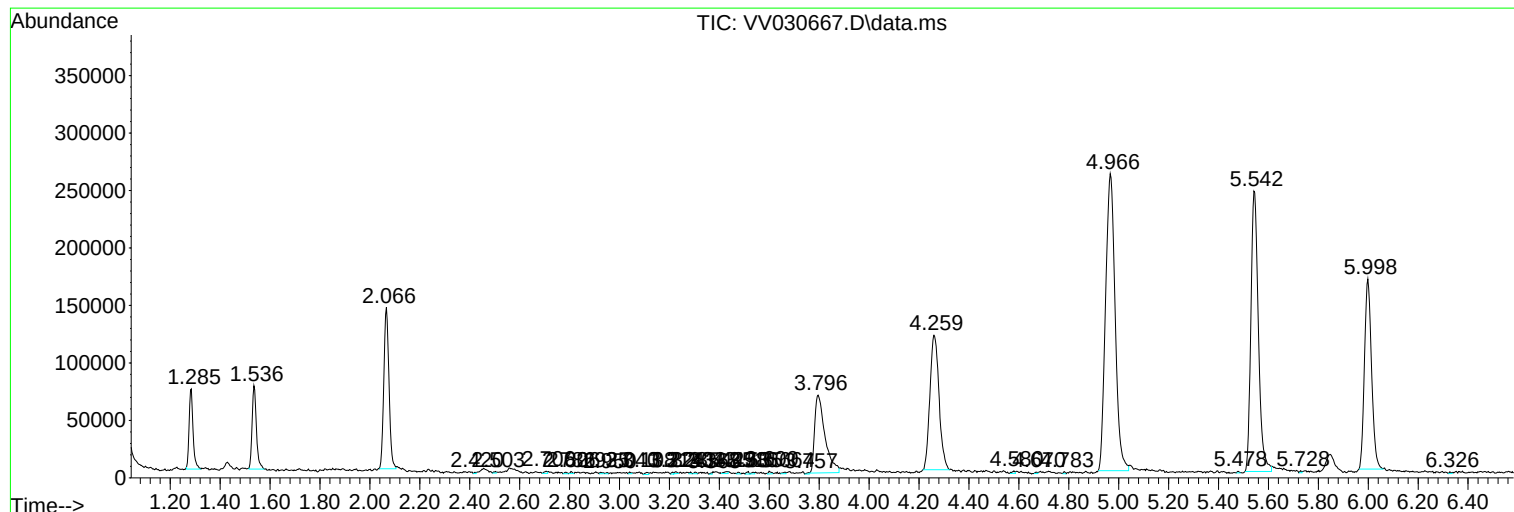

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030667.D
Acq On : 19 Apr 2023 16:09
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030667.D
Acq On : 19 Apr 2023 16:09
Operator : SY/MD
Sample : VIBLK202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK202

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------