

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030669.D
 Acq On : 19 Apr 2023 16:54
 Operator : SY/MD
 Sample : VIBLK204
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	91	rVB	137565	150509	16.77%	2.199%
2	1.535	148	154	168	rVB	123292	147821	16.47%	2.160%
3	2.066	310	319	334	rVB	241488	347360	38.70%	5.075%
4	2.224	365	368	370	rBV4	2164	1049	0.12%	0.015%
5	2.381	415	417	420	rBV4	1176	732	0.08%	0.011%
6	2.519	457	460	465	rVB6	1202	1071	0.12%	0.016%
7	2.580	476	479	482	rBV5	2172	1596	0.18%	0.023%
8	2.635	494	496	498	rVB2	1747	547	0.06%	0.008%
9	2.648	498	500	501	rBV2	1525	591	0.07%	0.009%
10	2.709	517	519	521	rBV3	1741	1023	0.11%	0.015%
11	2.786	540	543	544	rBV3	1454	807	0.09%	0.012%
12	2.841	555	560	562	rBV5	2459	1564	0.17%	0.023%
13	3.008	610	612	616	rVB5	1211	626	0.07%	0.009%
14	3.111	640	644	646	rBV5	1563	1273	0.14%	0.019%
15	3.124	646	648	650	rVB2	1416	724	0.08%	0.011%
16	3.137	650	652	654	rVB3	1645	869	0.10%	0.013%
17	3.153	654	657	659	rBV4	1608	1059	0.12%	0.015%
18	3.201	671	672	676	rVB4	1671	961	0.11%	0.014%
19	3.297	697	702	703	rBV4	1982	1726	0.19%	0.025%
20	3.365	719	723	727	rVB6	1512	1357	0.15%	0.020%
21	3.490	758	762	766	rVB5	1335	983	0.11%	0.014%
22	3.510	766	768	771	rBV3	1143	626	0.07%	0.009%
23	3.719	830	833	836	rBV5	1531	1190	0.13%	0.017%
24	3.744	840	841	844	rBV3	1497	834	0.09%	0.012%
25	3.799	849	858	888	rBV	50893	153165	17.06%	2.238%
26	4.111	952	955	957	rBV4	1464	750	0.08%	0.011%
27	4.259	988	1001	1024	rVB	144195	362781	40.42%	5.300%
28	4.748	1151	1153	1158	rVB6	2054	1368	0.15%	0.020%
29	4.770	1158	1160	1163	rBV4	882	643	0.07%	0.009%
30	4.850	1183	1185	1186	rBV2	2158	1027	0.11%	0.015%
31	4.966	1205	1221	1248	rBV2	336367	897611	100.00%	13.113%
32	5.542	1388	1400	1427	rBV	260369	551043	61.39%	8.050%
33	5.998	1530	1542	1558	rVV	198516	407061	45.35%	5.947%
34	6.301	1633	1636	1640	rBV6	2189	1287	0.14%	0.019%
35	6.381	1659	1661	1666	rBV4	1542	1117	0.12%	0.016%
36	6.448	1680	1682	1684	rBV2	1057	552	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030669.D
 Acq On : 19 Apr 2023 16:54
 Operator : SY/MD
 Sample : VIBLK204
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.590	1724	1726	1728	rBV3	1289	582	0.06%	0.009%
38	6.645	1741	1743	1750	rVB8	2108	1390	0.15%	0.020%
39	6.674	1750	1752	1755	rBV3	1620	934	0.10%	0.014%
40	6.831	1796	1801	1808	rBV10	2132	2808	0.31%	0.041%
41	6.921	1816	1829	1850	rBV2	102259	203923	22.72%	2.979%
42	7.252	1920	1932	1952	rBV	385202	686092	76.44%	10.023%
43	7.506	2009	2011	2015	rVB4	1609	928	0.10%	0.014%
44	7.561	2015	2028	2047	rBV	72826	141857	15.80%	2.072%
45	7.741	2082	2084	2090	rBV6	1490	1131	0.13%	0.017%
46	7.924	2139	2141	2144	rVB4	1390	758	0.08%	0.011%
47	8.034	2166	2175	2207	rBV	174600	348077	38.78%	5.085%
48	8.484	2313	2315	2318	rBV4	1156	838	0.09%	0.012%
49	8.593	2346	2349	2351	rBV4	1243	625	0.07%	0.009%
50	8.792	2400	2411	2435	rVV	400827	691992	77.09%	10.109%
51	9.127	2513	2515	2520	rBV6	1611	902	0.10%	0.013%
52	9.275	2559	2561	2563	rBV3	1454	544	0.06%	0.008%
53	9.320	2572	2575	2582	rVB6	2052	2267	0.25%	0.033%
54	9.349	2582	2584	2585	rBV2	1358	639	0.07%	0.009%
55	9.477	2622	2624	2626	rBV4	1170	709	0.08%	0.010%
56	9.673	2683	2685	2688	rBV4	1105	867	0.10%	0.013%
57	9.834	2731	2735	2737	rBV5	1288	1121	0.12%	0.016%
58	9.979	2777	2780	2781	rBV3	1877	825	0.09%	0.012%
59	10.159	2825	2836	2851	rBV	261566	412532	45.96%	6.027%
60	10.387	2901	2907	2908	rBV5	1390	1245	0.14%	0.018%
61	10.593	2968	2971	2972	rBV3	1619	861	0.10%	0.013%
62	10.625	2979	2981	2984	rBV4	1593	933	0.10%	0.014%
63	10.654	2987	2990	2991	rBV3	1482	871	0.10%	0.013%
64	10.741	3016	3017	3021	rVB4	899	559	0.06%	0.008%
65	10.873	3056	3058	3061	rBV3	1756	928	0.10%	0.014%
66	10.937	3074	3078	3081	rBV6	1347	1177	0.13%	0.017%
67	11.030	3104	3107	3108	rBV3	1089	580	0.06%	0.008%
68	11.130	3134	3138	3142	rBV6	2324	2144	0.24%	0.031%
69	11.194	3144	3158	3178	rBV	381361	627202	69.87%	9.163%
70	11.570	3263	3275	3292	rVV	386101	628879	70.06%	9.187%
71	11.725	3320	3323	3325	rBV4	1404	747	0.08%	0.011%
72	11.738	3325	3327	3329	rBV3	1178	752	0.08%	0.011%
73	11.866	3364	3367	3368	rBV3	1245	652	0.07%	0.010%
74	11.876	3368	3370	3372	rVV3	1547	812	0.09%	0.012%
75	11.905	3376	3379	3381	rBV5	1053	654	0.07%	0.010%
76	12.004	3406	3410	3412	rBV5	1373	850	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030669.D
 Acq On : 19 Apr 2023 16:54
 Operator : SY/MD
 Sample : VIBLK204
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.069	3428	3430	3435	rVB7	1667	1251	0.14%	0.018%
78	12.136	3449	3451	3453	rBV3	1307	650	0.07%	0.009%
79	12.329	3508	3511	3512	rBV3	1007	735	0.08%	0.011%
80	12.583	3587	3590	3592	rBV4	1416	648	0.07%	0.009%
81	12.619	3598	3601	3609	rVB9	1201	1266	0.14%	0.018%
82	12.709	3625	3629	3631	rVB5	1375	945	0.11%	0.014%
83	12.722	3631	3633	3637	rBV3	933	668	0.07%	0.010%
84	12.857	3673	3675	3678	rBV4	1351	837	0.09%	0.012%
85	12.885	3681	3684	3687	rBV4	1761	1093	0.12%	0.016%
86	13.021	3719	3726	3731	rBV4	2647	3482	0.39%	0.051%
87	13.043	3731	3733	3736	rVB4	1987	1023	0.11%	0.015%
88	13.062	3736	3739	3740	rBV3	1997	983	0.11%	0.014%
89	13.165	3769	3771	3774	rBV4	1360	763	0.09%	0.011%
90	13.307	3810	3815	3820	rBV8	2261	2427	0.27%	0.035%
91	13.368	3831	3834	3837	rBV4	1845	1165	0.13%	0.017%
92	13.583	3900	3901	3903	rBV2	1807	935	0.10%	0.014%
93	13.779	3961	3962	3964	rBV2	1029	568	0.06%	0.008%
94	13.805	3968	3970	3974	rVV5	1219	958	0.11%	0.014%
95	13.853	3983	3985	3988	rVB3	1440	626	0.07%	0.009%
96	14.101	4060	4062	4065	rBV4	1458	976	0.11%	0.014%
97	14.146	4074	4076	4078	rBV3	1903	960	0.11%	0.014%
98	14.159	4078	4080	4085	rVB5	1964	1414	0.16%	0.021%
99	14.345	4135	4138	4141	rBV5	2422	1663	0.19%	0.024%
100	15.020	4344	4348	4350	rBV4	1819	1596	0.18%	0.023%

Sum of corrected areas: 6845122




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030669.D
Acq On : 19 Apr 2023 16:54
Operator : SY/MD
Sample : VIBLK204
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

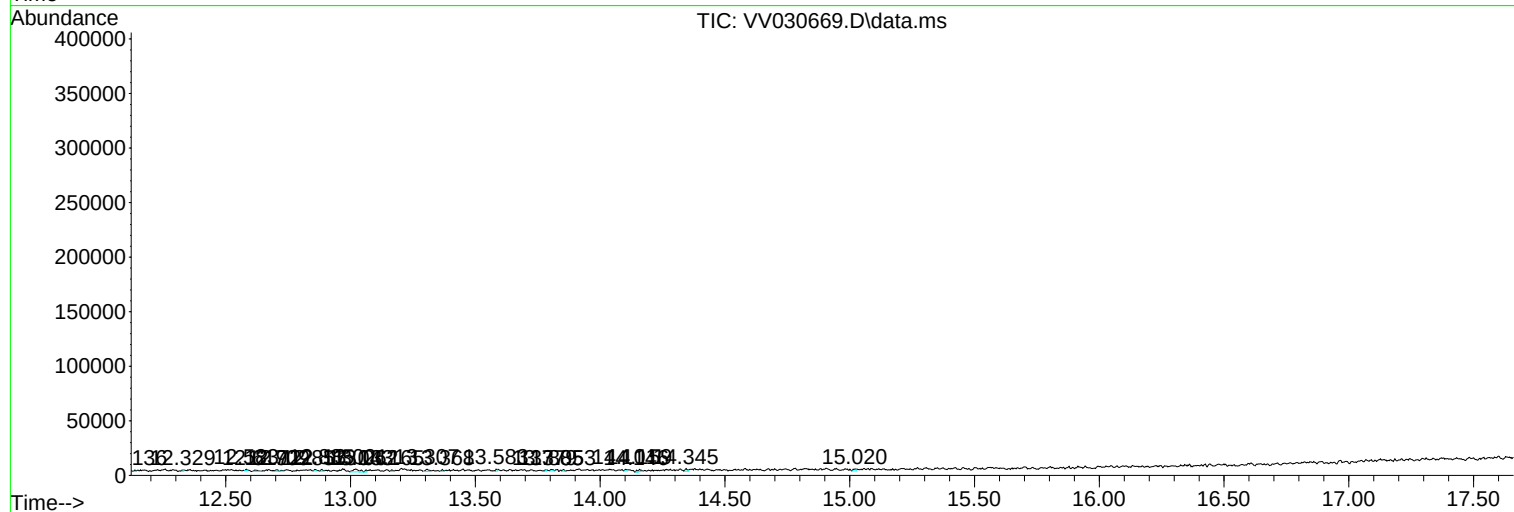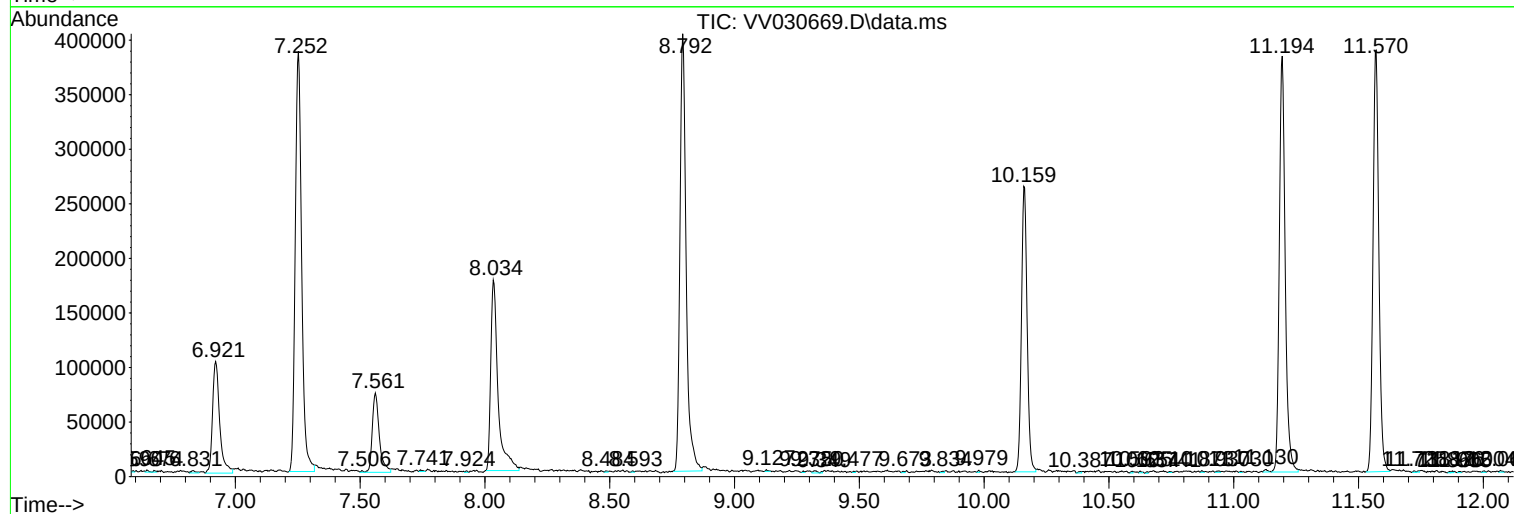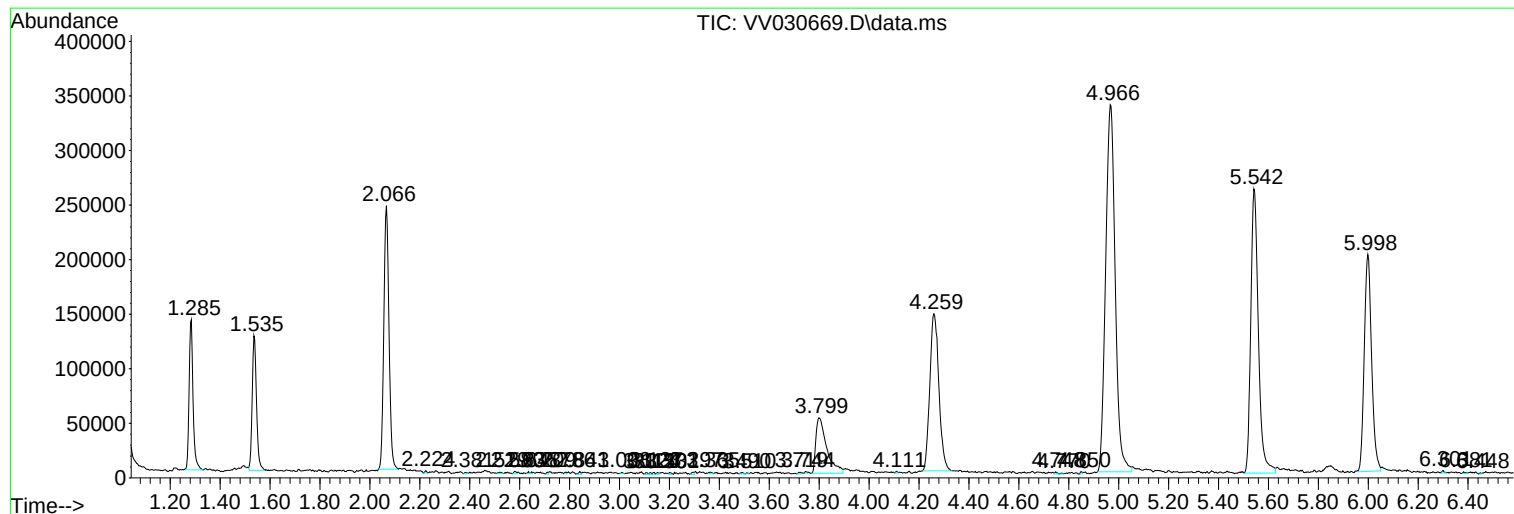

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030669.D
Acq On : 19 Apr 2023 16:54
Operator : SY/MD
Sample : VIBLK204
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030669.D
Acq On : 19 Apr 2023 16:54
Operator : SY/MD
Sample : VIBLK204
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK204

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------