

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030670.D
 Acq On : 19 Apr 2023 17:18
 Operator : SY/MD
 Sample : 02334-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	94	rVB	77891	87607	11.85%	1.426%
2	1.536	148	154	168	rVB	83705	100098	13.54%	1.630%
3	2.066	310	319	333	rVB	155543	223698	30.26%	3.642%
4	2.217	364	366	368	rBV3	1573	836	0.11%	0.014%
5	2.282	384	386	387	rBV2	1914	764	0.10%	0.012%
6	2.458	439	441	443	rVV3	1675	686	0.09%	0.011%
7	2.529	459	463	465	rBV4	1151	862	0.12%	0.014%
8	2.584	476	480	481	rVB4	1571	1036	0.14%	0.017%
9	2.606	481	487	491	rBV8	2365	2951	0.40%	0.048%
10	3.095	636	639	640	rBV4	1573	805	0.11%	0.013%
11	3.217	672	677	678	rBV4	1417	1283	0.17%	0.021%
12	3.346	710	717	718	rBV8	1565	1587	0.21%	0.026%
13	3.420	738	740	743	rBV4	1108	854	0.12%	0.014%
14	3.436	743	745	746	rBV2	1578	646	0.09%	0.011%
15	3.478	754	758	761	rBV7	2023	1609	0.22%	0.026%
16	3.536	774	776	781	rVB5	1232	1052	0.14%	0.017%
17	3.590	790	793	794	rBV3	1242	631	0.09%	0.010%
18	3.671	814	818	820	rBV4	1266	924	0.12%	0.015%
19	3.799	849	858	883	rBV	52527	150724	20.39%	2.454%
20	4.185	976	978	979	rBV2	1557	712	0.10%	0.012%
21	4.259	986	1001	1024	rBV	121002	312220	42.24%	5.084%
22	4.510	1077	1079	1082	rBV4	1319	939	0.13%	0.015%
23	4.831	1176	1179	1180	rBV3	1402	699	0.09%	0.011%
24	4.966	1204	1221	1232	rBV2	259266	704822	95.34%	11.476%
25	5.375	1345	1348	1350	rBV4	1684	1163	0.16%	0.019%
26	5.542	1388	1400	1421	rBV	258073	535026	72.37%	8.712%
27	5.995	1530	1541	1560	rBV	162926	332869	45.03%	5.420%
28	6.172	1593	1596	1599	rBV4	1468	1047	0.14%	0.017%
29	6.272	1625	1627	1629	rBV3	1520	705	0.10%	0.011%
30	6.346	1647	1650	1652	rBV3	1454	1011	0.14%	0.016%
31	6.481	1690	1692	1695	rBV4	1637	813	0.11%	0.013%
32	6.564	1714	1718	1720	rBV5	2047	1680	0.23%	0.027%
33	6.629	1733	1738	1739	rBV5	2050	1583	0.21%	0.026%
34	6.664	1746	1749	1751	rBV4	1482	798	0.11%	0.013%
35	6.696	1756	1759	1761	rBV5	1593	1204	0.16%	0.020%
36	6.815	1795	1796	1800	rBV4	1023	674	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030670.D
 Acq On : 19 Apr 2023 17:18
 Operator : SY/MD
 Sample : 02334-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.851	1804	1807	1808	rBV3	1731	953	0.13%	0.016%
38	6.921	1818	1829	1846	rBV	80708	154965	20.96%	2.523%
39	7.207	1914	1918	1919	rBV4	1368	865	0.12%	0.014%
40	7.252	1919	1932	1948	rBV	282929	506112	68.46%	8.241%
41	7.484	2002	2004	2009	rBV6	1715	1290	0.17%	0.021%
42	7.561	2019	2028	2042	rBV	55748	101690	13.76%	1.656%
43	7.879	2125	2127	2130	rBV4	1828	1139	0.15%	0.019%
44	7.947	2145	2148	2150	rBV4	1524	1150	0.16%	0.019%
45	7.976	2155	2157	2162	rVB6	1587	632	0.09%	0.010%
46	8.034	2165	2175	2205	rBV	171645	345008	46.67%	5.618%
47	8.449	2302	2304	2306	rBV3	1418	837	0.11%	0.014%
48	8.651	2365	2367	2370	rBV4	1371	985	0.13%	0.016%
49	8.793	2400	2411	2418	rBV	404488	721568	97.61%	11.749%
50	9.095	2501	2505	2506	rBV4	2235	1376	0.19%	0.022%
51	9.323	2573	2576	2578	rBV4	1816	1040	0.14%	0.017%
52	9.477	2621	2624	2626	rBV4	1212	888	0.12%	0.014%
53	9.532	2639	2641	2643	rBV3	1417	791	0.11%	0.013%
54	9.584	2654	2657	2660	rBV5	1874	1529	0.21%	0.025%
55	9.661	2674	2681	2682	rBV6	1666	1546	0.21%	0.025%
56	9.699	2690	2693	2695	rBV5	1343	1000	0.14%	0.016%
57	9.976	2777	2779	2782	rBV3	1264	761	0.10%	0.012%
58	10.050	2799	2802	2807	rBV7	1668	1219	0.16%	0.020%
59	10.159	2826	2836	2856	rVB	235395	382881	51.79%	6.234%
60	10.307	2878	2882	2884	rBV5	2430	1785	0.24%	0.029%
61	10.416	2913	2916	2918	rBV3	2398	1630	0.22%	0.027%
62	10.513	2943	2946	2947	rBV2	1334	683	0.09%	0.011%
63	10.567	2959	2963	2967	rBV7	993	830	0.11%	0.014%
64	10.609	2974	2976	2978	rBV3	1242	586	0.08%	0.010%
65	10.796	3030	3034	3035	rBV4	1398	959	0.13%	0.016%
66	10.956	3079	3084	3086	rBV4	1082	972	0.13%	0.016%
67	11.008	3097	3100	3101	rBV3	1116	716	0.10%	0.012%
68	11.088	3122	3125	3126	rBV3	1621	1166	0.16%	0.019%
69	11.194	3147	3158	3177	rBV2	383420	739244	100.00%	12.037%
70	11.571	3263	3275	3292	rBV2	349427	638647	86.39%	10.399%
71	11.809	3347	3349	3351	rBV3	1276	757	0.10%	0.012%
72	11.857	3361	3364	3366	rBV4	1721	1081	0.15%	0.018%
73	11.927	3384	3386	3388	rBV3	1241	594	0.08%	0.010%
74	11.995	3404	3407	3409	rBV4	2021	1389	0.19%	0.023%
75	12.130	3446	3449	3450	rBV2	1468	769	0.10%	0.013%
76	12.178	3462	3464	3468	rBV5	1441	966	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030670.D
 Acq On : 19 Apr 2023 17:18
 Operator : SY/MD
 Sample : 02334-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.246	3482	3485	3487	rBV3	1249	947	0.13%	0.015%
78	12.313	3504	3506	3508	rBV3	1532	923	0.12%	0.015%
79	12.448	3546	3548	3551	rBV4	1706	1260	0.17%	0.021%
80	12.484	3557	3559	3562	rBV3	1398	1087	0.15%	0.018%
81	12.564	3581	3584	3589	rBV6	1997	1538	0.21%	0.025%
82	12.693	3619	3624	3627	rBV7	1552	1336	0.18%	0.022%
83	12.873	3678	3680	3686	rBV6	1260	1319	0.18%	0.021%
84	12.944	3697	3702	3704	rBV5	2017	1508	0.20%	0.025%
85	13.104	3748	3752	3753	rBV4	1213	723	0.10%	0.012%
86	13.114	3753	3755	3758	rVB4	1651	781	0.11%	0.013%
87	13.140	3761	3763	3766	rBV4	1261	898	0.12%	0.015%
88	13.214	3776	3786	3794	rBV9	8060	15341	2.08%	0.250%
89	13.297	3810	3812	3816	rVB5	1545	796	0.11%	0.013%
90	13.313	3816	3817	3820	rBV2	1721	1154	0.16%	0.019%
91	13.410	3845	3847	3848	rBV2	1773	891	0.12%	0.015%
92	13.474	3864	3867	3870	rVB5	1774	974	0.13%	0.016%
93	13.525	3881	3883	3885	rBV3	1317	644	0.09%	0.010%
94	13.725	3940	3945	3947	rBV6	2665	2105	0.28%	0.034%
95	13.747	3949	3952	3959	rVV6	1806	2024	0.27%	0.033%
96	13.818	3972	3974	3979	rVB6	1317	910	0.12%	0.015%
97	13.844	3979	3982	3985	rBV5	2190	1527	0.21%	0.025%
98	13.886	3993	3995	3997	rBV3	1294	650	0.09%	0.011%
99	14.005	4030	4032	4038	rVB7	1708	929	0.13%	0.015%
100	14.583	4209	4212	4216	rBV6	1614	1586	0.21%	0.026%




Sum of corrected areas: 6141468

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030670.D
Acq On : 19 Apr 2023 17:18
Operator : SY/MD
Sample : 02334-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

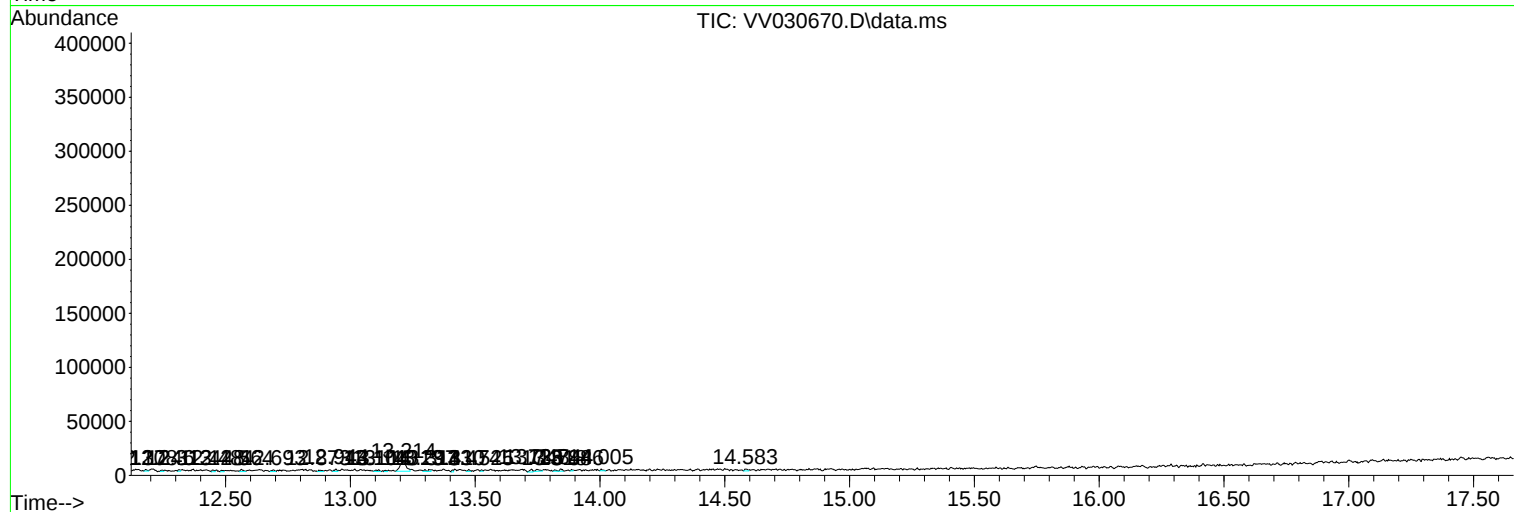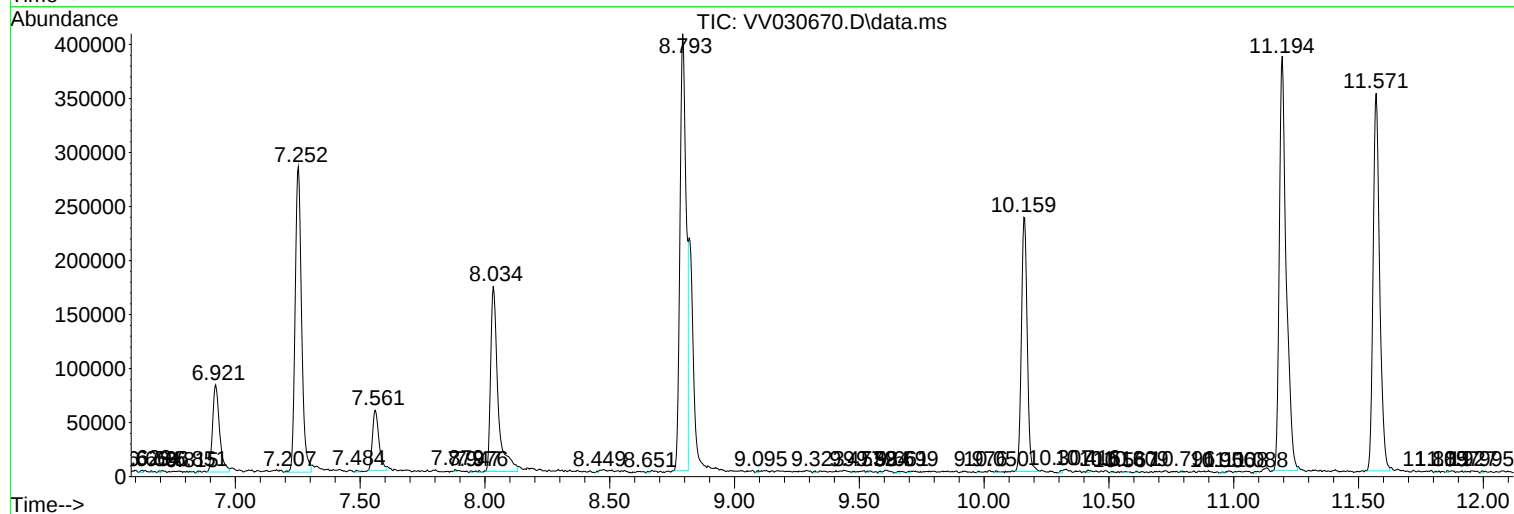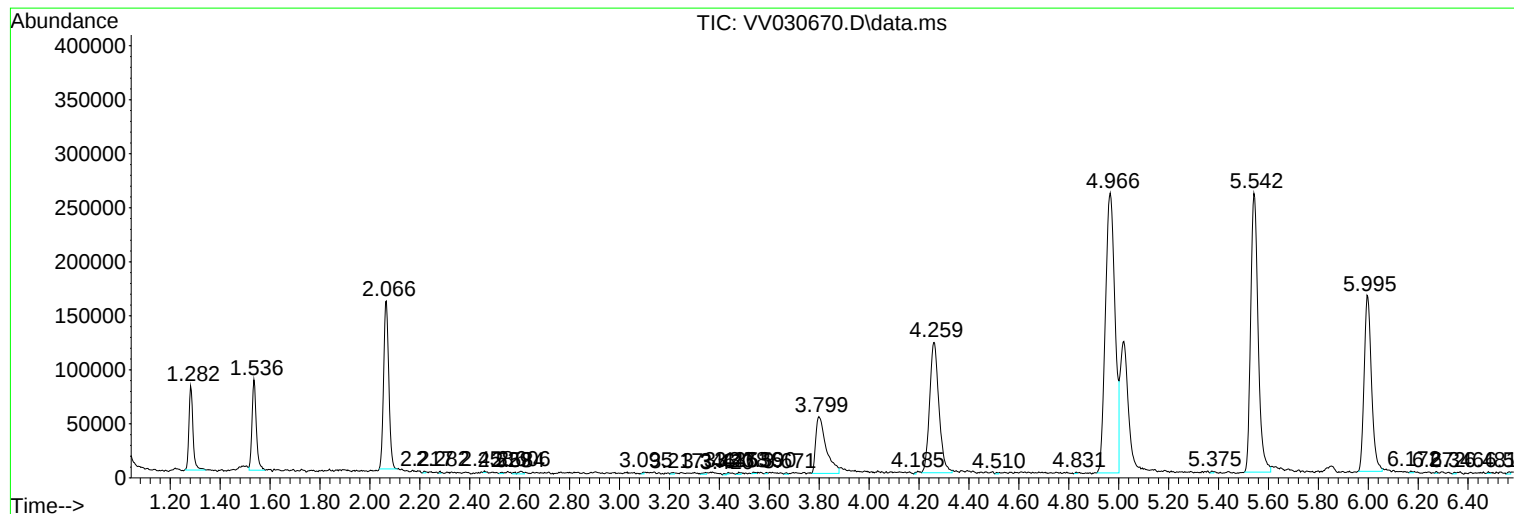

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030670.D
Acq On : 19 Apr 2023 17:18
Operator : SY/MD
Sample : 02334-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030670.D
Acq On : 19 Apr 2023 17:18
Operator : SY/MD
Sample : 02334-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------