

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030671.D
 Acq On : 19 Apr 2023 17:42
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rBV	132530	150661	16.30%	2.159%
2	1.539	148	155	167	rVB	125890	150899	16.33%	2.163%
3	2.066	310	319	332	rBV	242251	349190	37.78%	5.005%
4	2.159	345	348	350	rBV4	2452	1551	0.17%	0.022%
5	2.330	399	401	406	rVB5	1787	1533	0.17%	0.022%
6	2.384	414	418	421	rBV5	1413	1222	0.13%	0.018%
7	2.529	461	463	466	rBV4	1763	929	0.10%	0.013%
8	2.587	477	481	482	rBV4	1210	913	0.10%	0.013%
9	2.597	482	484	486	rVB3	1961	722	0.08%	0.010%
10	3.088	635	637	639	rVB3	1489	648	0.07%	0.009%
11	3.108	639	643	646	rBV5	1599	1279	0.14%	0.018%
12	3.185	664	667	671	rVB6	1155	761	0.08%	0.011%
13	3.288	694	699	702	rBV6	2524	2477	0.27%	0.035%
14	3.336	712	714	718	rBV5	1181	716	0.08%	0.010%
15	3.471	752	756	757	rBV3	1830	1238	0.13%	0.018%
16	3.568	784	786	788	rBV3	1514	800	0.09%	0.011%
17	3.609	797	799	803	rBV4	1290	648	0.07%	0.009%
18	3.667	814	817	818	rBV4	1967	927	0.10%	0.013%
19	3.735	834	838	842	rBV7	1285	1276	0.14%	0.018%
20	3.805	850	860	882	rBV	51867	150700	16.30%	2.160%
21	4.259	986	1001	1022	rBV	146540	371975	40.24%	5.331%
22	4.703	1137	1139	1140	rBV2	1680	724	0.08%	0.010%
23	4.966	1204	1221	1256	rBV2	342870	924321	100.00%	13.247%
24	5.397	1353	1355	1357	rBV3	1341	779	0.08%	0.011%
25	5.542	1388	1400	1420	rBV	270824	562736	60.88%	8.065%
26	5.998	1531	1542	1560	rBV	203174	399606	43.23%	5.727%
27	6.374	1657	1659	1662	rVB4	1751	798	0.09%	0.011%
28	6.448	1677	1682	1685	rBV6	1987	1648	0.18%	0.024%
29	6.493	1694	1696	1701	rVB6	1317	751	0.08%	0.011%
30	6.542	1709	1711	1715	rVB5	1773	1088	0.12%	0.016%
31	6.664	1746	1749	1750	rBV3	1868	1181	0.13%	0.017%
32	6.696	1757	1759	1763	rBV4	1440	799	0.09%	0.011%
33	6.738	1766	1772	1773	rBV5	2317	1929	0.21%	0.028%
34	6.918	1818	1828	1843	rBV	103954	196512	21.26%	2.816%
35	7.252	1920	1932	1953	rBV	391118	694938	75.18%	9.960%
36	7.561	2014	2028	2040	rBV	76791	139570	15.10%	2.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030671.D
 Acq On : 19 Apr 2023 17:42
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.825	2107	2110	2113	rBV4	2195	1267	0.14%	0.018%
38	7.873	2123	2125	2128	rBV4	1902	1387	0.15%	0.020%
39	7.979	2155	2158	2159	rBV3	1242	674	0.07%	0.010%
40	8.034	2164	2175	2207	rBV	179995	374165	40.48%	5.362%
41	8.275	2248	2250	2255	rVB5	1620	1030	0.11%	0.015%
42	8.484	2313	2315	2317	rBV3	1648	877	0.09%	0.013%
43	8.506	2320	2322	2327	rVB5	1851	1053	0.11%	0.015%
44	8.609	2352	2354	2356	rBV4	1564	773	0.08%	0.011%
45	8.792	2400	2411	2437	rBV	403863	712461	77.08%	10.211%
46	9.133	2515	2517	2521	rVB6	1498	1096	0.12%	0.016%
47	9.165	2521	2527	2529	rBV7	2086	1811	0.20%	0.026%
48	9.194	2532	2536	2540	rBV7	1121	970	0.10%	0.014%
49	9.243	2550	2551	2555	rBV4	1399	645	0.07%	0.009%
50	9.323	2573	2576	2578	rBV4	1621	957	0.10%	0.014%
51	9.603	2660	2663	2665	rBV5	1012	768	0.08%	0.011%
52	9.651	2676	2678	2681	rBV3	1696	1100	0.12%	0.016%
53	9.825	2730	2732	2736	rVB5	1620	1194	0.13%	0.017%
54	9.873	2744	2747	2748	rBV3	1811	830	0.09%	0.012%
55	9.934	2764	2766	2769	rVB2	1596	789	0.09%	0.011%
56	9.956	2771	2773	2777	rVV5	1848	1171	0.13%	0.017%
57	9.988	2781	2783	2788	rVB5	1555	1108	0.12%	0.016%
58	10.046	2798	2801	2803	rBV3	1260	972	0.11%	0.014%
59	10.159	2825	2836	2852	rBV	259902	419566	45.39%	6.013%
60	10.281	2872	2874	2876	rBV2	1697	988	0.11%	0.014%
61	10.333	2885	2890	2893	rVB6	2142	1957	0.21%	0.028%
62	10.365	2896	2900	2902	rBV5	1105	762	0.08%	0.011%
63	10.397	2909	2910	2914	rBV4	1171	731	0.08%	0.010%
64	10.442	2922	2924	2928	rBV5	1224	893	0.10%	0.013%
65	10.754	3018	3021	3022	rBV3	1775	865	0.09%	0.012%
66	10.889	3061	3063	3065	rBV3	1915	867	0.09%	0.012%
67	10.921	3071	3073	3078	rVB6	1456	910	0.10%	0.013%
68	10.960	3082	3085	3088	rBV3	2223	1451	0.16%	0.021%
69	11.043	3110	3111	3114	rBV3	1131	776	0.08%	0.011%
70	11.101	3125	3129	3132	rBV7	2033	1655	0.18%	0.024%
71	11.194	3147	3158	3178	rBV	395319	646644	69.96%	9.268%
72	11.426	3228	3230	3235	rVB4	1430	1084	0.12%	0.016%
73	11.448	3235	3237	3239	rBV3	1816	1141	0.12%	0.016%
74	11.506	3253	3255	3258	rVB4	1650	763	0.08%	0.011%
75	11.567	3264	3274	3294	rVB	391152	645116	69.79%	9.246%
76	11.770	3333	3337	3338	rBV3	1099	650	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030671.D
 Acq On : 19 Apr 2023 17:42
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.828	3352	3355	3359	rBV5	1608	1049	0.11%	0.015%
78	11.892	3372	3375	3379	rBV6	1694	869	0.09%	0.012%
79	11.937	3387	3389	3394	rBV6	1399	1454	0.16%	0.021%
80	12.111	3440	3443	3445	rBV4	1188	820	0.09%	0.012%
81	12.213	3473	3475	3478	rVB4	1390	794	0.09%	0.011%
82	12.233	3478	3481	3484	rBV5	1603	1307	0.14%	0.019%
83	12.464	3551	3553	3555	rBV3	1162	786	0.09%	0.011%
84	12.580	3587	3589	3593	rBV5	1279	1039	0.11%	0.015%
85	12.619	3599	3601	3604	rVB3	1509	726	0.08%	0.010%
86	12.676	3616	3619	3621	rBV3	1235	957	0.10%	0.014%
87	12.953	3701	3705	3706	rBV3	1367	968	0.10%	0.014%
88	13.078	3740	3744	3745	rBV4	1169	713	0.08%	0.010%
89	13.149	3763	3766	3769	rBV5	1117	710	0.08%	0.010%
90	13.168	3769	3772	3774	rBV4	1410	782	0.08%	0.011%
91	13.207	3779	3784	3788	rBV7	2093	2438	0.26%	0.035%
92	13.271	3799	3804	3807	rBV5	1222	1092	0.12%	0.016%
93	13.406	3843	3846	3847	rBV3	1572	819	0.09%	0.012%
94	13.683	3930	3932	3935	rVV3	1891	1161	0.13%	0.017%
95	13.779	3960	3962	3964	rBV3	1343	651	0.07%	0.009%
96	14.229	4101	4102	4105	rBV3	1461	691	0.07%	0.010%
97	14.368	4143	4145	4149	rBV5	1658	1363	0.15%	0.020%
98	14.522	4190	4193	4194	rBV2	1359	768	0.08%	0.011%
99	14.850	4292	4295	4300	rBV6	1745	1885	0.20%	0.027%
100	15.188	4398	4400	4405	rBV4	1755	1296	0.14%	0.019%




Sum of corrected areas: 6977500

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030671.D
Acq On : 19 Apr 2023 17:42
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

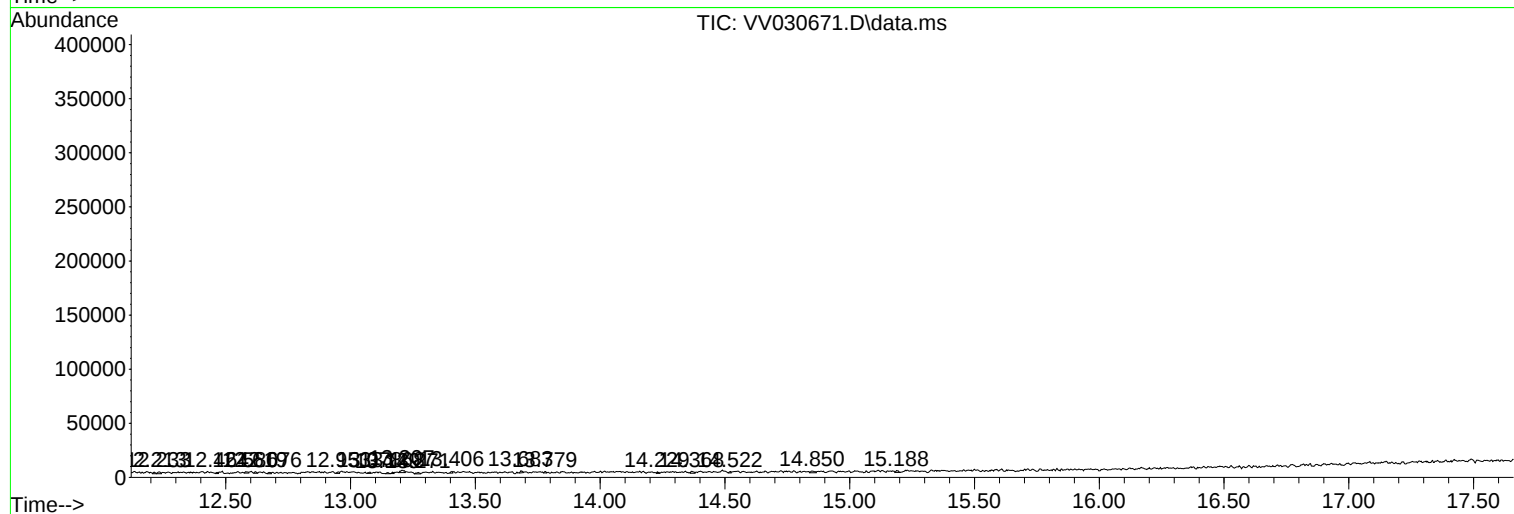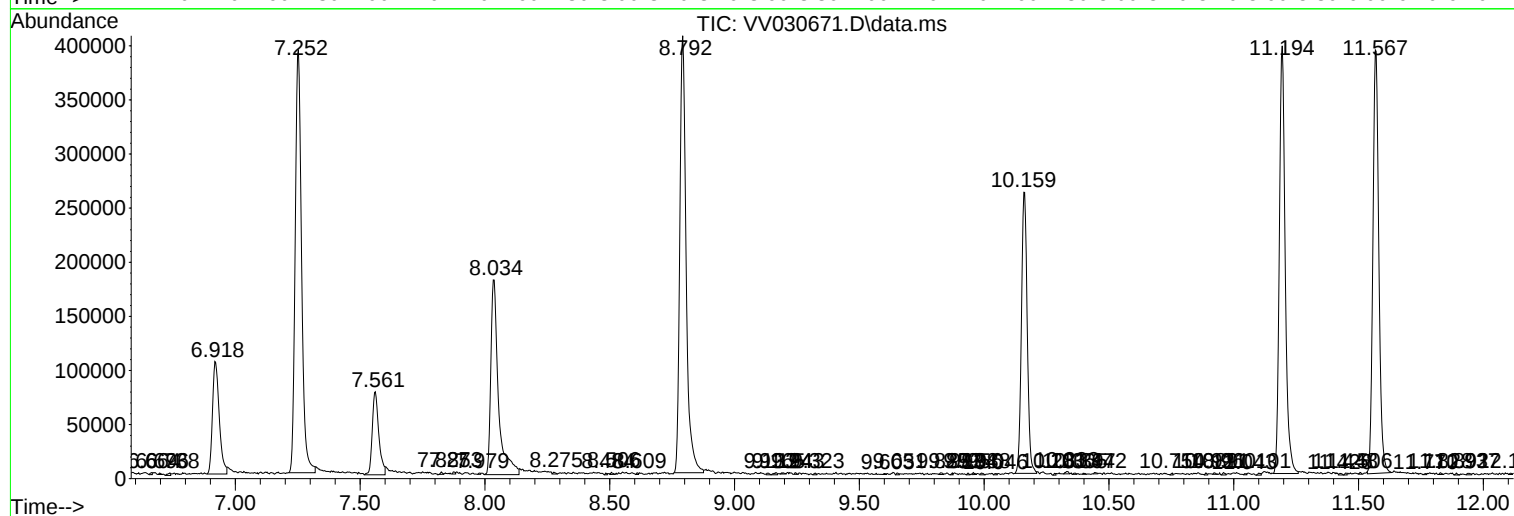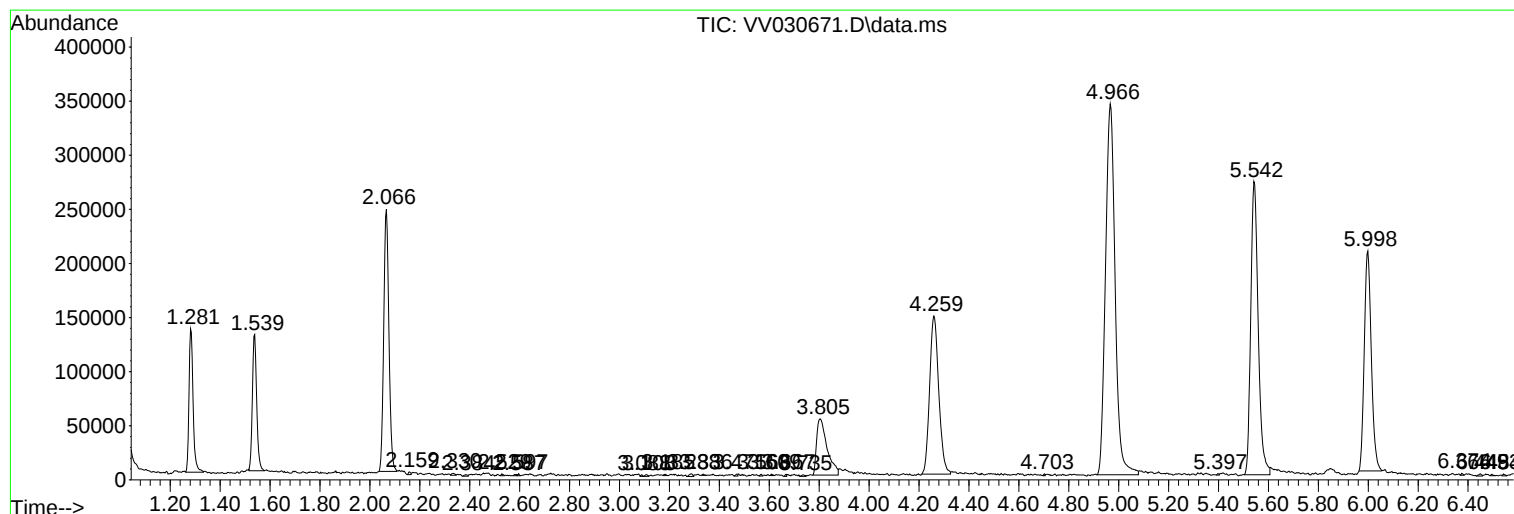

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030671.D
Acq On : 19 Apr 2023 17:42
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030671.D
Acq On : 19 Apr 2023 17:42
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------