

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030672.D
 Acq On : 19 Apr 2023 18:06
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	83	rBV	78870	81708	11.08%	1.326%
2	1.539	148	155	165	rBV	84051	96249	13.05%	1.561%
3	2.066	310	319	332	rBV	166292	241956	32.80%	3.925%
4	2.423	427	430	433	rBV5	1846	1324	0.18%	0.021%
5	2.503	452	455	462	rVB8	2535	2660	0.36%	0.043%
6	2.680	507	510	513	rVB5	1639	801	0.11%	0.013%
7	2.764	533	536	539	rBV5	1453	1169	0.16%	0.019%
8	2.854	561	564	567	rVB5	1422	809	0.11%	0.013%
9	2.873	567	570	571	rBV3	1386	897	0.12%	0.015%
10	2.918	582	584	587	rBV4	1599	1100	0.15%	0.018%
11	2.982	602	604	609	rBV6	1312	1104	0.15%	0.018%
12	3.056	623	627	630	rVB6	1410	1108	0.15%	0.018%
13	3.079	630	634	637	rBV6	1677	1607	0.22%	0.026%
14	3.108	641	643	646	rVB2	1551	774	0.10%	0.013%
15	3.124	646	648	652	rBV4	1803	979	0.13%	0.016%
16	3.143	652	654	659	rVB6	1220	905	0.12%	0.015%
17	3.236	680	683	686	rBV5	1684	1140	0.15%	0.018%
18	3.313	705	707	709	rBV3	1595	884	0.12%	0.014%
19	3.368	722	724	730	rVB7	1449	1055	0.14%	0.017%
20	3.500	764	765	769	rVB5	1934	1065	0.14%	0.017%
21	3.809	851	861	881	rBV	50233	149640	20.29%	2.428%
22	4.259	990	1001	1026	rVB	125812	321326	43.56%	5.213%
23	4.590	1099	1104	1111	rBV10	1892	2619	0.36%	0.042%
24	4.683	1131	1133	1138	rBV5	1523	1040	0.14%	0.017%
25	4.850	1181	1185	1190	rBV7	1019	818	0.11%	0.013%
26	4.882	1190	1195	1196	rBV5	1398	801	0.11%	0.013%
27	4.966	1206	1221	1244	rBV2	274703	737585	100.00%	11.966%
28	5.381	1347	1350	1351	rBV3	1614	859	0.12%	0.014%
29	5.542	1388	1400	1422	rBV	267495	555537	75.32%	9.012%
30	5.998	1531	1542	1566	rVB2	173131	353642	47.95%	5.737%
31	6.262	1621	1624	1627	rBV4	1451	1132	0.15%	0.018%
32	6.307	1634	1638	1645	rVB9	1968	1986	0.27%	0.032%
33	6.342	1646	1649	1651	rBV3	1652	819	0.11%	0.013%
34	6.519	1701	1704	1708	rBV6	1179	1005	0.14%	0.016%
35	6.599	1725	1729	1732	rBV5	1353	1440	0.20%	0.023%
36	6.709	1761	1763	1766	rVB4	1909	1155	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041923\
 Data File : VW030672.D
 Acq On : 19 Apr 2023 18:06
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.741	1770	1773	1775	rBV4	1664	853	0.12%	0.014%
38	6.799	1786	1791	1793	rBV5	1496	1273	0.17%	0.021%
39	6.828	1796	1800	1802	rVB5	1260	838	0.11%	0.014%
40	6.921	1816	1829	1847	rBV	87509	167703	22.74%	2.721%
41	7.252	1921	1932	1950	rBV	303731	537504	72.87%	8.720%
42	7.561	2020	2028	2044	rBV	59950	103231	14.00%	1.675%
43	7.696	2067	2070	2073	rBV4	2215	1564	0.21%	0.025%
44	7.731	2079	2081	2087	rBV8	1153	1103	0.15%	0.018%
45	7.879	2121	2127	2132	rVB9	3016	3942	0.53%	0.064%
46	7.966	2151	2154	2157	rBV5	1506	1153	0.16%	0.019%
47	8.033	2166	2175	2206	rBV	174019	365672	49.58%	5.932%
48	8.622	2353	2358	2360	rBV4	1615	1249	0.17%	0.020%
49	8.680	2375	2376	2381	rVB5	1609	993	0.13%	0.016%
50	8.709	2381	2385	2387	rBV4	1341	1164	0.16%	0.019%
51	8.792	2400	2411	2433	rBV	413839	709857	96.24%	11.516%
52	9.140	2516	2519	2522	rBV4	1674	987	0.13%	0.016%
53	9.442	2612	2613	2616	rVB3	1896	776	0.11%	0.013%
54	9.603	2659	2663	2664	rBV3	1005	782	0.11%	0.013%
55	9.702	2690	2694	2695	rBV4	1759	1144	0.16%	0.019%
56	9.821	2729	2731	2736	rBV6	1318	1092	0.15%	0.018%
57	10.162	2826	2837	2860	rVB	254187	411295	55.76%	6.672%
58	10.275	2868	2872	2873	rBV4	1869	1334	0.18%	0.022%
59	10.320	2883	2886	2887	rBV4	2050	1066	0.14%	0.017%
60	10.406	2909	2913	2915	rBV5	1889	1212	0.16%	0.020%
61	10.474	2931	2934	2936	rBV3	1776	1319	0.18%	0.021%
62	10.603	2971	2974	2978	rVB5	1926	1541	0.21%	0.025%
63	10.683	2995	2999	3004	rBV7	1874	1787	0.24%	0.029%
64	10.718	3004	3010	3012	rBV5	1492	1766	0.24%	0.029%
65	11.059	3112	3116	3119	rBV5	1382	919	0.12%	0.015%
66	11.082	3119	3123	3126	rBV6	856	900	0.12%	0.015%
67	11.111	3130	3132	3134	rBV3	1606	961	0.13%	0.016%
68	11.194	3146	3158	3178	rBV	399715	651754	88.36%	10.573%
69	11.361	3207	3210	3213	rBV5	1401	1049	0.14%	0.017%
70	11.432	3230	3232	3235	rBV4	1498	897	0.12%	0.015%
71	11.570	3264	3275	3292	rVB	355475	573074	77.70%	9.297%
72	11.850	3358	3362	3364	rBV4	2155	1488	0.20%	0.024%
73	11.943	3385	3391	3397	rVB10	1725	2175	0.29%	0.035%
74	11.979	3397	3402	3405	rBV6	1502	1730	0.23%	0.028%
75	12.101	3436	3440	3443	rBV5	974	944	0.13%	0.015%
76	12.210	3471	3474	3476	rBV4	1167	860	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030672.D
 Acq On : 19 Apr 2023 18:06
 Operator : SY/MD
 Sample : 02360-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.271	3487	3493	3494	rBV6	1393	1149	0.16%	0.019%
78	12.419	3535	3539	3540	rBV4	1444	888	0.12%	0.014%
79	12.442	3545	3546	3551	rVB5	1764	1082	0.15%	0.018%
80	12.477	3551	3557	3559	rBV5	2365	2120	0.29%	0.034%
81	12.500	3559	3564	3567	rBV6	1323	1373	0.19%	0.022%
82	12.545	3575	3578	3581	rBV5	2017	1719	0.23%	0.028%
83	12.596	3592	3594	3598	rVB5	2072	1092	0.15%	0.018%
84	12.619	3598	3601	3605	rVB5	1882	1223	0.17%	0.020%
85	12.641	3605	3608	3612	rBV6	1294	1171	0.16%	0.019%
86	12.689	3620	3623	3629	rVB8	1683	1674	0.23%	0.027%
87	12.863	3674	3677	3679	rBV4	1802	1014	0.14%	0.016%
88	12.969	3707	3710	3715	rVB7	1988	1405	0.19%	0.023%
89	13.004	3715	3721	3723	rBV5	2221	2023	0.27%	0.033%
90	13.043	3730	3733	3736	rBV5	1469	1050	0.14%	0.017%
91	13.117	3753	3756	3760	rBV6	1657	1428	0.19%	0.023%
92	13.303	3807	3814	3817	rBV8	2004	2119	0.29%	0.034%
93	13.397	3840	3843	3845	rBV4	1375	784	0.11%	0.013%
94	13.869	3987	3990	3993	rBV5	2052	1543	0.21%	0.025%
95	13.934	4007	4010	4012	rBV4	2080	1529	0.21%	0.025%
96	13.969	4018	4021	4024	rBV4	2286	1711	0.23%	0.028%
97	14.278	4114	4117	4119	rBV4	1351	982	0.13%	0.016%
98	14.461	4170	4174	4178	rVB6	1557	1608	0.22%	0.026%
99	14.509	4187	4189	4193	rBV5	1151	869	0.12%	0.014%
100	14.573	4205	4209	4210	rBV4	1527	1055	0.14%	0.017%




Sum of corrected areas: 6164260

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030672.D
Acq On : 19 Apr 2023 18:06
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

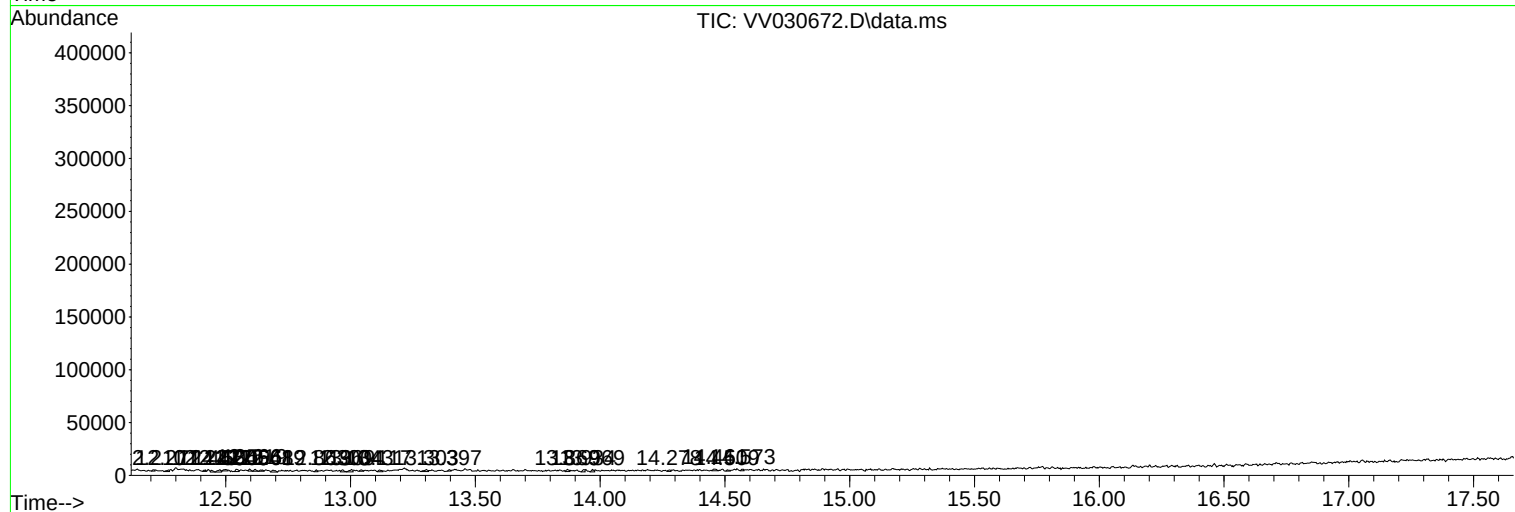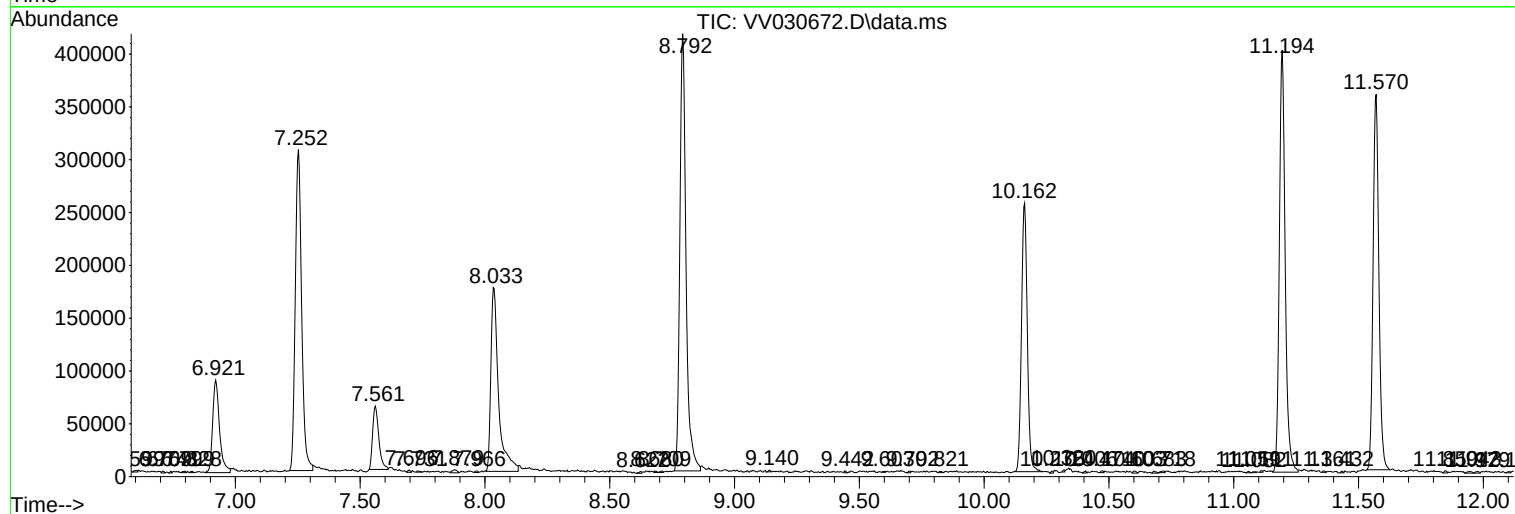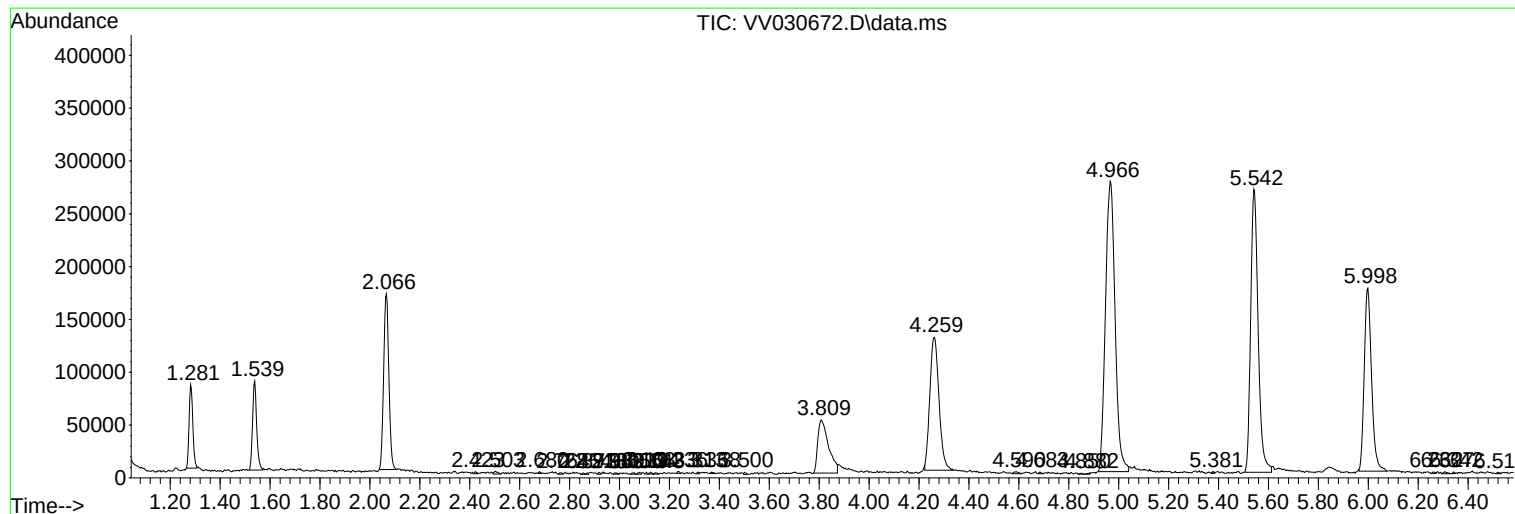

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030672.D
Acq On : 19 Apr 2023 18:06
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030672.D
Acq On : 19 Apr 2023 18:06
Operator : SY/MD
Sample : 02360-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------