

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030674.D
 Acq On : 19 Apr 2023 18:53
 Operator : SY/MD
 Sample : 02334-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	87	rVB	75928	82198	5.05%	1.065%
2	1.535	148	154	166	rVB	84702	99328	6.10%	1.287%
3	2.066	310	319	335	rVB	156253	229839	14.12%	2.978%
4	2.564	471	474	475	rBV3	1737	1034	0.06%	0.013%
5	2.834	555	558	561	rBV5	1675	1311	0.08%	0.017%
6	2.937	586	590	593	rBV4	947	682	0.04%	0.009%
7	2.973	598	601	603	rBV4	1939	1241	0.08%	0.016%
8	3.063	627	629	631	rBV4	1067	521	0.03%	0.007%
9	3.188	665	668	670	rVB4	1368	817	0.05%	0.011%
10	3.201	670	672	674	rVB3	1877	917	0.06%	0.012%
11	3.217	674	677	680	rBV4	2542	1945	0.12%	0.025%
12	3.252	686	688	690	rBV3	835	453	0.03%	0.006%
13	3.281	694	697	699	rBV3	1421	1009	0.06%	0.013%
14	3.387	724	730	732	rBV6	2471	2621	0.16%	0.034%
15	3.429	740	743	744	rBV3	1434	692	0.04%	0.009%
16	3.471	754	756	758	rBV3	1042	689	0.04%	0.009%
17	3.490	759	762	764	rVV4	1536	801	0.05%	0.010%
18	3.564	783	785	787	rBV2	996	461	0.03%	0.006%
19	3.584	787	791	794	rVV5	981	907	0.06%	0.012%
20	3.603	794	797	798	rBV3	1240	598	0.04%	0.008%
21	3.677	817	820	824	rVB6	2266	1761	0.11%	0.023%
22	3.696	824	826	827	rBV2	1217	561	0.03%	0.007%
23	3.802	850	859	878	rBV2	50063	133963	8.23%	1.736%
24	4.127	958	960	962	rBV3	1507	507	0.03%	0.007%
25	4.259	986	1001	1026	rVV	124704	318688	19.58%	4.129%
26	4.651	1122	1123	1126	rVB3	1191	504	0.03%	0.007%
27	4.725	1143	1146	1148	rBV4	1340	827	0.05%	0.011%
28	4.809	1169	1172	1176	rBV6	1739	1405	0.09%	0.018%
29	4.854	1183	1186	1188	rBV5	1561	1206	0.07%	0.016%
30	4.876	1191	1193	1196	rBV4	1286	601	0.04%	0.008%
31	4.966	1205	1221	1260	rBV2	268058	729713	44.83%	9.455%
32	5.542	1386	1400	1425	rBV	265297	558206	34.29%	7.233%
33	5.953	1526	1528	1529	rBV2	1576	656	0.04%	0.009%
34	5.998	1530	1542	1560	rVV	163761	345545	21.23%	4.477%
35	6.384	1660	1662	1666	rBV4	1535	1052	0.06%	0.014%
36	6.548	1711	1713	1716	rBV4	1478	844	0.05%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041923\
 Data File : VW030674.D
 Acq On : 19 Apr 2023 18:53
 Operator : SY/MD
 Sample : 02334-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.731	1768	1770	1771	rBV2	1483	575	0.04%	0.007%
38	6.854	1806	1808	1811	rBV4	1722	1059	0.07%	0.014%
39	6.921	1819	1829	1843	rBV	83779	155146	9.53%	2.010%
40	7.252	1918	1932	1952	rBV	289111	523337	32.15%	6.781%
41	7.561	2019	2028	2046	rBV2	57620	107083	6.58%	1.388%
42	7.844	2112	2116	2118	rBV4	1346	979	0.06%	0.013%
43	7.870	2118	2124	2127	rBV8	2600	3341	0.21%	0.043%
44	7.905	2133	2135	2137	rBV2	1611	976	0.06%	0.013%
45	7.979	2155	2158	2160	rBV3	1087	657	0.04%	0.009%
46	8.034	2166	2175	2206	rBV	164993	337682	20.74%	4.375%
47	8.384	2282	2284	2285	rBV2	1957	768	0.05%	0.010%
48	8.506	2321	2322	2323	rBV	1226	425	0.03%	0.006%
49	8.564	2337	2340	2341	rBV3	1561	1007	0.06%	0.013%
50	8.686	2376	2378	2383	rBV5	1731	1513	0.09%	0.020%
51	8.792	2400	2411	2440	rBV2	411945	874532	53.72%	11.332%
52	9.056	2492	2493	2495	rBV2	1221	474	0.03%	0.006%
53	9.104	2506	2508	2510	rBV3	1379	603	0.04%	0.008%
54	9.149	2518	2522	2524	rBV4	1510	1151	0.07%	0.015%
55	9.339	2579	2581	2586	rBV5	1136	731	0.04%	0.009%
56	9.381	2591	2594	2595	rBV3	1952	987	0.06%	0.013%
57	9.400	2598	2600	2602	rBV3	2124	995	0.06%	0.013%
58	9.542	2642	2644	2646	rBV3	936	431	0.03%	0.006%
59	9.561	2647	2650	2651	rBV3	1566	690	0.04%	0.009%
60	9.648	2674	2677	2678	rBV3	1119	468	0.03%	0.006%
61	9.657	2678	2680	2683	rVB3	1782	819	0.05%	0.011%
62	9.673	2683	2685	2687	rBV3	1753	999	0.06%	0.013%
63	9.824	2729	2732	2734	rBV4	1367	858	0.05%	0.011%
64	10.159	2826	2836	2855	rBV	248104	391378	24.04%	5.071%
65	10.262	2866	2868	2872	rVB5	1788	841	0.05%	0.011%
66	10.535	2951	2953	2955	rBV2	1350	658	0.04%	0.009%
67	10.599	2971	2973	2977	rVB5	1058	627	0.04%	0.008%
68	10.628	2980	2982	2984	rBV3	1157	718	0.04%	0.009%
69	10.664	2990	2993	2994	rBV3	1166	622	0.04%	0.008%
70	10.734	3013	3015	3019	rVB5	1533	661	0.04%	0.009%
71	10.750	3019	3020	3024	rVB4	1083	470	0.03%	0.006%
72	10.786	3024	3031	3034	rVB8	2609	2896	0.18%	0.038%
73	11.127	3123	3137	3147	rBV	147531	238781	14.67%	3.094%
74	11.213	3148	3164	3182	rVB2	672929	1627812	100.00%	21.092%
75	11.512	3251	3257	3259	rBV7	2439	2386	0.15%	0.031%
76	11.567	3264	3274	3291	rVV2	366371	653300	40.13%	8.465%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030674.D
 Acq On : 19 Apr 2023 18:53
 Operator : SY/MD
 Sample : 02334-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.660	3301	3303	3305	rBV3	1690	1002	0.06%	0.013%
78	11.866	3365	3367	3371	rVB4	1491	652	0.04%	0.008%
79	11.918	3381	3383	3385	rBV3	1066	458	0.03%	0.006%
80	11.982	3400	3403	3406	rBV5	2121	1130	0.07%	0.015%
81	12.082	3431	3434	3437	rBV5	1416	951	0.06%	0.012%
82	12.181	3460	3465	3466	rBV4	1496	1277	0.08%	0.017%
83	12.635	3604	3606	3609	rVB4	1407	709	0.04%	0.009%
84	12.670	3613	3617	3623	rBV7	2172	2842	0.17%	0.037%
85	12.754	3640	3643	3647	rBV5	1879	1768	0.11%	0.023%
86	12.786	3650	3653	3655	rBV4	1443	754	0.05%	0.010%
87	12.799	3655	3657	3660	rBV4	1179	938	0.06%	0.012%
88	12.815	3660	3662	3667	rVB5	1399	934	0.06%	0.012%
89	13.062	3737	3739	3742	rBV4	1146	865	0.05%	0.011%
90	13.123	3756	3758	3762	rBV4	1661	1417	0.09%	0.018%
91	13.207	3773	3784	3796	rBV	98666	158315	9.73%	2.051%
92	13.374	3833	3836	3837	rBV3	1673	891	0.05%	0.012%
93	13.619	3909	3912	3913	rBV2	1438	760	0.05%	0.010%
94	13.689	3924	3934	3947	rVB	44829	73644	4.52%	0.954%
95	13.754	3951	3954	3955	rBV3	1429	640	0.04%	0.008%
96	14.091	4057	4059	4063	rBV5	1477	982	0.06%	0.013%
97	14.188	4086	4089	4092	rBV5	1753	1301	0.08%	0.017%
98	14.265	4111	4113	4114	rBV3	1091	460	0.03%	0.006%
99	14.361	4140	4143	4145	rBV3	1706	912	0.06%	0.012%
100	14.374	4145	4147	4148	rBV2	1321	490	0.03%	0.006%




Sum of corrected areas: 7717631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030674.D
Acq On : 19 Apr 2023 18:53
Operator : SY/MD
Sample : 02334-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

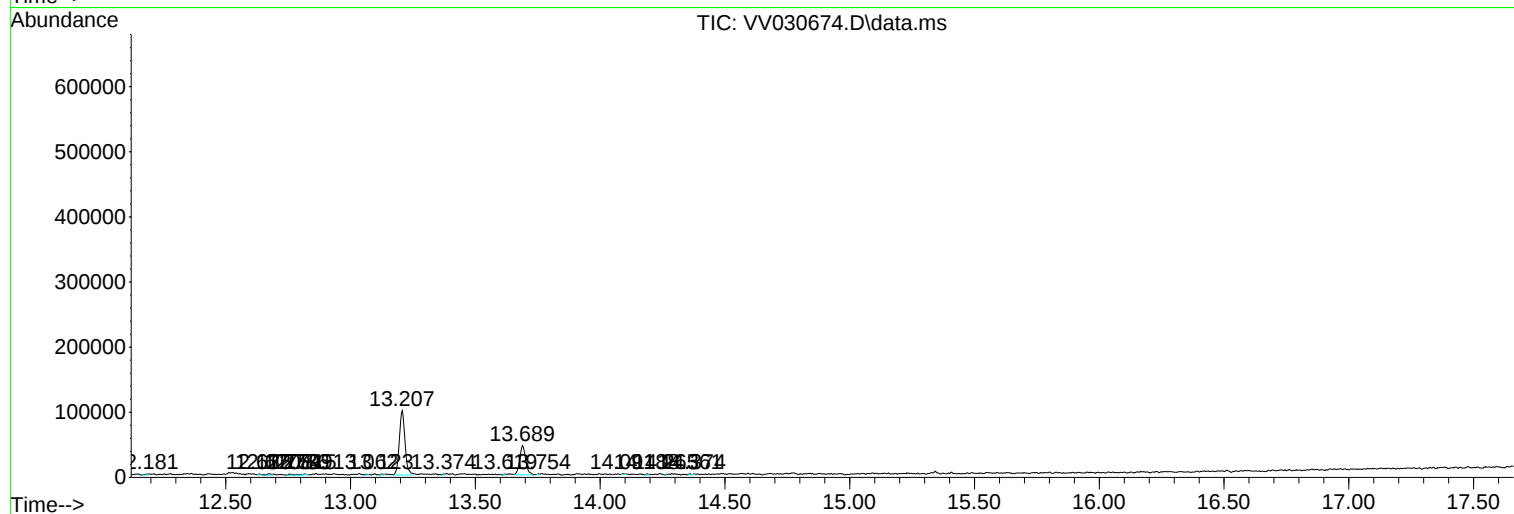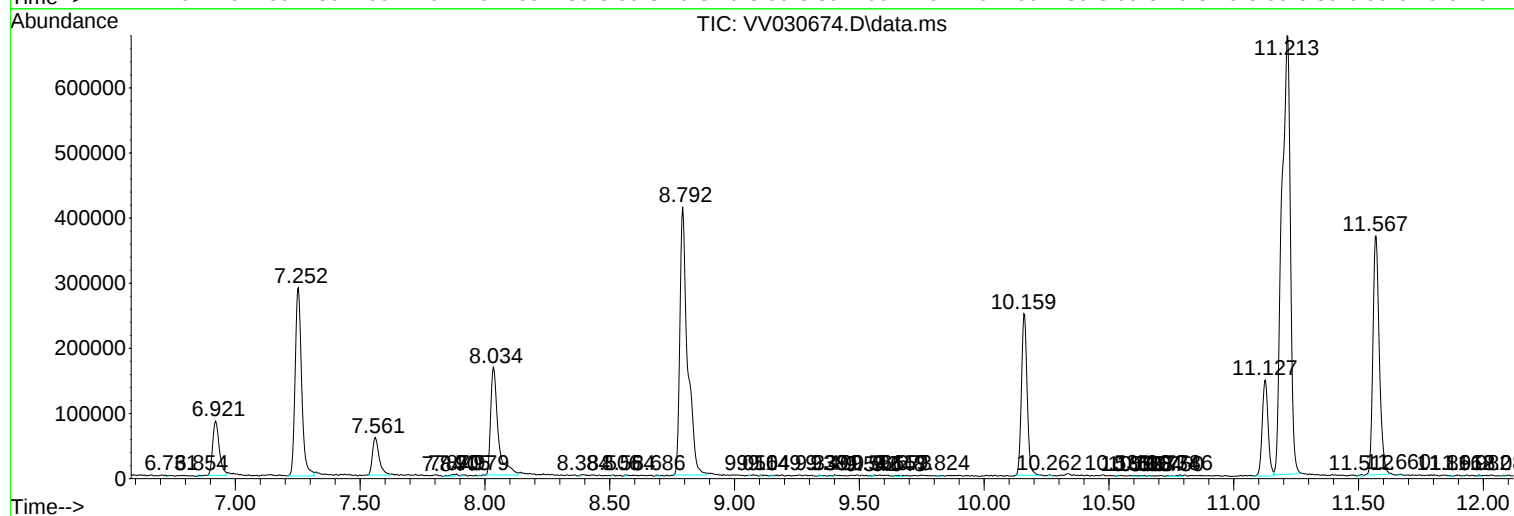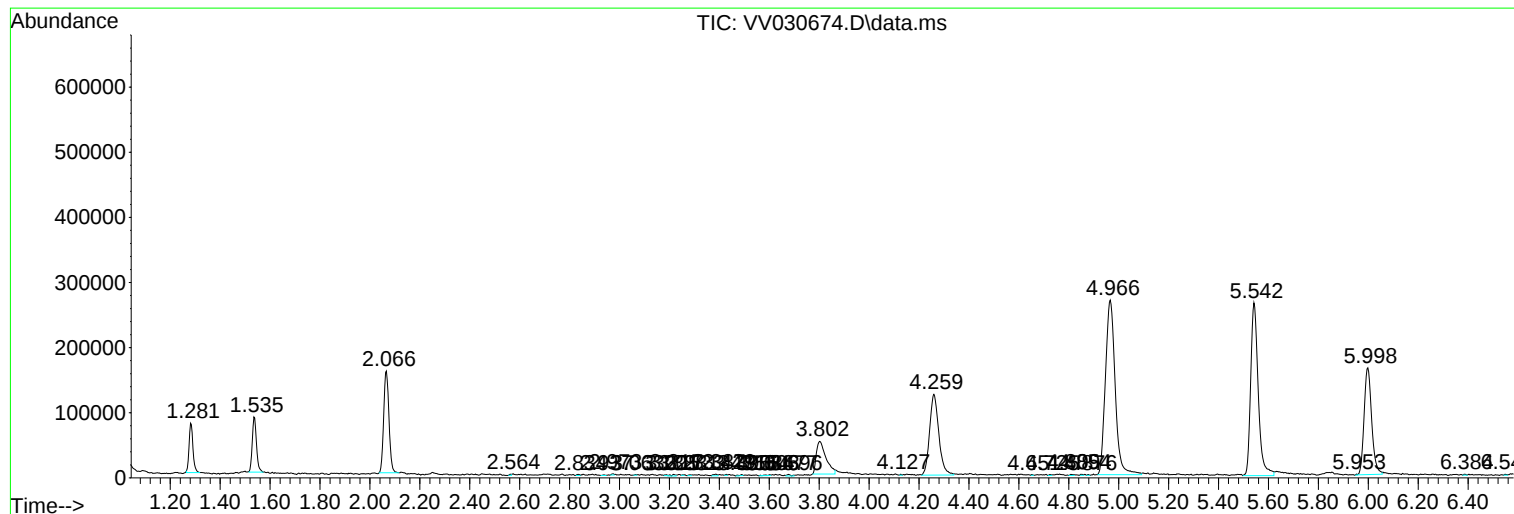

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030674.D
Acq On : 19 Apr 2023 18:53
Operator : SY/MD
Sample : 02334-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030674.D
Acq On : 19 Apr 2023 18:53
Operator : SY/MD
Sample : 02334-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------