

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030675.D
 Acq On : 19 Apr 2023 19:17
 Operator : SY/MD
 Sample : 02334-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	70	75	86	rVB	76050	80775	0.48%	0.169%
2	1.539	148	155	169	rVB	82768	99826	0.60%	0.209%
3	2.066	310	319	339	rVB	158330	234484	1.41%	0.492%
4	2.362	407	411	414	rVV7	1019	817	0.00%	0.002%
5	2.394	418	421	422	rBV3	1247	722	0.00%	0.002%
6	2.458	438	441	444	rBV5	2144	1374	0.01%	0.003%
7	2.536	463	465	468	rBV4	1266	911	0.01%	0.002%
8	2.590	477	482	483	rBV4	1872	1121	0.01%	0.002%
9	2.671	505	507	510	rBV4	1098	682	0.00%	0.001%
10	2.851	559	563	566	rBV6	2092	1865	0.01%	0.004%
11	3.153	653	657	659	rVB4	1585	978	0.01%	0.002%
12	3.166	659	661	665	rVB4	1423	789	0.00%	0.002%
13	3.211	670	675	676	rBV5	1025	712	0.00%	0.001%
14	3.278	693	696	697	rVV2	1648	804	0.00%	0.002%
15	3.352	714	719	720	rBV4	1270	908	0.01%	0.002%
16	3.436	742	745	746	rBV3	1257	682	0.00%	0.001%
17	3.458	751	752	756	rVB3	1643	967	0.01%	0.002%
18	3.558	777	783	787	rBV9	2051	2390	0.01%	0.005%
19	3.606	793	798	805	rBV10	1280	1598	0.01%	0.003%
20	3.651	810	812	814	rBV3	1273	769	0.00%	0.002%
21	3.799	849	858	885	rBV	54245	156536	0.94%	0.328%
22	4.195	979	981	983	rBV3	1114	760	0.00%	0.002%
23	4.207	983	985	987	rVV3	2218	1333	0.01%	0.003%
24	4.262	987	1002	1026	rVV	121562	317398	1.90%	0.665%
25	4.384	1038	1040	1042	rBV3	2026	1010	0.01%	0.002%
26	4.519	1078	1082	1085	rBV5	1855	1711	0.01%	0.004%
27	4.670	1127	1129	1132	rVB4	1550	902	0.01%	0.002%
28	4.728	1145	1147	1149	rVV2	1251	673	0.00%	0.001%
29	4.966	1205	1221	1248	rBV2	264109	711806	4.27%	1.492%
30	5.342	1336	1338	1341	rVB4	1420	663	0.00%	0.001%
31	5.439	1365	1368	1372	rVB6	1249	794	0.00%	0.002%
32	5.497	1383	1386	1387	rBV2	2203	1430	0.01%	0.003%
33	5.542	1389	1400	1427	rVV	263221	545681	3.27%	1.144%
34	5.998	1528	1542	1559	rBV2	165268	343980	2.06%	0.721%
35	6.207	1605	1607	1613	rBV7	1209	1301	0.01%	0.003%
36	6.294	1631	1634	1637	rVB5	1219	742	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030675.D
 Acq On : 19 Apr 2023 19:17
 Operator : SY/MD
 Sample : 02334-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.317	1637	1641	1643	rBV5	1738	1278	0.01%	0.003%
38	6.477	1689	1691	1694	rVB4	1974	946	0.01%	0.002%
39	6.513	1699	1702	1704	rBV4	1467	860	0.01%	0.002%
40	6.558	1714	1716	1720	rBV5	1018	834	0.01%	0.002%
41	6.654	1744	1746	1748	rVB3	2079	895	0.01%	0.002%
42	6.802	1789	1792	1793	rBV3	1713	978	0.01%	0.002%
43	6.921	1818	1829	1853	rBV	83344	159378	0.96%	0.334%
44	7.211	1916	1919	1920	rBV3	1644	849	0.01%	0.002%
45	7.252	1920	1932	1948	rVV	290597	520816	3.12%	1.092%
46	7.558	2018	2027	2043	rVV	59074	109786	0.66%	0.230%
47	7.751	2086	2087	2090	rBV3	1103	742	0.00%	0.002%
48	7.883	2125	2128	2129	rBV3	2386	1423	0.01%	0.003%
49	8.034	2163	2175	2204	rBV	185646	364164	2.18%	0.763%
50	8.397	2282	2288	2293	rBV	2022	2322	0.01%	0.005%
51	8.635	2358	2362	2364	rBV4	1784	1285	0.01%	0.003%
52	8.821	2399	2420	2442	rBV2	1530176	3162846	18.98%	6.631%
53	9.111	2507	2510	2512	rBV4	1606	958	0.01%	0.002%
54	9.320	2572	2575	2578	rVB5	2099	1438	0.01%	0.003%
55	9.339	2578	2581	2583	rBV4	1034	655	0.00%	0.001%
56	9.452	2614	2616	2621	rVB5	2355	1278	0.01%	0.003%
57	9.564	2647	2651	2653	rBV3	1811	1212	0.01%	0.003%
58	9.905	2755	2757	2759	rVB3	1798	726	0.00%	0.002%
59	9.924	2759	2763	2765	rBV4	1513	1029	0.01%	0.002%
60	9.979	2778	2780	2784	rVB4	1535	1057	0.01%	0.002%
61	10.001	2784	2787	2788	rBV3	1409	673	0.00%	0.001%
62	10.063	2801	2806	2808	rBV4	1300	1040	0.01%	0.002%
63	10.159	2825	2836	2853	rBV	254296	408460	2.45%	0.856%
64	10.255	2864	2866	2870	rBV4	1533	1190	0.01%	0.002%
65	10.320	2881	2886	2887	rBV5	3151	2313	0.01%	0.005%
66	10.477	2931	2935	2936	rBV4	1575	902	0.01%	0.002%
67	10.516	2944	2947	2950	rBV4	1328	964	0.01%	0.002%
68	10.590	2967	2970	2973	rVV5	1233	761	0.00%	0.002%
69	10.648	2986	2988	2990	rBV3	1987	920	0.01%	0.002%
70	10.728	3008	3013	3015	rBV6	933	870	0.01%	0.002%
71	10.976	3087	3090	3092	rBV3	1527	960	0.01%	0.002%
72	10.989	3092	3094	3098	rBV5	1366	1232	0.01%	0.003%
73	11.011	3098	3101	3106	rVB7	1387	1319	0.01%	0.003%
74	11.124	3123	3136	3148	rBV	1382325	2126515	12.76%	4.458%
75	11.217	3149	3165	3184	rVB	5910845	9348848	56.09%	19.600%
76	11.590	3265	3281	3308	rBV	10852697	16667226	100.00%	34.942%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030675.D
 Acq On : 19 Apr 2023 19:17
 Operator : SY/MD
 Sample : 02334-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.902	3376	3378	3380	rBV3	2098	1246	0.01%	0.003%
78	12.162	3456	3459	3462	rBV6	1013	780	0.00%	0.002%
79	12.281	3494	3496	3498	rBV3	1496	674	0.00%	0.001%
80	12.445	3544	3547	3551	rBV5	1566	1248	0.01%	0.003%
81	12.519	3559	3570	3574	rBV5	5236	8556	0.05%	0.018%
82	12.689	3619	3623	3624	rBV4	4182	2619	0.02%	0.005%
83	12.866	3672	3678	3681	rBV7	2141	2095	0.01%	0.004%
84	12.886	3681	3684	3685	rBV3	1913	846	0.01%	0.002%
85	12.931	3696	3698	3701	rBV3	1316	767	0.00%	0.002%
86	13.095	3745	3749	3753	rBV6	1219	1042	0.01%	0.002%
87	13.140	3759	3763	3764	rBV4	2351	1247	0.01%	0.003%
88	13.207	3771	3784	3807	rBV	5514322	8017939	48.11%	16.809%
89	13.689	3918	3934	3959	rBV	2726194	4089305	24.54%	8.573%
90	14.397	4151	4154	4155	rBV3	1988	902	0.01%	0.002%
91	14.564	4203	4206	4208	rBV4	1291	780	0.00%	0.002%
92	14.767	4254	4269	4282	rBV2	33179	74607	0.45%	0.156%
93	14.857	4295	4297	4301	rVB5	1675	1009	0.01%	0.002%
94	14.940	4320	4323	4325	rBV3	1945	1105	0.01%	0.002%
95	14.969	4329	4332	4335	rVB5	1831	1035	0.01%	0.002%
96	14.988	4335	4338	4343	rBV7	2643	2512	0.02%	0.005%
97	15.040	4352	4354	4357	rVB4	1497	724	0.00%	0.002%
98	15.056	4357	4359	4361	rBV4	1541	789	0.00%	0.002%
99	15.342	4441	4448	4462	rVB2	41734	64418	0.39%	0.135%
100	15.426	4471	4474	4475	rBV3	1788	1052	0.01%	0.002%




Sum of corrected areas: 47699139

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030675.D
Acq On : 19 Apr 2023 19:17
Operator : SY/MD
Sample : 02334-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

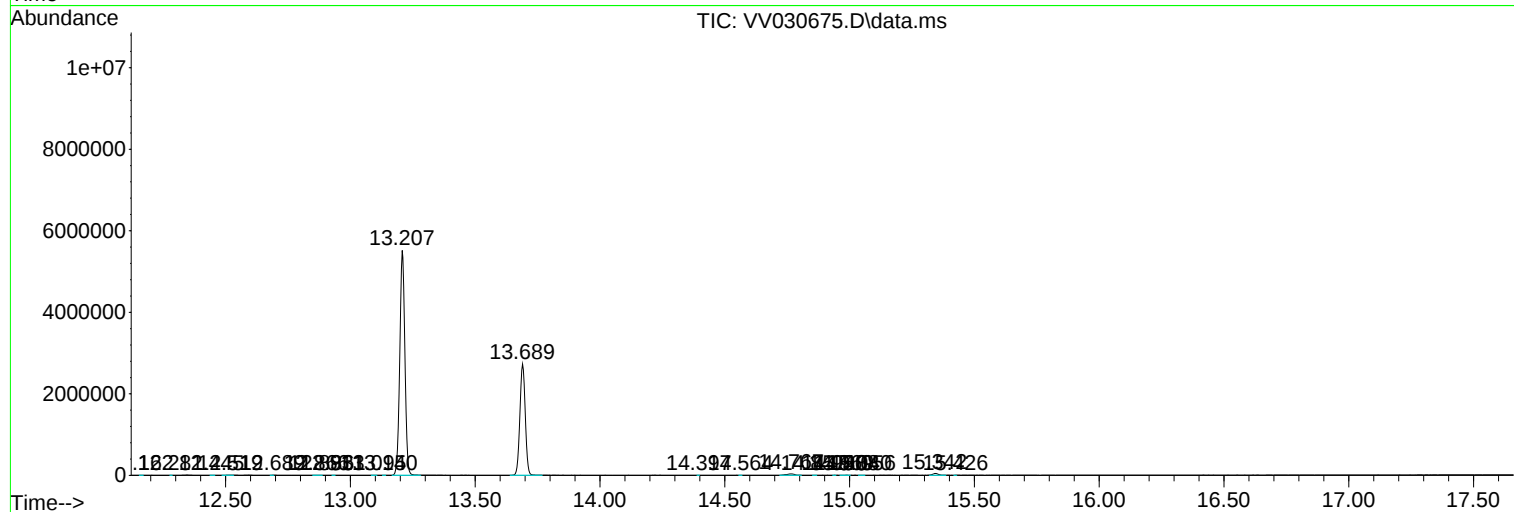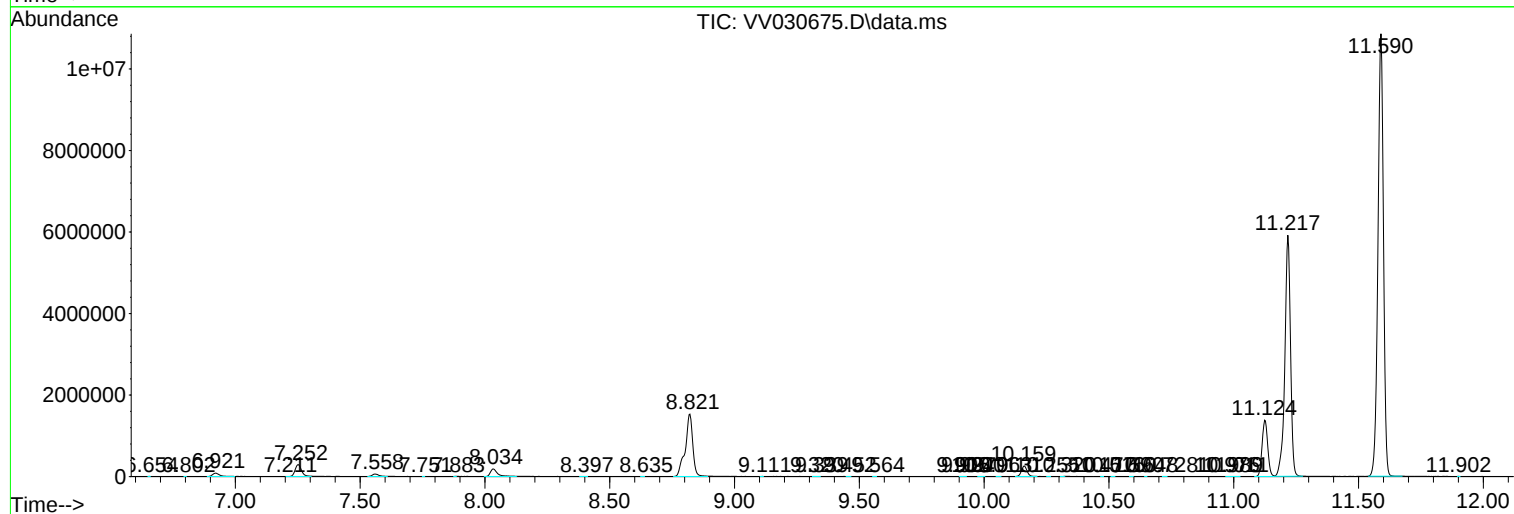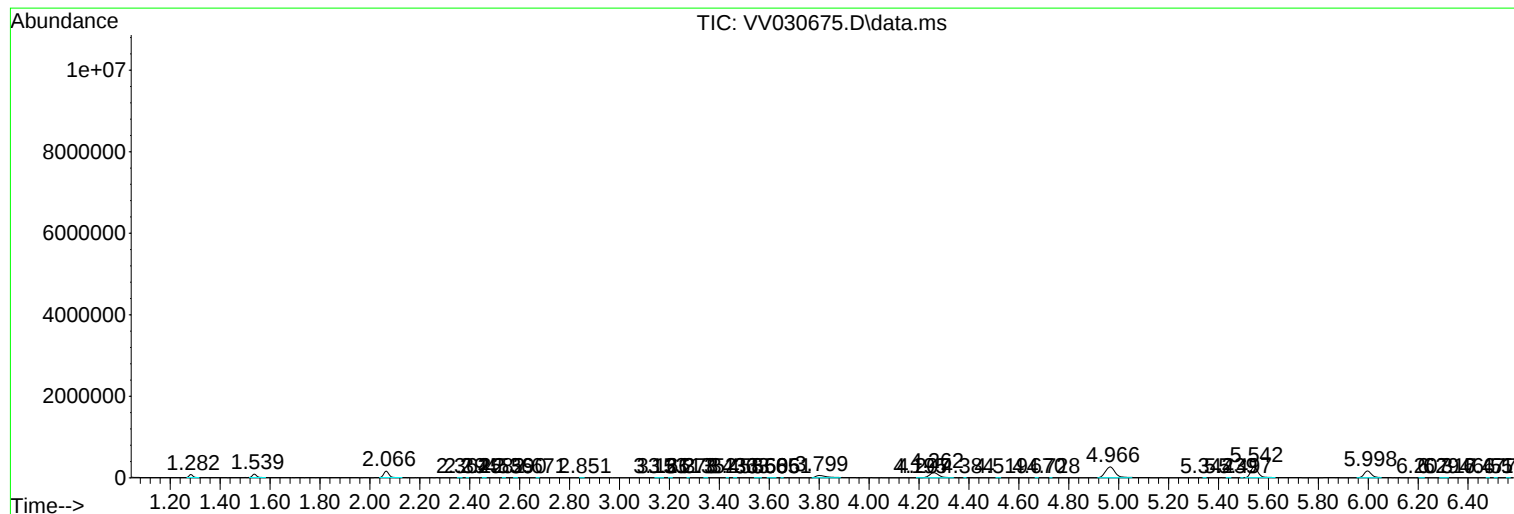

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030675.D
Acq On : 19 Apr 2023 19:17
Operator : SY/MD
Sample : 02334-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030675.D
Acq On : 19 Apr 2023 19:17
Operator : SY/MD
Sample : 02334-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc