

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030678.D
 Acq On : 19 Apr 2023 20:29
 Operator : SY/MD
 Sample : 02398-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	93	rVB	76527	83989	9.37%	1.252%
2	1.535	147	154	165	rVB	75946	87313	9.74%	1.301%
3	2.063	310	318	333	rVB	153367	221973	24.76%	3.309%
4	2.169	349	351	353	rBV2	1559	799	0.09%	0.012%
5	2.227	366	369	371	rBV4	1870	1428	0.16%	0.021%
6	2.323	397	399	401	rBV3	1207	561	0.06%	0.008%
7	2.368	410	413	416	rVB6	1824	1269	0.14%	0.019%
8	2.394	416	421	424	rBV7	1794	1801	0.20%	0.027%
9	2.458	432	441	449	rBV5	6337	10939	1.22%	0.163%
10	2.555	469	471	472	rBV2	1370	632	0.07%	0.009%
11	2.597	482	484	487	rBV3	1166	834	0.09%	0.012%
12	2.806	544	549	551	rBV6	1504	1479	0.16%	0.022%
13	2.854	562	564	567	rBV3	1784	750	0.08%	0.011%
14	2.896	575	577	582	rVB5	1127	878	0.10%	0.013%
15	3.040	618	622	624	rBV5	1627	1239	0.14%	0.018%
16	3.056	624	627	630	rVV4	1233	1035	0.12%	0.015%
17	3.108	641	643	646	rBV5	938	771	0.09%	0.011%
18	3.150	654	656	660	rBV5	1039	826	0.09%	0.012%
19	3.195	667	670	673	rBV4	1367	986	0.11%	0.015%
20	3.310	703	706	708	rBV4	1387	804	0.09%	0.012%
21	3.407	732	736	739	rBV5	1194	941	0.10%	0.014%
22	3.468	752	755	760	rVB7	1684	1464	0.16%	0.022%
23	3.494	760	763	765	rBV4	1391	878	0.10%	0.013%
24	3.555	775	782	789	rBV4	1754	2632	0.29%	0.039%
25	3.590	789	793	795	rBV5	1297	922	0.10%	0.014%
26	3.622	799	803	804	rBV4	1165	811	0.09%	0.012%
27	3.748	837	842	843	rBV5	1175	743	0.08%	0.011%
28	3.796	848	857	877	rBV2	60090	166044	18.52%	2.475%
29	4.185	974	978	980	rBV5	2438	1480	0.17%	0.022%
30	4.259	983	1001	1027	rVV	122394	320367	35.73%	4.775%
31	4.966	1205	1221	1231	rBV2	265626	701340	78.23%	10.454%
32	5.542	1388	1400	1421	rBV	260864	545721	60.87%	8.135%
33	5.805	1480	1482	1484	rBV2	1634	699	0.08%	0.010%
34	5.998	1530	1542	1564	rBV	168404	339776	37.90%	5.065%
35	6.220	1608	1611	1614	rVB4	2008	1458	0.16%	0.022%
36	6.493	1693	1696	1697	rBV3	1315	856	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW041923\
 Data File : VW030678.D
 Acq On : 19 Apr 2023 20:29
 Operator : SY/MD
 Sample : 02398-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.747	1773	1775	1779	rVB5	2595	1475	0.16%	0.022%
38	6.837	1801	1803	1806	rVB3	1720	969	0.11%	0.014%
39	6.857	1806	1809	1810	rBV3	1680	851	0.09%	0.013%
40	6.879	1814	1816	1818	rBV3	1172	655	0.07%	0.010%
41	6.921	1818	1829	1843	rBV	81508	152516	17.01%	2.273%
42	7.252	1921	1932	1958	rBV	283167	510658	56.96%	7.612%
43	7.561	2020	2028	2041	rBV	58031	97818	10.91%	1.458%
44	7.963	2150	2153	2157	rBV5	912	879	0.10%	0.013%
45	8.034	2165	2175	2188	rBV	178859	318048	35.48%	4.741%
46	8.416	2292	2294	2298	rVB5	2441	1299	0.14%	0.019%
47	8.522	2324	2327	2329	rBV4	1707	772	0.09%	0.012%
48	8.712	2381	2386	2387	rBV4	2973	1915	0.21%	0.029%
49	8.792	2399	2411	2415	rBV	416787	647598	72.24%	9.653%
50	9.043	2487	2489	2493	rVB4	1529	775	0.09%	0.012%
51	9.442	2611	2613	2616	rBV5	2001	1264	0.14%	0.019%
52	9.477	2619	2624	2626	rBV6	1223	1401	0.16%	0.021%
53	9.603	2660	2663	2665	rBV4	1279	863	0.10%	0.013%
54	10.162	2825	2837	2852	rBV	243054	399727	44.59%	5.958%
55	10.304	2878	2881	2883	rBV4	931	559	0.06%	0.008%
56	10.451	2924	2927	2930	rBV4	1338	1019	0.11%	0.015%
57	10.484	2935	2937	2940	rVB4	1500	788	0.09%	0.012%
58	10.587	2968	2969	2973	rBV4	992	601	0.07%	0.009%
59	10.776	3024	3028	3031	rBV5	1722	1427	0.16%	0.021%
60	10.792	3031	3033	3036	rVB3	1713	895	0.10%	0.013%
61	10.886	3058	3062	3063	rBV4	737	556	0.06%	0.008%
62	10.924	3069	3074	3075	rBV5	1193	897	0.10%	0.013%
63	11.014	3100	3102	3105	rBV3	1282	583	0.07%	0.009%
64	11.066	3115	3118	3120	rBV4	1595	861	0.10%	0.013%
65	11.127	3127	3137	3147	rVV3	26543	45402	5.06%	0.677%
66	11.194	3148	3158	3182	rVB2	414669	896509	100.00%	13.363%
67	11.432	3230	3232	3235	rBV5	1666	1235	0.14%	0.018%
68	11.570	3263	3275	3296	rBV3	405382	892269	99.53%	13.300%
69	11.982	3401	3403	3407	rBV5	1342	912	0.10%	0.014%
70	12.133	3447	3450	3452	rBV4	1209	757	0.08%	0.011%
71	12.204	3466	3472	3475	rBV7	1565	1572	0.18%	0.023%
72	12.230	3478	3480	3483	rBV3	1506	1144	0.13%	0.017%
73	12.268	3490	3492	3495	rBV3	1227	913	0.10%	0.014%
74	12.422	3538	3540	3542	rBV4	1997	1087	0.12%	0.016%
75	12.458	3549	3551	3554	rBV3	945	589	0.07%	0.009%
76	12.519	3567	3570	3571	rBV3	2090	919	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030678.D
 Acq On : 19 Apr 2023 20:29
 Operator : SY/MD
 Sample : 02398-01DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMN0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.638	3604	3607	3609	rBV3	1225	618	0.07%	0.009%
78	12.680	3616	3620	3621	rBV4	1049	778	0.09%	0.012%
79	12.779	3648	3651	3655	rVB6	1606	1120	0.12%	0.017%
80	12.799	3655	3657	3661	rBV5	1142	989	0.11%	0.015%
81	12.837	3666	3669	3672	rVV5	1419	1244	0.14%	0.019%
82	12.908	3689	3691	3693	rBV3	1291	600	0.07%	0.009%
83	12.921	3693	3695	3697	rVB2	1466	597	0.07%	0.009%
84	13.075	3741	3743	3745	rBV3	1235	624	0.07%	0.009%
85	13.114	3751	3755	3756	rBV4	1104	697	0.08%	0.010%
86	13.152	3763	3767	3768	rBV4	1964	1401	0.16%	0.021%
87	13.207	3774	3784	3798	rVB2	88115	138945	15.50%	2.071%
88	13.361	3826	3832	3833	rBV6	1805	1618	0.18%	0.024%
89	13.429	3851	3853	3854	rBV3	1552	671	0.07%	0.010%
90	13.590	3901	3903	3905	rBV3	1202	683	0.08%	0.010%
91	13.689	3925	3934	3945	rBV3	32168	51599	5.76%	0.769%
92	13.921	4001	4006	4007	rBV5	2022	1408	0.16%	0.021%
93	14.030	4037	4040	4042	rBV3	1794	1184	0.13%	0.018%
94	14.162	4078	4081	4083	rBV4	1340	956	0.11%	0.014%
95	14.538	4196	4198	4201	rBV3	1654	919	0.10%	0.014%
96	14.554	4201	4203	4206	rBV4	1523	910	0.10%	0.014%
97	14.609	4218	4220	4221	rBV2	1173	575	0.06%	0.009%
98	14.657	4229	4235	4237	rBV6	1410	1430	0.16%	0.021%
99	14.850	4293	4295	4296	rBV3	1603	716	0.08%	0.011%
100	14.914	4312	4315	4316	rBV3	1732	982	0.11%	0.015%

Sum of corrected areas: 6708679




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030678.D
Acq On : 19 Apr 2023 20:29
Operator : SY/MD
Sample : 02398-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMMONDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

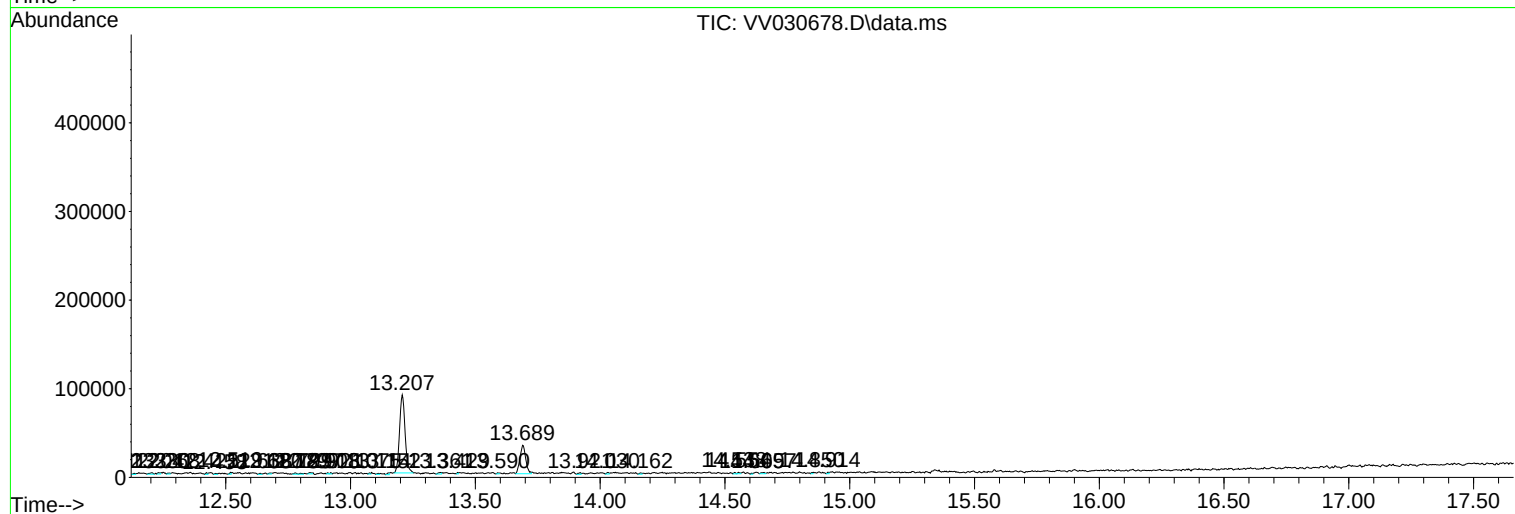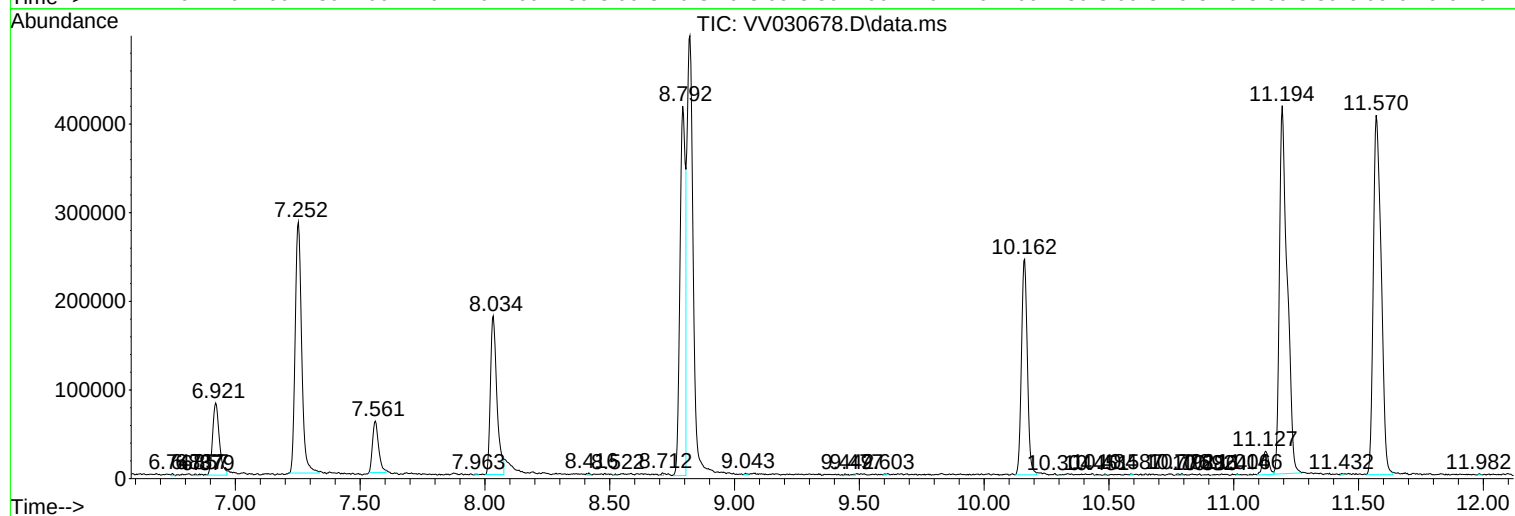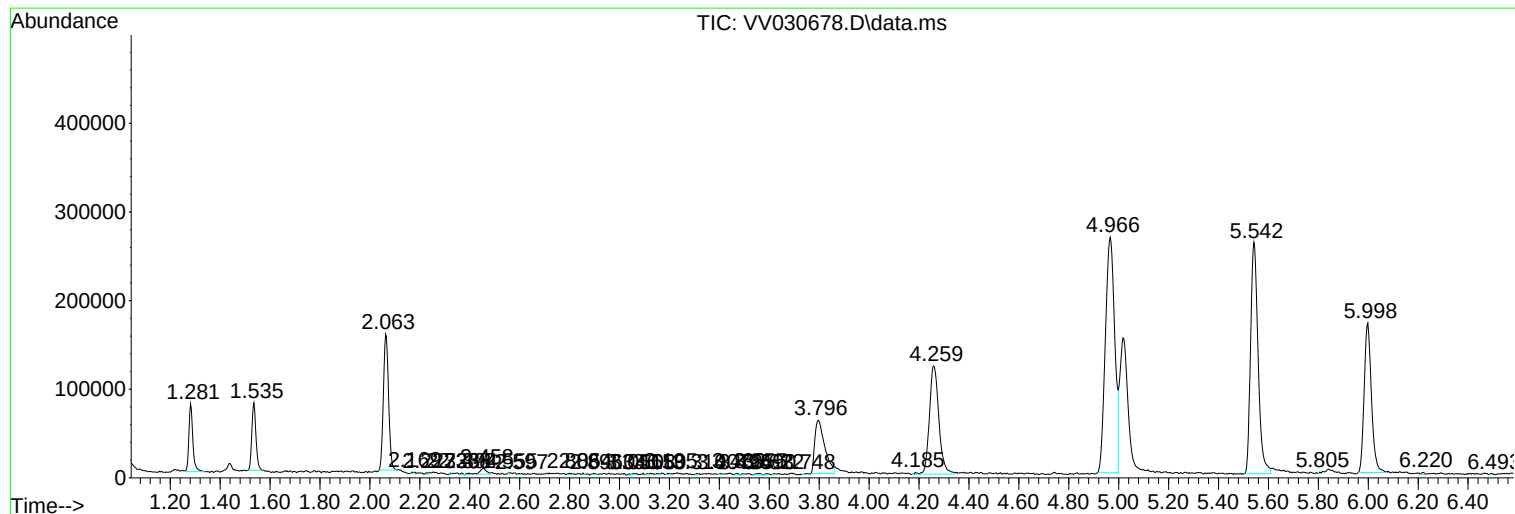

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030678.D
Acq On : 19 Apr 2023 20:29
Operator : SY/MD
Sample : 02398-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMMONDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030678.D
Acq On : 19 Apr 2023 20:29
Operator : SY/MD
Sample : 02398-01DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMMONDL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------