

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030680.D
 Acq On : 19 Apr 2023 21:40
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rBV	139137	148550	15.89%	2.100%
2	1.536	148	154	165	rVB	118090	136849	14.64%	1.935%
3	2.063	309	318	330	rBV	246143	360689	38.58%	5.100%
4	2.616	489	490	493	rBV3	1221	810	0.09%	0.011%
5	2.764	533	536	540	rVB6	1373	964	0.10%	0.014%
6	2.790	540	544	546	rBV4	1077	897	0.10%	0.013%
7	2.899	573	578	584	rBV9	1771	2411	0.26%	0.034%
8	2.970	599	600	604	rVV4	1263	697	0.07%	0.010%
9	3.050	623	625	630	rVB5	1219	713	0.08%	0.010%
10	3.082	632	635	637	rVB4	1599	794	0.08%	0.011%
11	3.220	675	678	682	rBV5	1637	1426	0.15%	0.020%
12	3.253	686	688	695	rBV7	1761	1892	0.20%	0.027%
13	3.298	699	702	705	rVB5	1397	930	0.10%	0.013%
14	3.320	705	709	710	rBV3	1130	783	0.08%	0.011%
15	3.471	751	756	758	rBV5	1700	1480	0.16%	0.021%
16	3.484	758	760	763	rVB4	1509	768	0.08%	0.011%
17	3.500	763	765	772	rBV7	1585	1930	0.21%	0.027%
18	3.539	774	777	779	rVB3	1777	892	0.10%	0.013%
19	3.642	807	809	812	rBV3	1155	957	0.10%	0.014%
20	3.706	825	829	832	rVB6	1849	1479	0.16%	0.021%
21	3.751	838	843	844	rBV5	1139	1140	0.12%	0.016%
22	3.793	848	856	885	rVV2	59390	164117	17.55%	2.320%
23	4.121	954	958	962	rBV6	2024	1522	0.16%	0.022%
24	4.259	987	1001	1021	rBV	149692	372041	39.80%	5.260%
25	4.558	1091	1094	1097	rBV6	1691	1287	0.14%	0.018%
26	4.786	1162	1165	1168	rBV5	2328	1760	0.19%	0.025%
27	4.966	1203	1221	1247	rBV2	350127	934874	100.00%	13.218%
28	5.301	1321	1325	1326	rBV3	1390	862	0.09%	0.012%
29	5.400	1353	1356	1359	rBV5	1741	1007	0.11%	0.014%
30	5.542	1387	1400	1424	rBV	270655	568458	60.81%	8.038%
31	5.998	1529	1542	1559	rBV	203692	421192	45.05%	5.955%
32	6.185	1596	1600	1601	rBV3	1879	1073	0.11%	0.015%
33	6.539	1706	1710	1717	rVB7	2378	2643	0.28%	0.037%
34	6.571	1717	1720	1722	rBV4	1933	1307	0.14%	0.018%
35	6.584	1722	1724	1728	rVV4	1344	856	0.09%	0.012%
36	6.828	1797	1800	1803	rVB5	1479	785	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030680.D
 Acq On : 19 Apr 2023 21:40
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1847	rBV	105891	194229	20.78%	2.746%
38	7.252	1920	1932	1959	rBV	395904	703732	75.28%	9.950%
39	7.558	2019	2027	2045	rBV	77364	131216	14.04%	1.855%
40	8.034	2165	2175	2208	rBV	188120	380438	40.69%	5.379%
41	8.719	2384	2388	2390	rBV5	1453	924	0.10%	0.013%
42	8.754	2394	2399	2400	rBV5	1200	1002	0.11%	0.014%
43	8.792	2400	2411	2436	rBV	409577	699273	74.80%	9.887%
44	9.085	2499	2502	2506	rBV5	1712	1212	0.13%	0.017%
45	9.182	2529	2532	2535	rBV4	1778	1414	0.15%	0.020%
46	9.313	2568	2573	2576	rBV6	1537	1266	0.14%	0.018%
47	9.352	2583	2585	2591	rVB5	1307	1261	0.13%	0.018%
48	9.471	2619	2622	2624	rBV4	1376	775	0.08%	0.011%
49	9.815	2728	2729	2734	rBV5	1358	758	0.08%	0.011%
50	9.937	2764	2767	2768	rBV3	1350	717	0.08%	0.010%
51	10.014	2788	2791	2794	rBV5	1728	1178	0.13%	0.017%
52	10.159	2825	2836	2856	rBV	265199	436339	46.67%	6.169%
53	10.275	2870	2872	2875	rBV4	1692	904	0.10%	0.013%
54	10.294	2875	2878	2880	rVV3	1429	828	0.09%	0.012%
55	10.400	2909	2911	2914	rBV3	1363	950	0.10%	0.013%
56	10.567	2961	2963	2967	rVB4	1323	702	0.08%	0.010%
57	10.680	2996	2998	3001	rVB4	1778	858	0.09%	0.012%
58	10.706	3001	3006	3007	rBV4	1780	1668	0.18%	0.024%
59	10.751	3017	3020	3023	rBV4	1093	865	0.09%	0.012%
60	10.789	3028	3032	3033	rBV3	1908	1125	0.12%	0.016%
61	10.850	3048	3051	3054	rBV4	1483	1187	0.13%	0.017%
62	10.937	3075	3078	3081	rVV4	1586	1141	0.12%	0.016%
63	10.976	3086	3090	3092	rBV5	1182	829	0.09%	0.012%
64	11.059	3112	3116	3121	rBV8	1843	1837	0.20%	0.026%
65	11.194	3146	3158	3179	rBV	399124	651507	69.69%	9.212%
66	11.567	3264	3274	3296	rVB	387719	642554	68.73%	9.085%
67	11.715	3317	3320	3324	rBV5	2341	1976	0.21%	0.028%
68	11.799	3339	3346	3352	rBV10	2840	3435	0.37%	0.049%
69	11.828	3352	3355	3359	rBV4	1173	906	0.10%	0.013%
70	12.001	3407	3409	3411	rBV3	1263	692	0.07%	0.010%
71	12.307	3500	3504	3507	rVB6	1509	1084	0.12%	0.015%
72	12.365	3520	3522	3528	rBV5	1441	1486	0.16%	0.021%
73	12.413	3534	3537	3539	rBV5	1629	745	0.08%	0.011%
74	12.426	3539	3541	3545	rVB4	2229	1318	0.14%	0.019%
75	12.461	3549	3552	3553	rBV3	1833	903	0.10%	0.013%
76	12.487	3556	3560	3561	rBV3	1364	760	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030680.D
 Acq On : 19 Apr 2023 21:40
 Operator : SY/MD
 Sample : VV0419WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK326

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.529	3569	3573	3575	rBV4	1451	1329	0.14%	0.019%
78	12.554	3579	3581	3585	rVB4	1542	780	0.08%	0.011%
79	12.590	3587	3592	3604	rVB4	3811	5790	0.62%	0.082%
80	12.696	3621	3625	3626	rBV4	1075	730	0.08%	0.010%
81	12.747	3639	3641	3646	rBV5	1980	1866	0.20%	0.026%
82	12.866	3675	3678	3681	rBV5	1426	1019	0.11%	0.014%
83	12.956	3704	3706	3711	rBV5	1159	1248	0.13%	0.018%
84	12.979	3711	3713	3716	rVV4	1507	845	0.09%	0.012%
85	13.210	3778	3785	3795	rVB9	8762	13731	1.47%	0.194%
86	13.577	3894	3899	3903	rVB8	1381	1202	0.13%	0.017%
87	13.599	3903	3906	3908	rBV5	1332	945	0.10%	0.013%
88	13.693	3924	3935	3943	rBV5	7529	13272	1.42%	0.188%
89	13.738	3947	3949	3955	rBV6	1945	1545	0.17%	0.022%
90	13.876	3989	3992	3997	rBV8	1326	1280	0.14%	0.018%
91	13.927	4005	4008	4010	rBV4	1812	1092	0.12%	0.015%
92	14.091	4057	4059	4064	rBV6	1325	1173	0.13%	0.017%
93	14.156	4077	4079	4082	rBV4	1380	813	0.09%	0.011%
94	14.210	4093	4096	4099	rBV4	1502	864	0.09%	0.012%
95	14.230	4099	4102	4105	rBV5	1578	1008	0.11%	0.014%
96	14.332	4133	4134	4138	rVB4	2077	817	0.09%	0.012%
97	14.429	4162	4164	4166	rVB3	1616	712	0.08%	0.010%
98	14.513	4187	4190	4194	rBV6	1699	1047	0.11%	0.015%
99	14.654	4231	4234	4237	rVB4	2285	1256	0.13%	0.018%
100	15.098	4368	4372	4375	rBV6	1686	1355	0.14%	0.019%




Sum of corrected areas: 7072548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030680.D
Acq On : 19 Apr 2023 21:40
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

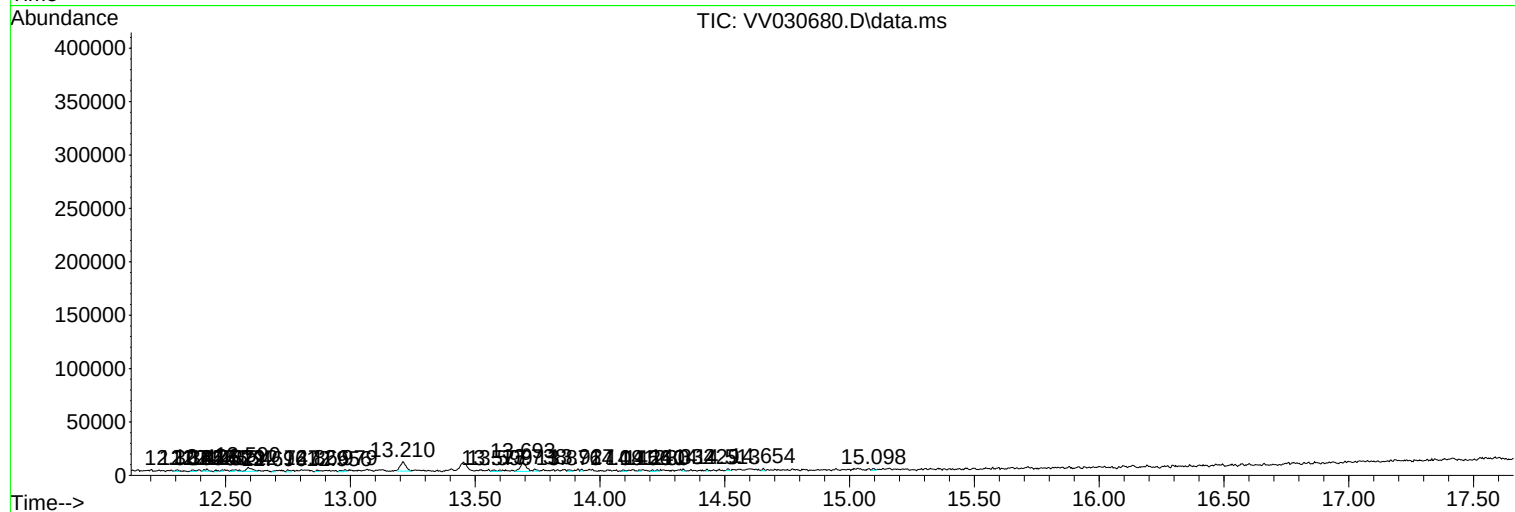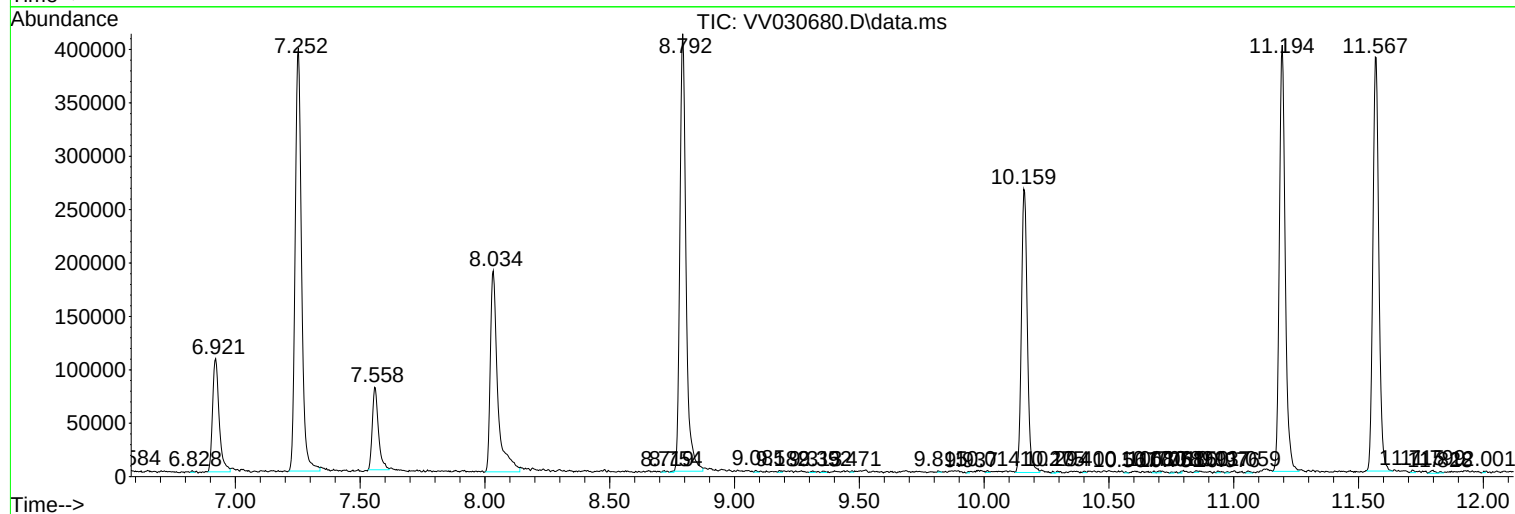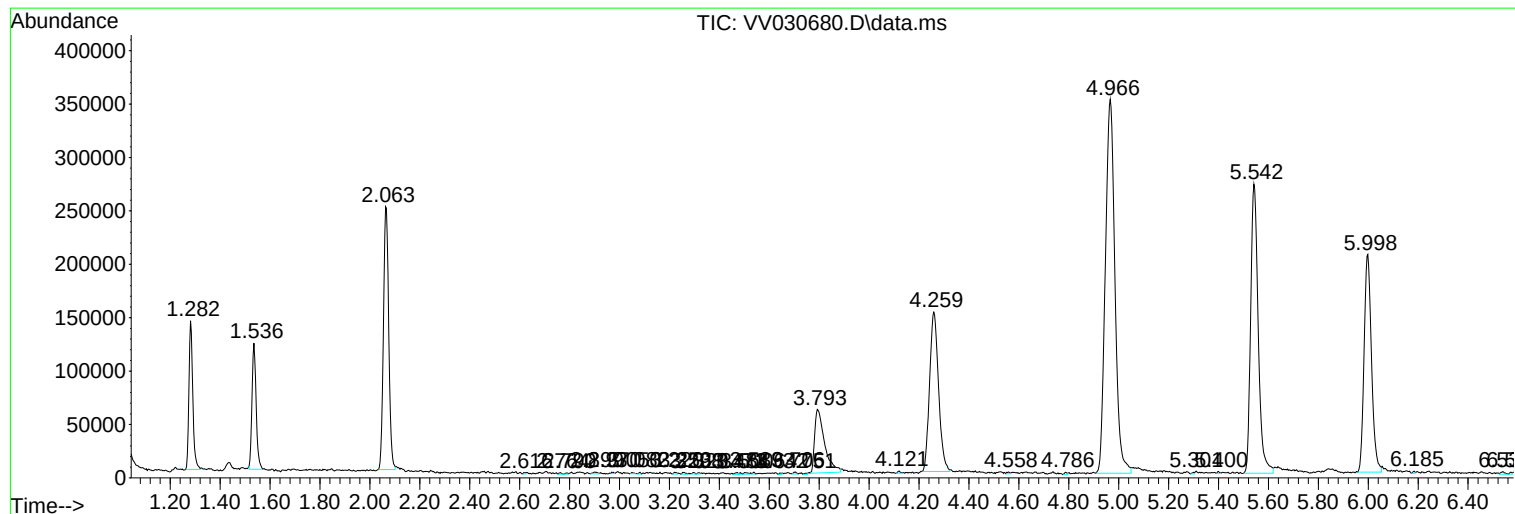

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030680.D
Acq On : 19 Apr 2023 21:40
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030680.D
Acq On : 19 Apr 2023 21:40
Operator : SY/MD
Sample : VV0419WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK326

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------