

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030682.D
 Acq On : 19 Apr 2023 22:34
 Operator : SY/MD
 Sample : 02334-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	76759	81371	11.61%	1.407%
2	1.400	110	112	113	rBV2	2293	822	0.12%	0.014%
3	1.535	148	154	165	rVB	75596	86406	12.33%	1.494%
4	2.063	309	318	334	rBV	156750	232684	33.19%	4.025%
5	2.320	396	398	401	rBV4	1295	1011	0.14%	0.017%
6	2.500	452	454	457	rBV4	1257	837	0.12%	0.014%
7	2.526	460	462	466	rBV5	1275	779	0.11%	0.013%
8	2.593	480	483	484	rBV2	1774	840	0.12%	0.015%
9	2.825	552	555	561	rVB7	2302	2070	0.30%	0.036%
10	2.857	563	565	567	rVB3	1584	738	0.11%	0.013%
11	2.937	587	590	593	rVB4	1258	919	0.13%	0.016%
12	2.989	604	606	611	rBV6	1200	965	0.14%	0.017%
13	3.063	626	629	631	rBV4	1219	683	0.10%	0.012%
14	3.088	635	637	641	rVB5	2018	1242	0.18%	0.021%
15	3.121	643	647	650	rVB6	1847	1361	0.19%	0.024%
16	3.143	650	654	656	rBV5	1196	804	0.11%	0.014%
17	3.339	707	715	717	rBV10	1341	1659	0.24%	0.029%
18	3.439	744	746	751	rVB6	2152	1501	0.21%	0.026%
19	3.468	751	755	758	rBV5	1457	1243	0.18%	0.021%
20	3.532	773	775	777	rBV2	1190	721	0.10%	0.012%
21	3.616	796	801	804	rBV6	2591	1914	0.27%	0.033%
22	3.719	831	833	837	rBV3	1053	769	0.11%	0.013%
23	3.748	840	842	847	rVB6	1559	991	0.14%	0.017%
24	3.793	847	856	881	rBV	58697	158970	22.68%	2.750%
25	4.146	963	966	970	rBV5	1445	1383	0.20%	0.024%
26	4.259	989	1001	1024	rVB	118939	295876	42.21%	5.118%
27	4.661	1122	1126	1130	rVB6	1006	770	0.11%	0.013%
28	4.805	1170	1171	1175	rVV3	1848	1025	0.15%	0.018%
29	4.863	1185	1189	1190	rBV4	1343	938	0.13%	0.016%
30	4.899	1198	1200	1204	rBV5	1169	802	0.11%	0.014%
31	4.966	1205	1221	1245	rVV3	265337	700973	100.00%	12.124%
32	5.368	1343	1346	1350	rBV4	1792	993	0.14%	0.017%
33	5.448	1368	1371	1373	rVB4	1533	710	0.10%	0.012%
34	5.542	1389	1400	1427	rBV	253121	524918	74.88%	9.079%
35	5.998	1530	1542	1560	rBV	162569	327689	46.75%	5.668%
36	6.243	1615	1618	1623	rVB6	1517	1243	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030682.D
 Acq On : 19 Apr 2023 22:34
 Operator : SY/MD
 Sample : 02334-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.313	1637	1640	1642	rBV2	1247	762	0.11%	0.013%
38	6.362	1652	1655	1657	rBV4	1274	778	0.11%	0.013%
39	6.510	1699	1701	1703	rVV3	1294	667	0.10%	0.012%
40	6.722	1763	1767	1769	rBV4	1608	1265	0.18%	0.022%
41	6.831	1798	1801	1802	rBV3	1374	720	0.10%	0.012%
42	6.921	1819	1829	1847	rBV2	81393	151641	21.63%	2.623%
43	7.114	1887	1889	1892	rBV3	1510	1205	0.17%	0.021%
44	7.169	1899	1906	1911	rBV10	2085	3370	0.48%	0.058%
45	7.252	1921	1932	1952	rBV	281185	496826	70.88%	8.593%
46	7.471	1997	2000	2002	rBV3	1165	727	0.10%	0.013%
47	7.561	2019	2028	2040	rBV	59192	99800	14.24%	1.726%
48	8.034	2165	2175	2188	rBV	175566	315631	45.03%	5.459%
49	8.387	2283	2285	2289	rVB5	1550	685	0.10%	0.012%
50	8.606	2351	2353	2360	rVB8	2169	2692	0.38%	0.047%
51	8.648	2360	2366	2367	rBV5	2038	1624	0.23%	0.028%
52	8.792	2400	2411	2434	rVV	392430	667092	95.17%	11.538%
53	9.062	2490	2495	2496	rBV4	1415	1243	0.18%	0.021%
54	9.146	2518	2521	2523	rVB3	1661	970	0.14%	0.017%
55	9.162	2523	2526	2529	rBV5	1292	1187	0.17%	0.021%
56	9.230	2544	2547	2548	rBV3	1568	785	0.11%	0.014%
57	9.329	2574	2578	2580	rBV5	1566	1202	0.17%	0.021%
58	9.342	2580	2582	2584	rBV3	1456	734	0.10%	0.013%
59	9.484	2621	2626	2629	rBV6	1220	1165	0.17%	0.020%
60	9.503	2629	2632	2635	rBV4	1529	965	0.14%	0.017%
61	9.606	2661	2664	2669	rBV6	2108	1912	0.27%	0.033%
62	9.712	2695	2697	2699	rVB2	2066	837	0.12%	0.014%
63	9.998	2783	2786	2789	rBV5	1366	1246	0.18%	0.022%
64	10.043	2797	2800	2802	rBV4	2053	1059	0.15%	0.018%
65	10.120	2821	2824	2825	rBV3	1291	868	0.12%	0.015%
66	10.162	2826	2837	2854	rVV	240697	390460	55.70%	6.753%
67	10.249	2862	2864	2867	rVB4	2080	826	0.12%	0.014%
68	10.294	2875	2878	2880	rBV4	1579	676	0.10%	0.012%
69	10.390	2904	2908	2912	rBV7	2011	1671	0.24%	0.029%
70	10.448	2922	2926	2929	rBV4	1277	693	0.10%	0.012%
71	10.802	3032	3036	3038	rBV5	1931	1501	0.21%	0.026%
72	11.072	3116	3120	3124	rBV8	1208	1001	0.14%	0.017%
73	11.120	3132	3135	3138	rBV4	1680	1322	0.19%	0.023%
74	11.194	3145	3158	3177	rBV	369887	613463	87.52%	10.611%
75	11.423	3227	3229	3232	rBV4	1455	848	0.12%	0.015%
76	11.570	3264	3275	3294	rVB	327743	539039	76.90%	9.323%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
 Data File : VV030682.D
 Acq On : 19 Apr 2023 22:34
 Operator : SY/MD
 Sample : 02334-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.709	3316	3318	3320	rBV3	1533	660	0.09%	0.011%
78	11.744	3325	3329	3334	rBV7	1234	1252	0.18%	0.022%
79	11.770	3334	3337	3339	rBV3	1475	700	0.10%	0.012%
80	11.808	3348	3349	3354	rBV4	1353	874	0.12%	0.015%
81	11.947	3389	3392	3393	rBV3	1576	856	0.12%	0.015%
82	12.014	3411	3413	3414	rBV2	1571	657	0.09%	0.011%
83	12.120	3442	3446	3447	rBV4	1373	678	0.10%	0.012%
84	12.156	3450	3457	3458	rBV6	1011	1101	0.16%	0.019%
85	12.384	3526	3528	3530	rBV3	1977	662	0.09%	0.011%
86	12.513	3566	3568	3572	rVV4	1175	668	0.10%	0.012%
87	12.702	3623	3627	3631	rBV7	1215	1178	0.17%	0.020%
88	12.802	3655	3658	3662	rBV5	1777	1358	0.19%	0.023%
89	12.863	3675	3677	3684	rVB7	2012	1723	0.25%	0.030%
90	12.998	3715	3719	3723	rBV7	1553	1693	0.24%	0.029%
91	13.053	3732	3736	3737	rBV4	1442	868	0.12%	0.015%
92	13.178	3770	3775	3776	rBV5	1774	1228	0.18%	0.021%
93	13.316	3815	3818	3821	rBV5	1971	1506	0.21%	0.026%
94	13.696	3926	3936	3943	rBV5	3670	7876	1.12%	0.136%
95	13.808	3968	3971	3974	rBV5	1318	966	0.14%	0.017%
96	13.866	3987	3989	3992	rBV4	1379	949	0.14%	0.016%
97	14.210	4094	4096	4098	rBV3	1429	732	0.10%	0.013%
98	14.516	4189	4191	4194	rBV4	1569	1079	0.15%	0.019%
99	14.754	4261	4265	4267	rBV5	1551	1076	0.15%	0.019%
100	14.998	4338	4341	4347	rBV8	1905	1504	0.21%	0.026%




Sum of corrected areas: 5781622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030682.D
Acq On : 19 Apr 2023 22:34
Operator : SY/MD
Sample : 02334-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

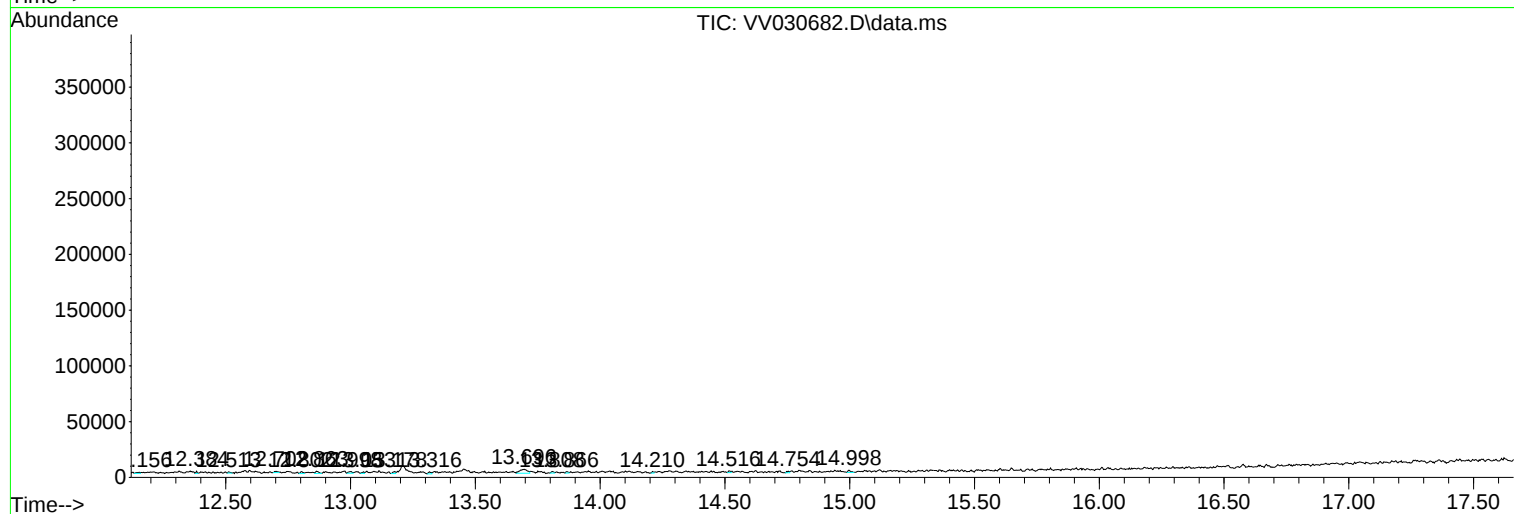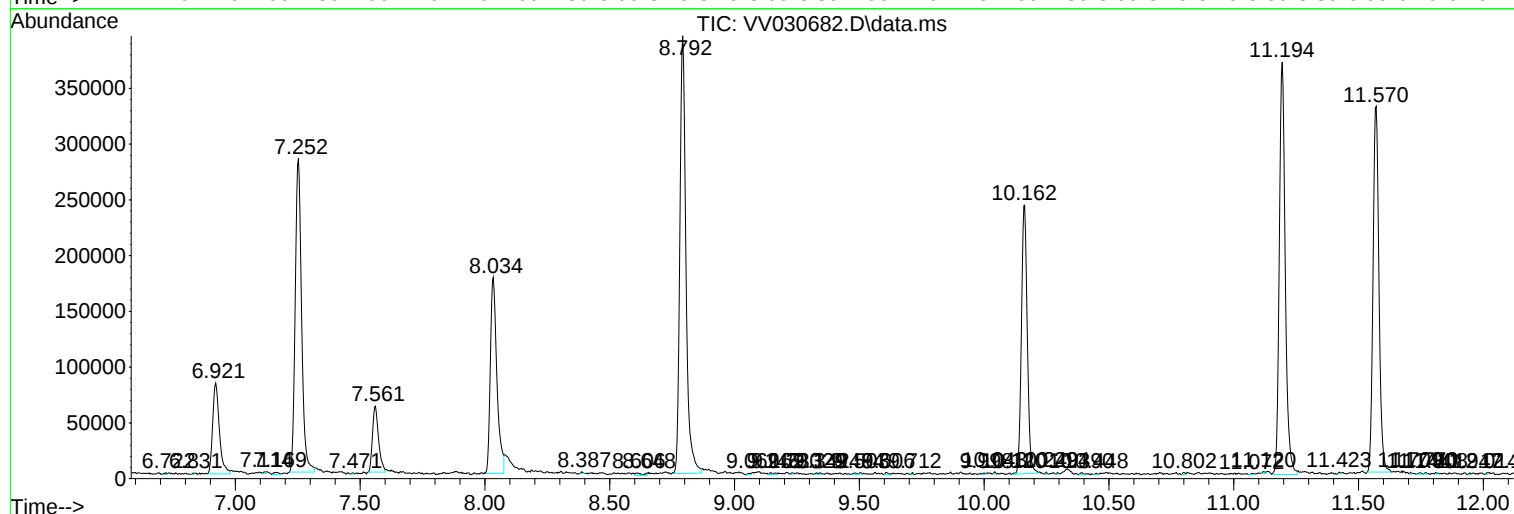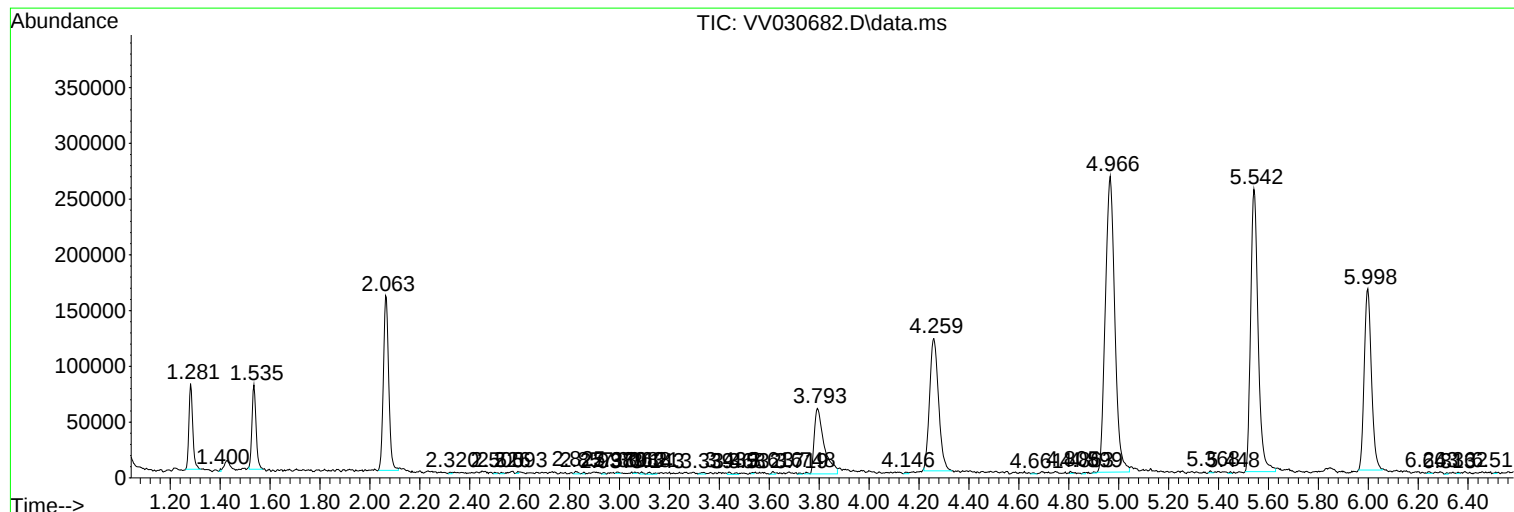

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030682.D
Acq On : 19 Apr 2023 22:34
Operator : SY/MD
Sample : 02334-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030682.D
Acq On : 19 Apr 2023 22:34
Operator : SY/MD
Sample : 02334-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------