
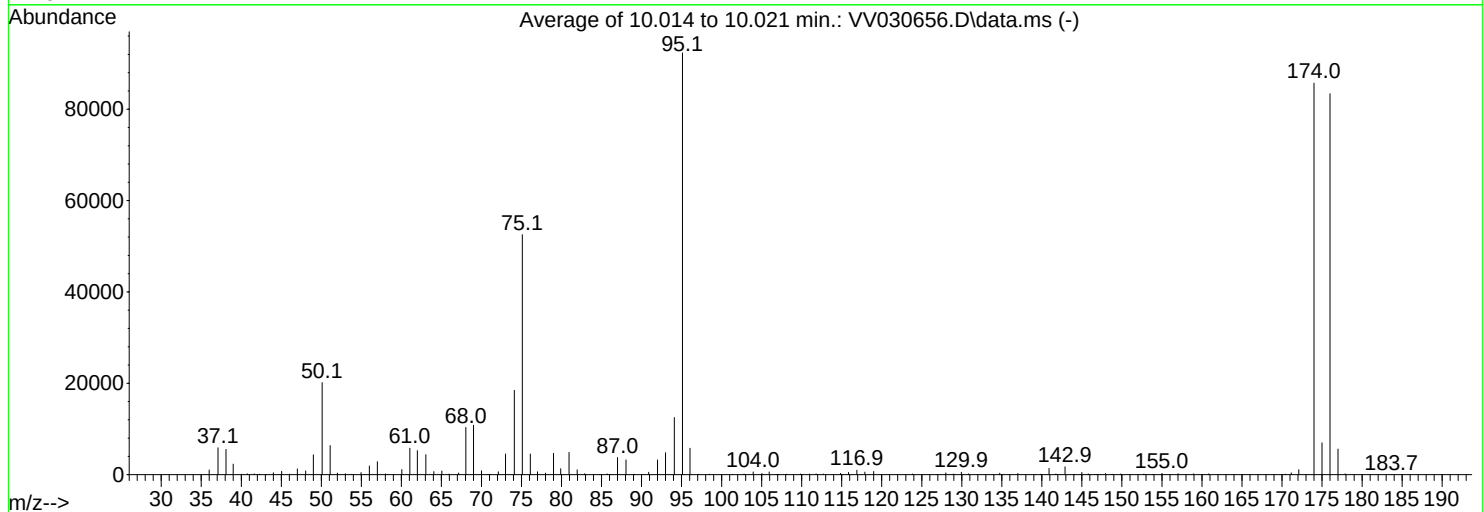


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV041923\
Data File : VV030656.D
Acq On : 19 Apr 2023 09:44
Operator : SY/MD
Sample : BFB368
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB368

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis
Last Update : Thu Apr 20 01:26:42 2023

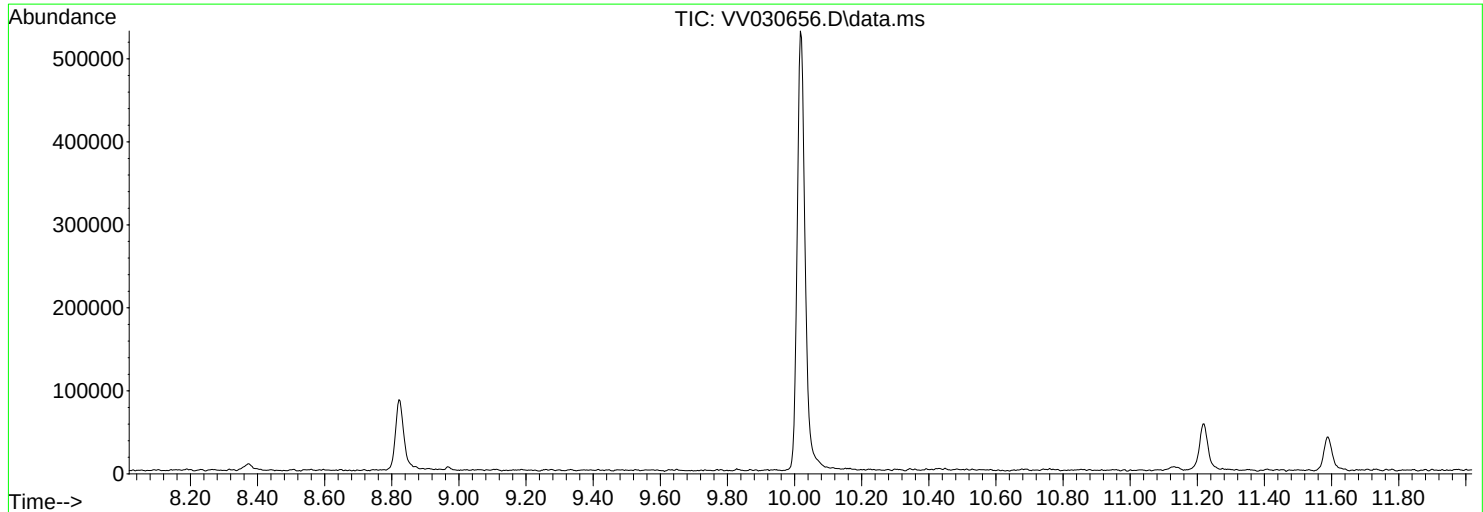

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	20131	PASS
75	95	30	80	56.9	52557	PASS
95	95	100	100	100.0	92341	PASS
96	95	5	9	6.2	5764	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.8	85720	PASS
175	174	5	9	8.1	6982	PASS
176	174	95	105	97.3	83400	PASS
177	176	5	10	6.7	5610	PASS

m/z	Abundance
35.90	140.0
36.70	115.0
37.70	150.0
39.10	168.0
40.00	211.0
41.30	114.0
42.00	202.0
43.00	167.0
43.90	277.0
44.20	297.0
45.10	225.0
46.20	130.0
46.70	118.0
48.50	146.0
49.70	164.0
50.80	131.0
53.70	146.0
54.50	117.0
55.40	105.0
56.10	123.0
57.70	142.0
59.50	107.0
62.20	125.0
65.10	122.0
67.30	112.0
68.60	186.0
69.90	108.0
71.10	116.0
71.80	105.0
73.00	132.0
81.70	108.0
97.10	110.0
120.10	127.0
132.60	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.10	1100.0
37.10	5772.0
38.10	5104.0
39.00	2481.0
40.00	264.0
40.70	150.0
41.70	158.0
42.30	124.0
43.00	172.0
44.00	1008.0
45.10	1038.0
46.00	239.0
47.00	1173.0
48.10	754.0
49.00	4171.0
50.10	19192.0
51.10	5974.0
52.00	370.0
53.00	236.0
53.90	190.0
54.90	522.0
56.00	1864.0
57.00	2785.0
58.00	176.0
59.20	115.0
60.10	1152.0
61.10	5235.0
62.00	5249.0
63.00	4271.0
64.00	556.0
65.00	898.0
66.10	155.0
67.10	461.0
68.10	9960.0
69.00	10524.0
70.00	957.0
72.10	541.0
73.00	4466.0
74.10	17416.0
75.10	49520.0
76.10	4146.0
77.00	691.0
78.00	355.0
79.00	4556.0
79.90	1248.0
80.90	4763.0
81.90	1012.0
82.90	159.0
85.70	164.0
87.00	3557.0
88.00	3122.0
89.10	144.0
90.90	451.0
92.00	3150.0
93.00	4630.0
94.10	11977.0
95.10	88848.0
96.10	5632.0
97.10	201.0
98.50	109.0
102.80	139.0
103.90	527.0
105.00	218.0
105.90	542.0
107.10	125.0
108.10	104.0
109.80	157.0
111.00	148.0
111.90	170.0
113.00	185.0
114.90	311.0
115.90	478.0
116.90	966.0
117.90	558.0
119.00	596.0
123.90	135.0
126.80	108.0
128.00	368.0
128.80	231.0
130.00	472.0
130.90	162.0
134.70	298.0
137.00	233.0
139.90	120.0
140.90	1330.0
141.80	162.0
142.90	1592.0
143.90	119.0
145.00	511.0
145.90	164.0
147.10	133.0
148.00	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

148.90	115.0
149.80	148.0
152.80	148.0
155.00	303.0
157.00	186.0
158.90	154.0
160.90	152.0
171.30	365.0
172.10	1094.0
174.00	80184.0
175.00	6650.0
176.00	77792.0
177.00	5283.0
177.90	156.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.10	1173.0
37.10	6160.0
38.10	5761.0
39.00	2600.0
40.00	298.0
40.70	168.0
41.60	177.0
42.30	116.0
43.00	177.0
44.00	1046.0
45.10	991.0
46.00	294.0
47.00	1289.0
48.00	838.0
49.00	4523.0
50.10	20896.0
51.10	6606.0
52.00	359.0
53.00	230.0
53.90	212.0
54.90	487.0
56.00	2095.0
57.00	2879.0
58.10	168.0
60.10	1139.0
61.00	5994.0
62.00	5551.0
63.00	4560.0
64.10	682.0
65.00	956.0
65.90	129.0
67.10	514.0
68.10	10694.0
69.00	11222.0
70.10	973.0
70.80	111.0
72.10	652.0
73.00	4807.0
74.10	19320.0
75.10	54360.0
76.10	4685.0
77.00	666.0
78.00	332.0
79.00	4809.0
79.90	1352.0
80.90	5042.0
82.00	1071.0
82.90	209.0
85.70	173.0
87.00	3883.0
88.10	3388.0
90.90	540.0
92.00	3311.0
93.00	5044.0
94.10	12814.0
95.10	95480.0
96.10	5949.0
97.10	194.0
98.50	106.0
102.80	134.0
103.90	618.0
105.00	255.0
105.90	602.0
108.20	104.0
109.90	152.0
111.00	160.0
111.80	167.0
112.70	207.0
114.90	269.0
115.80	505.0
116.90	1042.0
117.90	565.0
119.00	724.0
123.90	123.0
128.00	392.0
129.00	234.0
129.90	519.0
130.80	178.0
134.70	341.0
137.00	226.0
139.90	118.0
140.90	1442.0
141.70	175.0
142.90	1739.0
144.10	110.0
145.00	500.0
145.70	189.0
146.60	117.0
147.00	110.0
147.90	253.0
148.80	124.0
149.80	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

152.80	158.0
153.80	124.0
155.00	302.0
157.00	213.0
159.00	180.0
160.80	173.0
170.40	143.0
171.10	399.0
172.10	1115.0
174.00	88552.0
175.00	7241.0
176.00	86176.0
177.00	5803.0
177.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

m/z	Abundance
36.00	1170.0
37.10	5745.0
38.10	5706.0
39.00	2342.0
40.00	386.0
40.80	177.0
41.50	176.0
42.30	108.0
43.00	166.0
44.00	979.0
45.00	868.0
46.00	325.0
47.00	1300.0
48.00	825.0
49.00	4364.0
50.10	20304.0
51.10	6554.0
52.00	354.0
53.00	182.0
53.90	237.0
55.00	415.0
56.00	2130.0
57.00	2807.0
57.90	141.0
58.30	155.0
60.00	1071.0
61.00	6063.0
62.00	5366.0
63.10	4362.0
64.10	765.0
65.10	961.0
65.80	128.0
67.20	442.0
68.00	10330.0
69.00	10707.0
70.10	889.0
71.00	106.0
72.10	690.0
73.00	4738.0
74.10	18696.0
75.10	53792.0
76.10	4729.0
77.00	587.0
78.00	349.0
79.00	4663.0
79.90	1304.0
81.00	4850.0
82.00	1067.0
82.90	230.0
84.80	130.0
85.70	174.0
87.00	3861.0
88.00	3192.0
90.90	556.0
92.00	3193.0
93.00	4711.0
94.10	12710.0
95.10	92696.0
96.00	5711.0
97.10	194.0
98.40	101.0
101.40	111.0
102.80	117.0
104.00	633.0
105.10	307.0
106.00	604.0
106.80	142.0
108.20	103.0
109.80	149.0
111.00	153.0
111.70	144.0
112.70	214.0
114.80	229.0
115.80	519.0
116.90	963.0
117.90	529.0
119.00	800.0
123.70	113.0
128.00	423.0
129.00	238.0
129.90	548.0
130.80	211.0
134.80	344.0
137.00	237.0
139.20	123.0
139.80	131.0
140.90	1374.0
141.80	179.0
142.90	1801.0
144.10	121.0
145.00	428.0
145.80	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368

146.80	128.0
147.90	274.0
148.70	121.0
149.90	131.0
152.70	137.0
153.80	132.0
155.00	263.0
157.00	248.0
159.00	169.0
160.80	217.0
170.50	151.0
171.10	364.0
172.10	1086.0
174.00	88424.0
175.00	7055.0
176.00	86232.0
177.00	5743.0
177.90	174.0
183.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB368