

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042020\
 Data File : VV015578.D
 Acq On : 20 Apr 2020 13:22
 Operator : SY/MD
 Sample : L2333-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC9

Quant Time: Apr 21 01:25:27 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 21 00:05:52 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	94400	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	88613	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	41985	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	20337	4.15	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.00%
7) Chloroethane-d5	1.58	69	21076	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.40%
11) 1,1-Dichloroethene-d2	2.12	63	29646	2.87	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.40%#
20) 2-Butanone-d5	3.94	46	74327	54.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.08%
24) Chloroform-d	4.38	84	51219	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	5.06	65	29743	5.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.80%
32) Benzene-d6	5.08	84	94978	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.10	67	30536	4.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.80%
41) Toluene-d8	7.34	98	84291	4.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.80%
43) trans-1,3-Dichloropropene-	7.65	79	7724	2.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.00%
46) 2-Hexanone-d5	8.11	63	53262	41.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.94%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	22263	4.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.60%
64) 1,2-Dichlorobenzene-d4	11.65	152	32047	4.76	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.20%


Target Compounds					Ovalue
13) Acetone	2.22	43	4015	4.132 ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042020\
Data File : VV015578.D
Acq On : 20 Apr 2020 13:22
Operator : SY/MD
Sample : L2333-17
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC9

Quant Time: Apr 21 01:25:27 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR040920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 21 00:05:52 2020
Response via : Initial Calibration

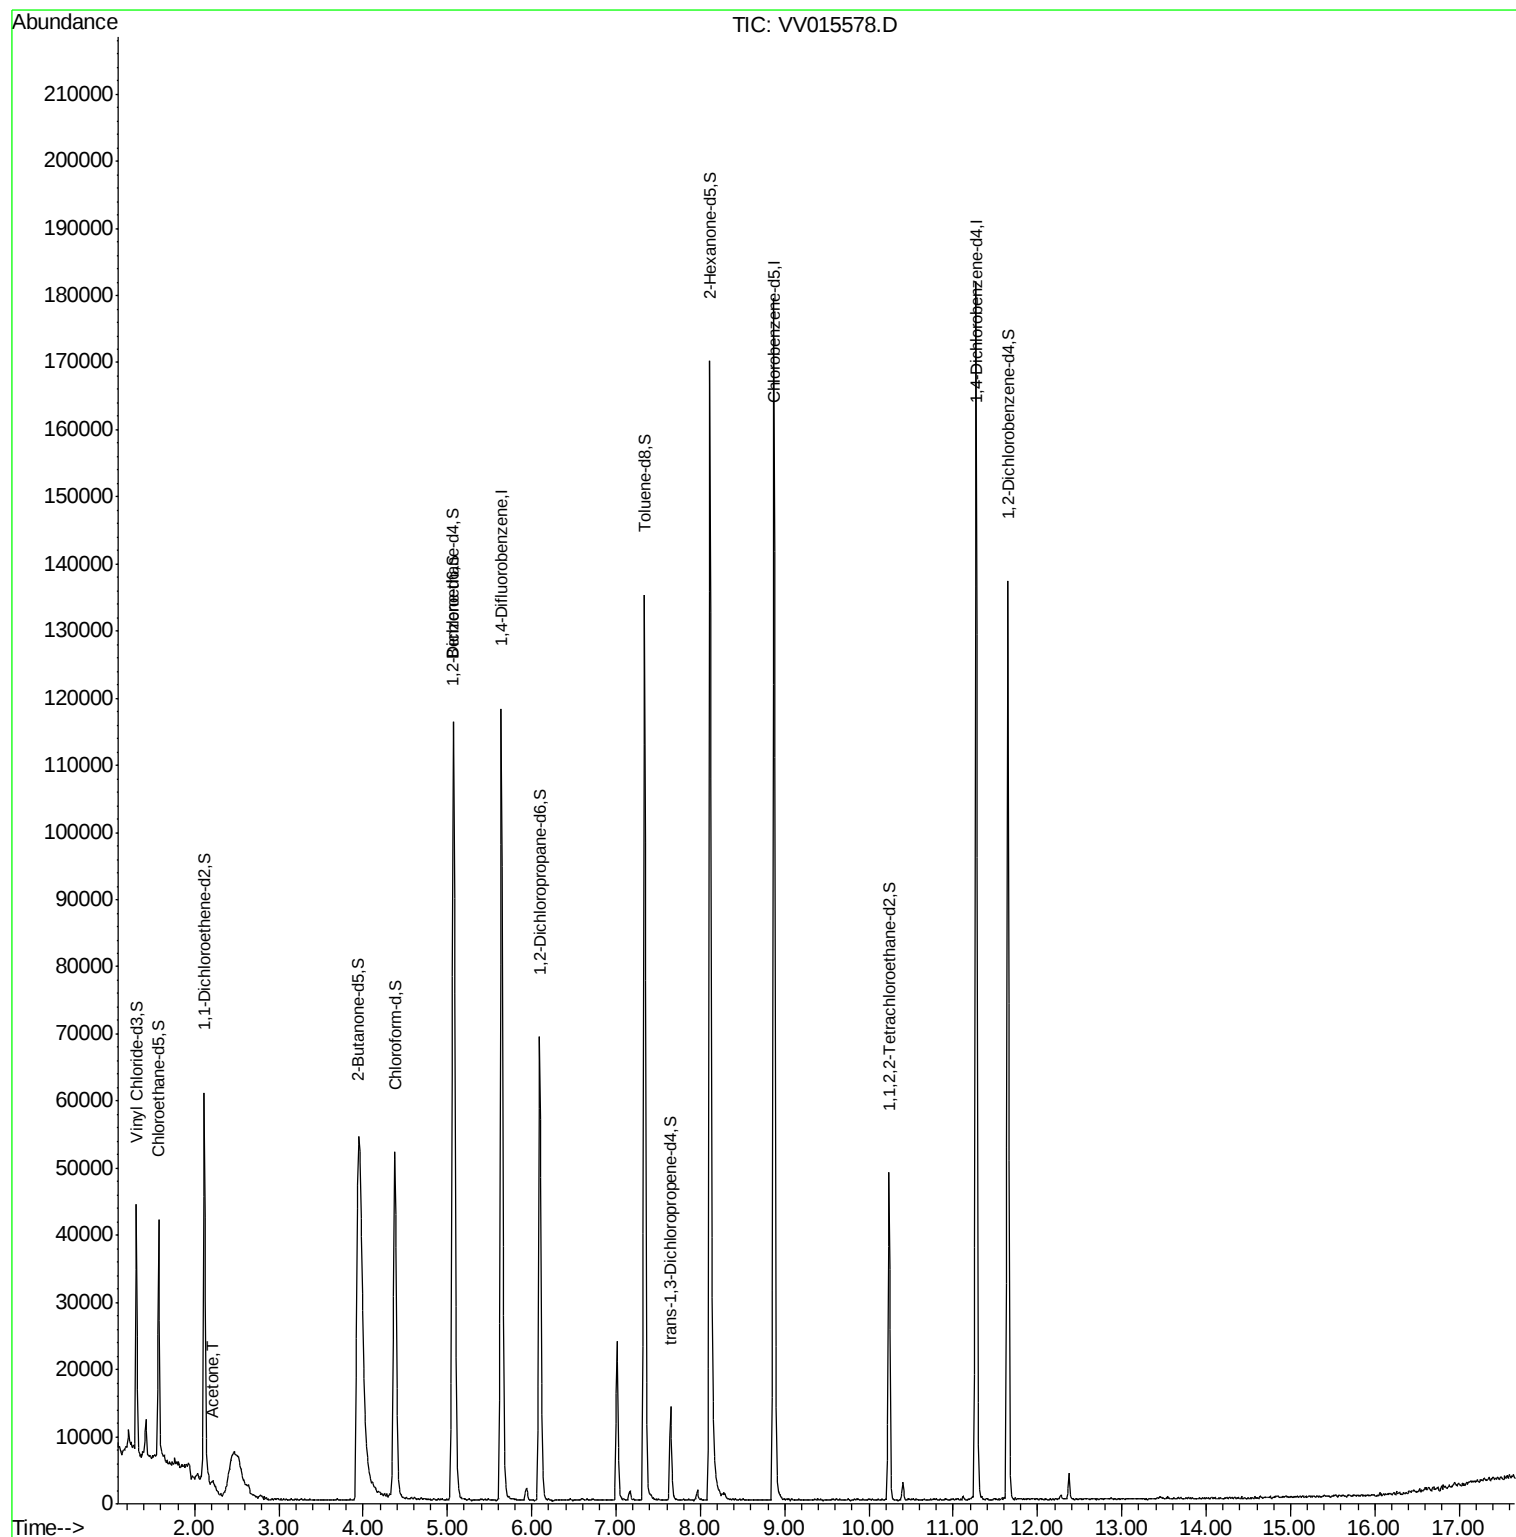

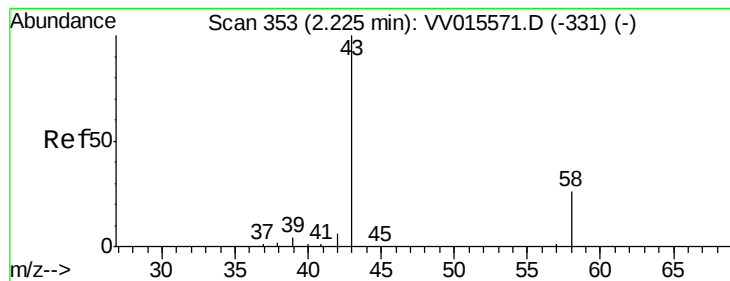

#13

Acetone

Concen: 4.132 ug/L

RT: 2.22 min Scan# 351

Delta R.T. -0.01 min

Lab File: VV015578.D

Acq: 20 Apr 2020 13:22

Instrument :
MSVOA_V
ClientSampleId :
C0AC9

Tot Ion: 43 Resp: 4015

Ion Ratio Lower Upper

43 100

58 20.9 0.0 22.2

