
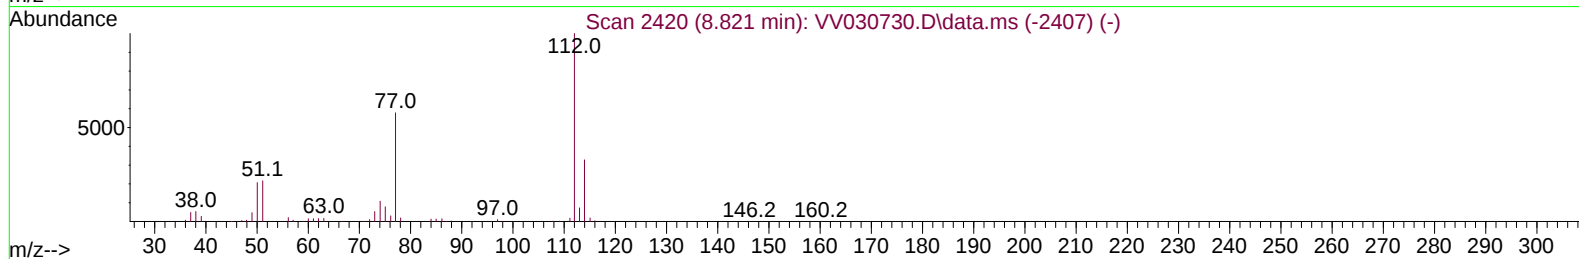
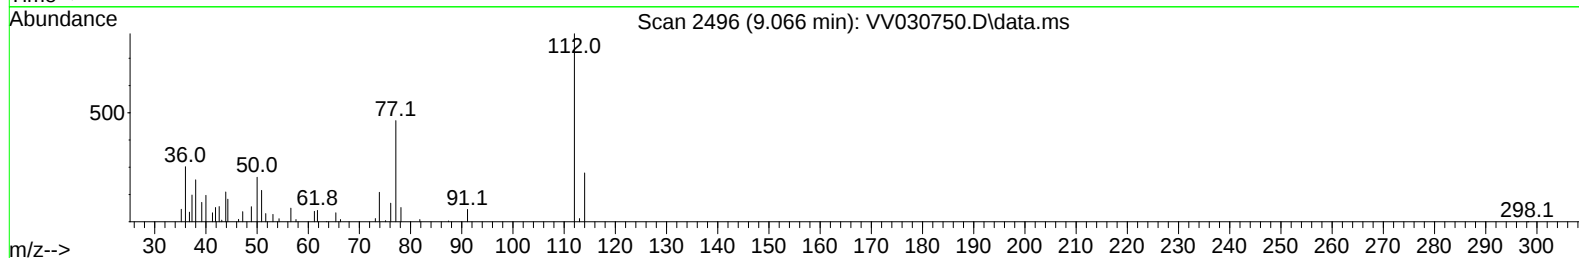


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030750.D
Acq On : 21 Apr 2023 04:52
Operator : SY/MD
Sample : 02398-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Apr 21 06:16:22 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

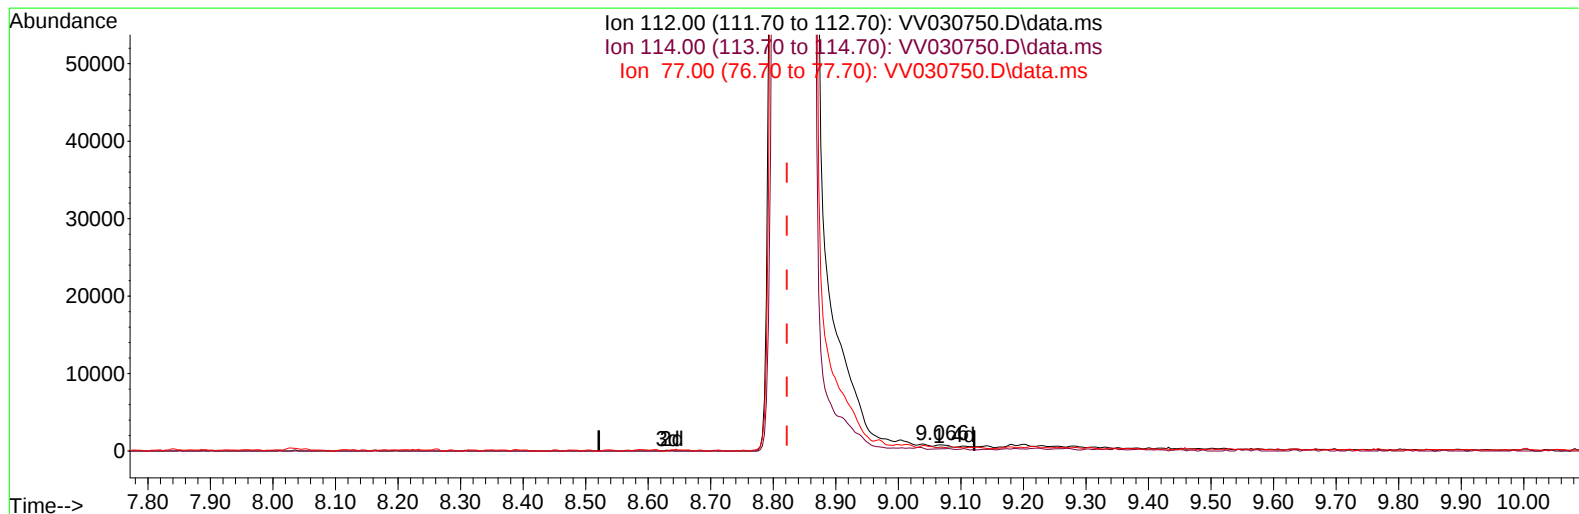

TIC: VV030750.D\data.ms

(51) Chlorobenzene (T)

9.066min (+ 0.244) 0.08 ug/L

response 431

Ion	Exp%	Act%
112.00	100.00	100.00
114.00	32.00	35.32
77.00	59.20	59.62
0.00	0.00	0.00