

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030729.D
 Acq On : 20 Apr 2023 20:06
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 21 00:21:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	195854	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	191676	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	92909	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	74624	51.975	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 103.960%	
7) Chloroethane-d5	1.539	69	65467	54.412	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 108.820%	
11) 1,1-Dichloroethene-d2	2.066	65	36067	52.971	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 105.940%	
21) 2-Butanone-d5	3.802	46	85100	107.912	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 107.910%	
24) Chloroform-d	4.259	84	132353	50.867	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 101.740%	
26) 1,2-Dichloroethane-d4	4.953	65	94465	56.470	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 112.940%	
32) Benzene-d6	4.969	84	248352	54.802	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 109.600%	
36) 1,2-Dichloropropane-d6	5.998	67	74811	53.145	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 106.280%	
41) Toluene-d8	7.252	98	219689	51.632	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 103.260%	
43) trans-1,3-Dichloroprop...	7.561	79	37515	52.875	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 105.760%	
47) 2-Hexanone-d5	8.034	63	54241	97.812	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 97.810%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	105895	51.843	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 103.680%	
66) 1,2-Dichlorobenzene-d4	11.570	152	88944	60.229	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 120.460%#	
Target Compounds						
44) trans-1,3-Dichloropropene	7.558	75	1732	0.750	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030729.D
Acq On : 20 Apr 2023 20:06
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 21 00:21:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 00:14:50 2023
Response via : Initial Calibration

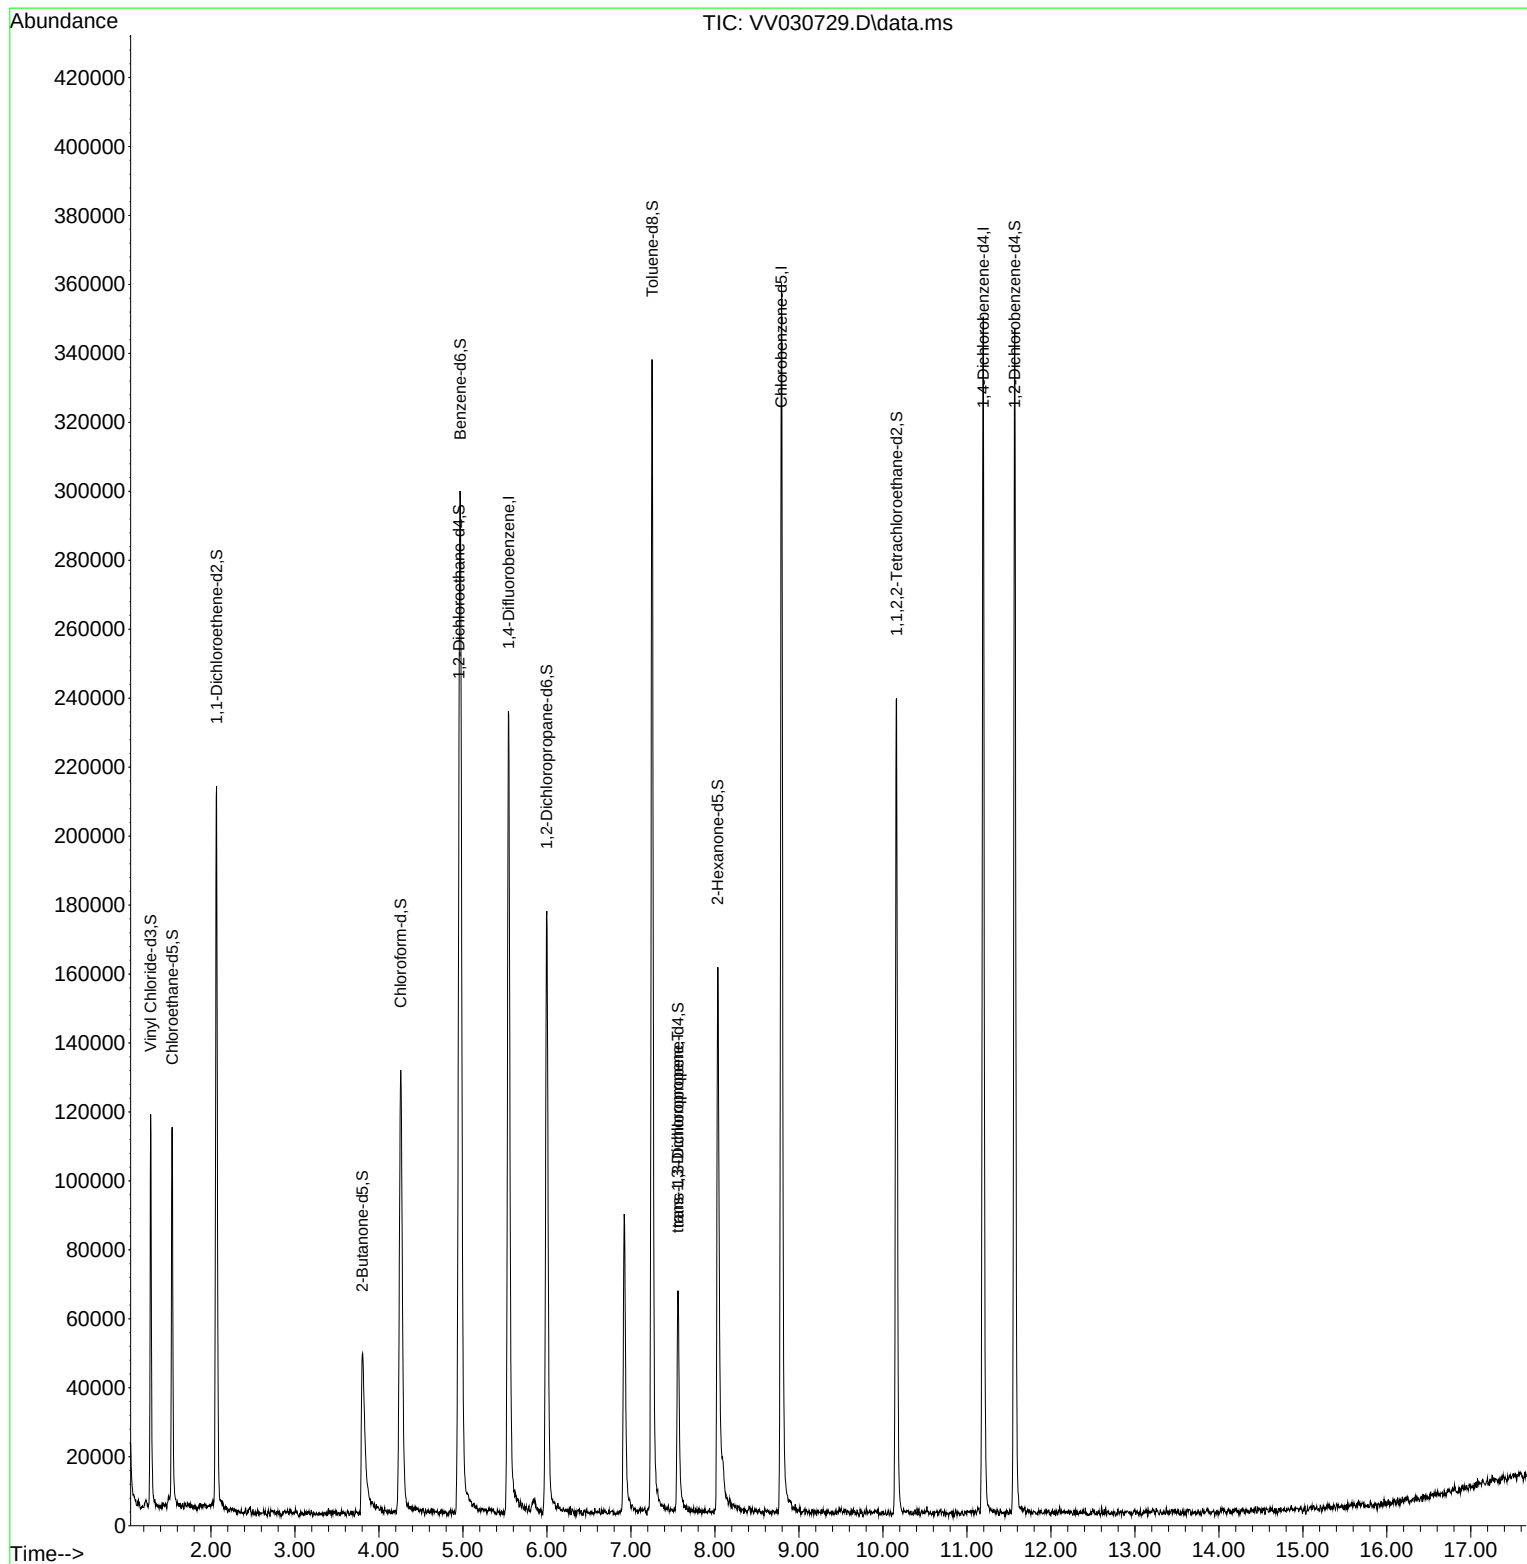

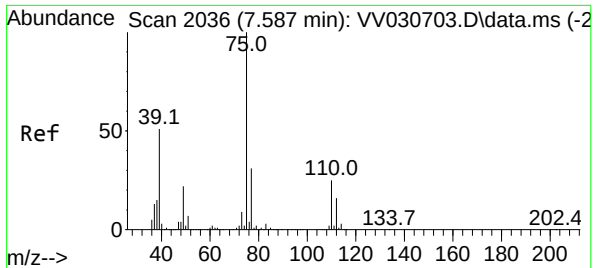

#44
 trans-1,3-Dichloropropene
 Concen: 0.750 ug/L
 RT: 7.558 min Scan# 20
 Delta R.T. -0.029 min
 Lab File: VV030729.D
 Acq: 20 Apr 2023 20:06

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 1732
 Ion Ratio Lower Upper
 75 100
 77 34.6 22.1 41.1

