

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030735.D
 Acq On : 20 Apr 2023 22:52
 Operator : SY/MD
 Sample : 02440-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Quant Time: Apr 21 06:13:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	230875	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	222278	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	107822	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	72855	43.046	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	86.100%
7) Chloroethane-d5	1.535	69	60775	42.850	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.700%
11) 1,1-Dichloroethene-d2	2.063	65	34989	43.593	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.180%
21) 2-Butanone-d5	3.796	46	89313	96.075	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	96.080%
24) Chloroform-d	4.259	84	135381	44.138	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.280%
26) 1,2-Dichloroethane-d4	4.950	65	96104	48.735	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.480%
32) Benzene-d6	4.969	84	249515	47.479	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.960%
36) 1,2-Dichloropropane-d6	5.995	67	76221	46.692	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.380%
41) Toluene-d8	7.252	98	218999	44.384	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.760%
43) trans-1,3-Dichloroprop...	7.561	79	36751	44.667	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.340%
47) 2-Hexanone-d5	8.034	63	55079	85.649	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.650%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	106081	44.784	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.560%
66) 1,2-Dichlorobenzene-d4	11.570	152	89810	52.404	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.800%
Target Compounds						
44) trans-1,3-Dichloropropene	7.567	75	2024	0.756	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030735.D
Acq On : 20 Apr 2023 22:52
Operator : SY/MD
Sample : 02440-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Time: Apr 21 06:13:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

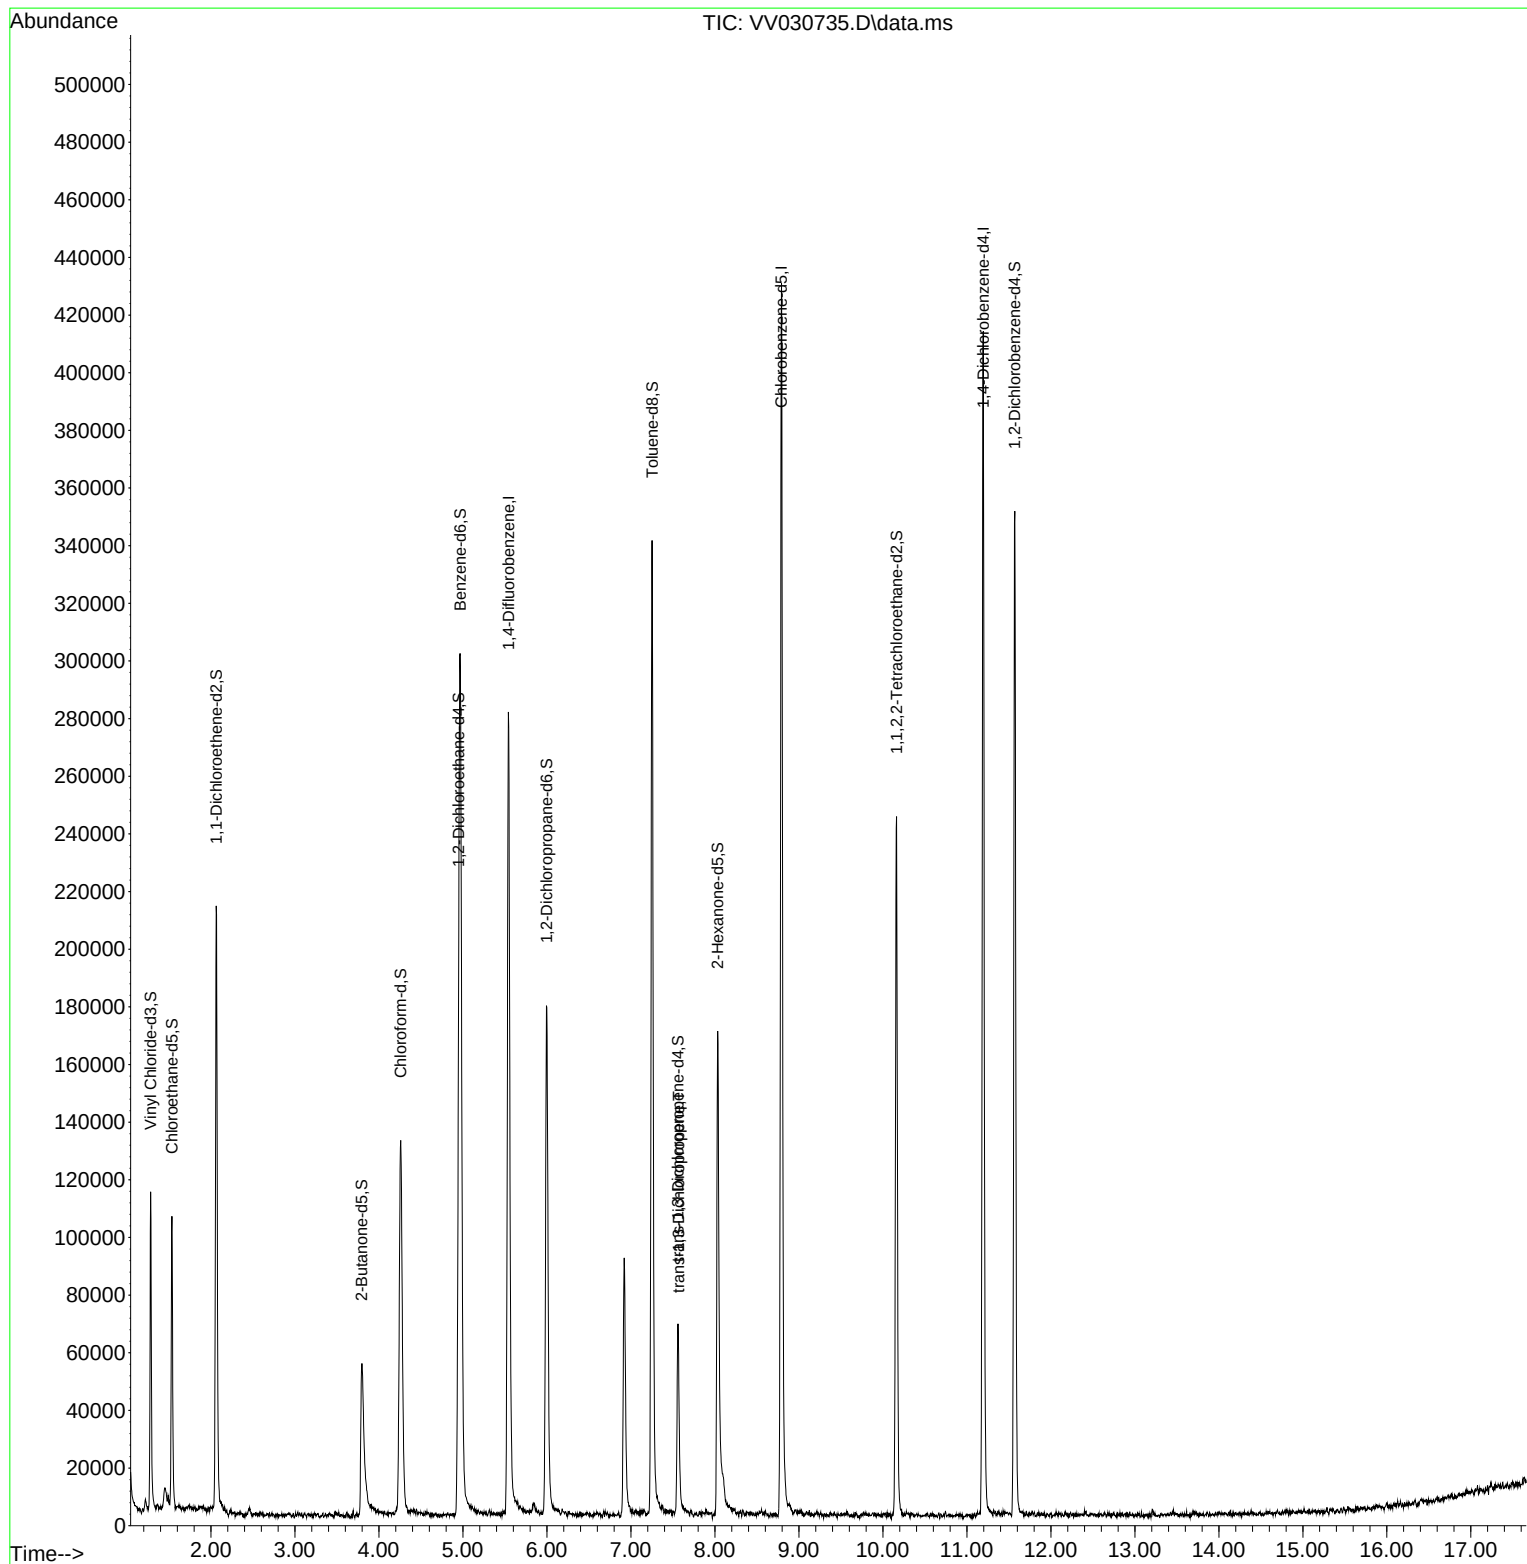

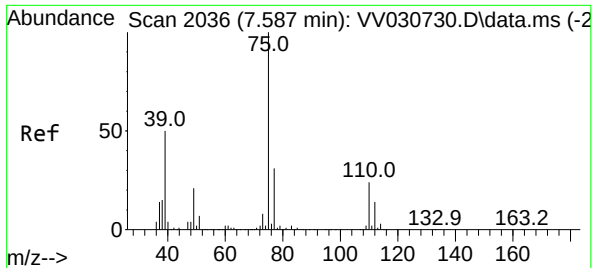

#44
 trans-1,3-Dichloropropene
 Concen: 0.756 ug/L
 RT: 7.567 min Scan# 2030
 Delta R.T. -0.019 min
 Lab File: VV030735.D
 Acq: 20 Apr 2023 22:52

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Tgt Ion: 75 Resp: 2024
 Ion Ratio Lower Upper
 75 100
 77 48.6 22.1 41.1#

