

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030737.D
 Acq On : 20 Apr 2023 23:40
 Operator : SY/MD
 Sample : 02440-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ1

Quant Time: Apr 21 06:13:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	226629	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	216651	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	105492	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	67929	40.887	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.780%		
7) Chloroethane-d5	1.535	69	56111	40.303	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	80.600%		
11) 1,1-Dichloroethene-d2	2.063	65	33962	43.106	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.220%		
21) 2-Butanone-d5	3.796	46	85447	93.638	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.640%		
24) Chloroform-d	4.259	84	128498	42.679	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.360%		
26) 1,2-Dichloroethane-d4	4.950	65	91794	47.422	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.840%		
32) Benzene-d6	4.969	84	234956	45.870	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.740%		
36) 1,2-Dichloropropane-d6	5.998	67	72673	45.675	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.340%		
41) Toluene-d8	7.252	98	205698	42.771	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.540%		
43) trans-1,3-Dichloroprop...	7.561	79	35000	43.644	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.280%		
47) 2-Hexanone-d5	8.034	63	54214	86.494	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.490%		
56) 1,1,2,2-Tetrachloroeth...	10.162	84	101138	43.806	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.620%		
66) 1,2-Dichlorobenzene-d4	11.570	152	85828	51.187	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.380%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	1925	0.737	ug/L	# 53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030737.D
Acq On : 20 Apr 2023 23:40
Operator : SY/MD
Sample : 02440-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ1

Quant Time: Apr 21 06:13:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

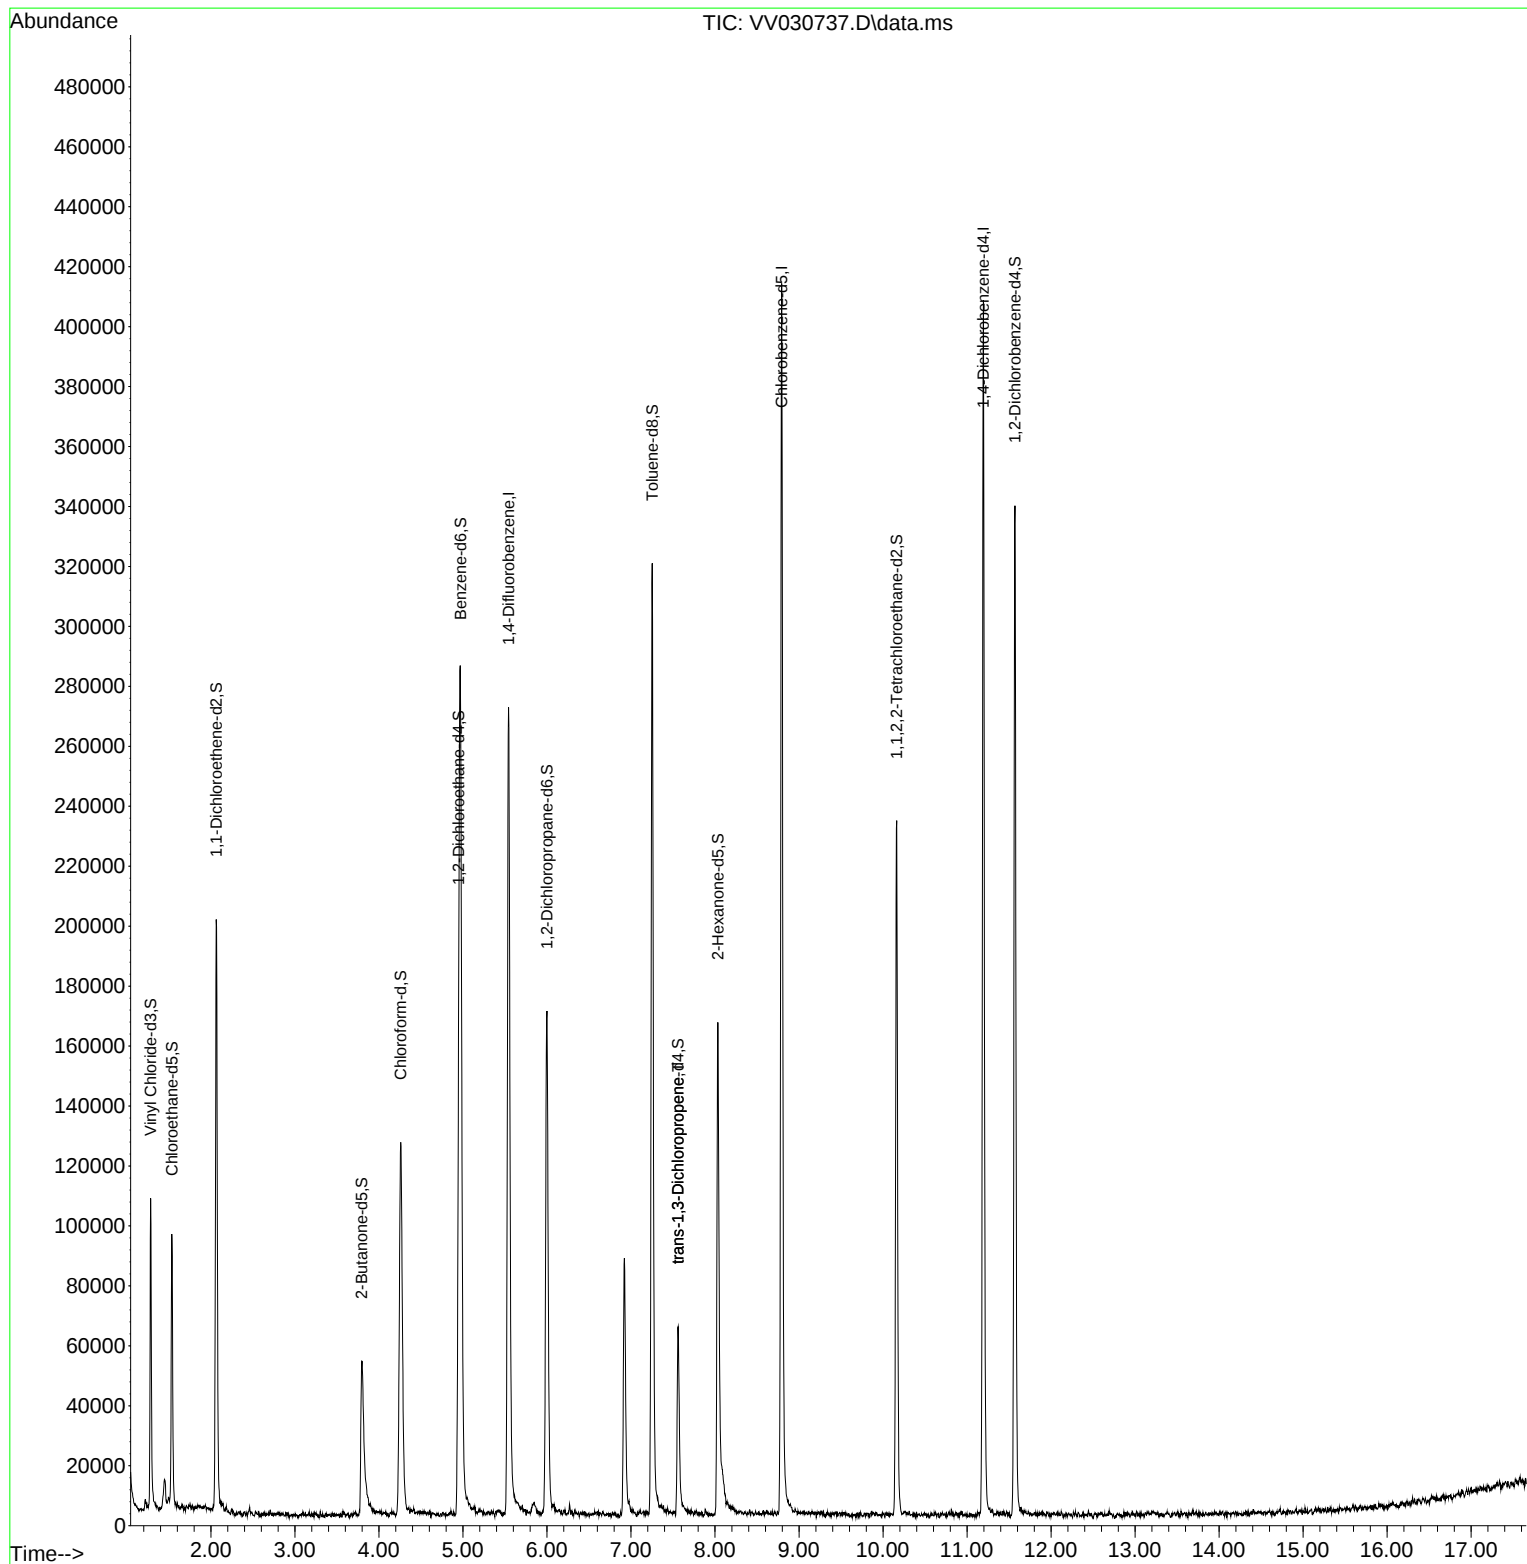

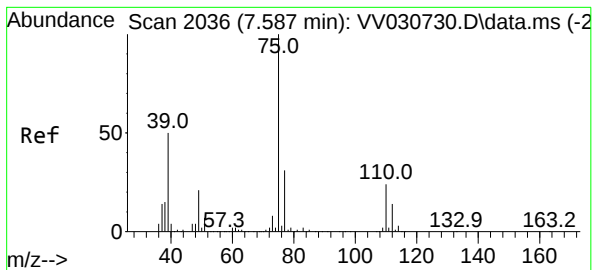

#44
 trans-1,3-Dichloropropene
 Concen: 0.737 ug/L
 RT: 7.561 min Scan# 2036
 Delta R.T. -0.026 min
 Lab File: VV030737.D
 Acq: 20 Apr 2023 23:40

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ1

Tgt Ion: 75 Resp: 1925
 Ion Ratio Lower Upper
 75 100
 77 57.4 22.1 41.1#

