

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030738.D
 Acq On : 21 Apr 2023 00:04
 Operator : SY/MD
 Sample : 02440-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ2

Quant Time: Apr 21 06:13:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	233676	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	226886	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108433	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	69561	40.607	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.220%
7) Chloroethane-d5	1.536	69	56400	39.289	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.580%
11) 1,1-Dichloroethene-d2	2.063	65	33988	41.838	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.680%
21) 2-Butanone-d5	3.796	46	86256	91.674	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.670%
24) Chloroform-d	4.259	84	127145	40.956	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.920%
26) 1,2-Dichloroethane-d4	4.950	65	89635	44.910	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.820%
32) Benzene-d6	4.970	84	237928	44.355	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.700%
36) 1,2-Dichloropropane-d6	5.998	67	71874	43.135	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.260%
41) Toluene-d8	7.252	98	204609	40.625	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.260%
43) trans-1,3-Dichloroprop...	7.561	79	34148	40.661	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.320%
47) 2-Hexanone-d5	8.034	63	53227	81.088	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.090%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	100420	41.533	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.060%
66) 1,2-Dichlorobenzene-d4	11.571	152	83636	48.527	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.060%
Target Compounds						
					Qvalue	
44) trans-1,3-Dichloropropene	7.561	75	2154	0.788	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030738.D
Acq On : 21 Apr 2023 00:04
Operator : SY/MD
Sample : 02440-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ2

Quant Time: Apr 21 06:13:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

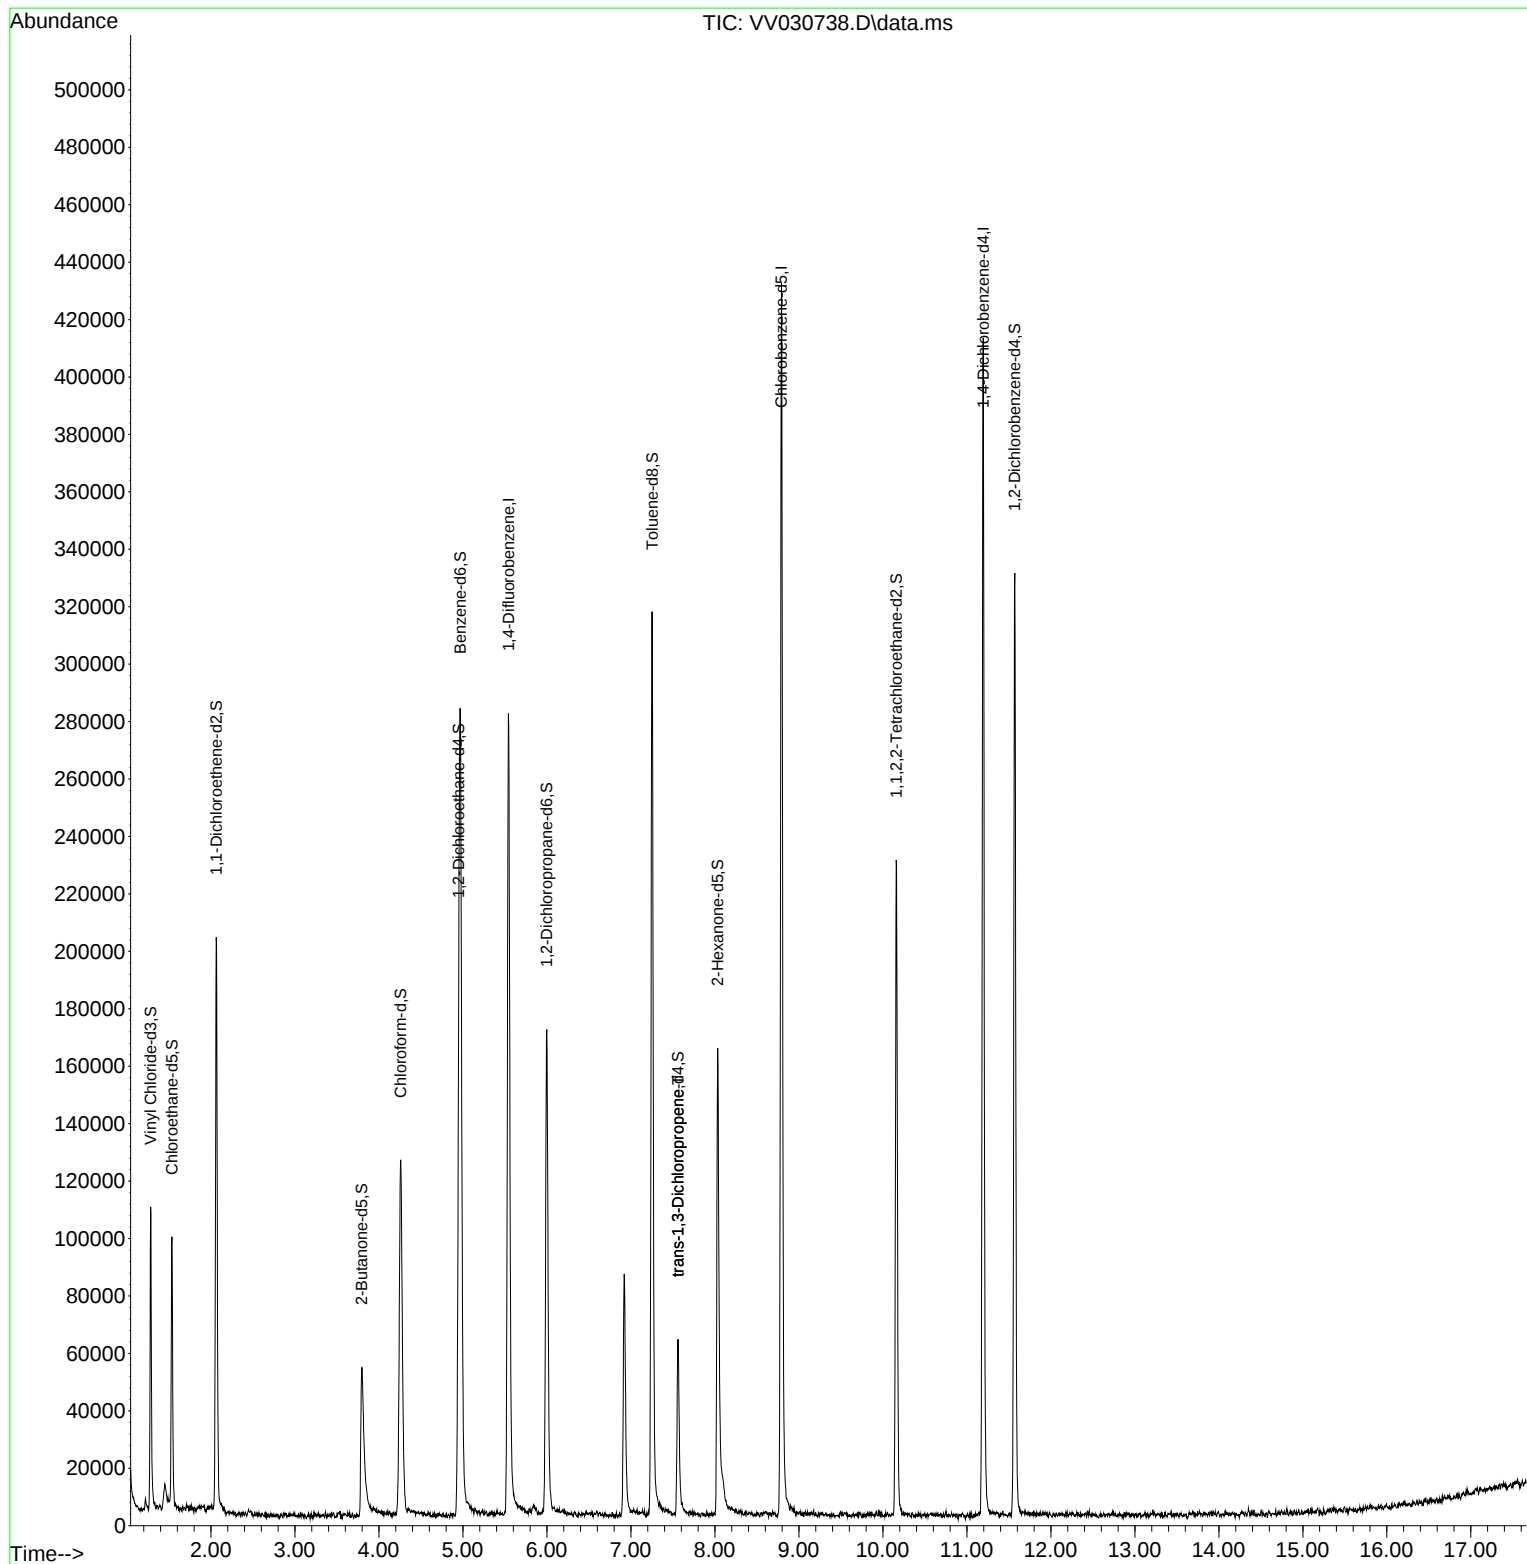

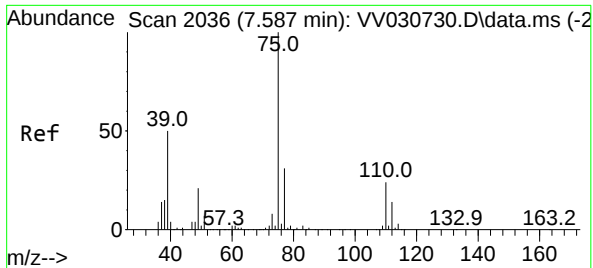

#44
 trans-1,3-Dichloropropene
 Concen: 0.788 ug/L
 RT: 7.561 min Scan# 2036
 Delta R.T. -0.026 min
 Lab File: VV030738.D
 Acq: 21 Apr 2023 00:04

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ2

Tgt Ion: 75 Resp: 2154
 Ion Ratio Lower Upper
 75 100
 77 49.8 22.1 41.1#

