

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030739.D
 Acq On : 21 Apr 2023 00:28
 Operator : SY/MD
 Sample : 02440-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ3

Quant Time: Apr 21 06:14:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	232165	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	225575	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	110361	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	69015	40.550	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.100%
7) Chloroethane-d5	1.536	69	55936	39.220	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.440%
11) 1,1-Dichloroethene-d2	2.063	65	33595	41.623	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.240%
21) 2-Butanone-d5	3.796	46	83601	89.431	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.430%
24) Chloroform-d	4.259	84	126323	40.956	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.920%
26) 1,2-Dichloroethane-d4	4.950	65	86685	43.715	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.420%
32) Benzene-d6	4.969	84	234152	43.904	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.800%
36) 1,2-Dichloropropane-d6	5.995	67	72236	43.604	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.200%
41) Toluene-d8	7.252	98	205808	41.101	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	7.561	79	33903	40.603	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.200%
47) 2-Hexanone-d5	8.030	63	51987	79.659	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.660%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	99830	41.529	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.060%
66) 1,2-Dichlorobenzene-d4	11.570	152	83053	47.347	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.700%
Target Compounds						
44) trans-1,3-Dichloropropene	7.555	75	2073	0.763	ug/L	Qvalue # 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030739.D
Acq On : 21 Apr 2023 00:28
Operator : SY/MD
Sample : 02440-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ3

Quant Time: Apr 21 06:14:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

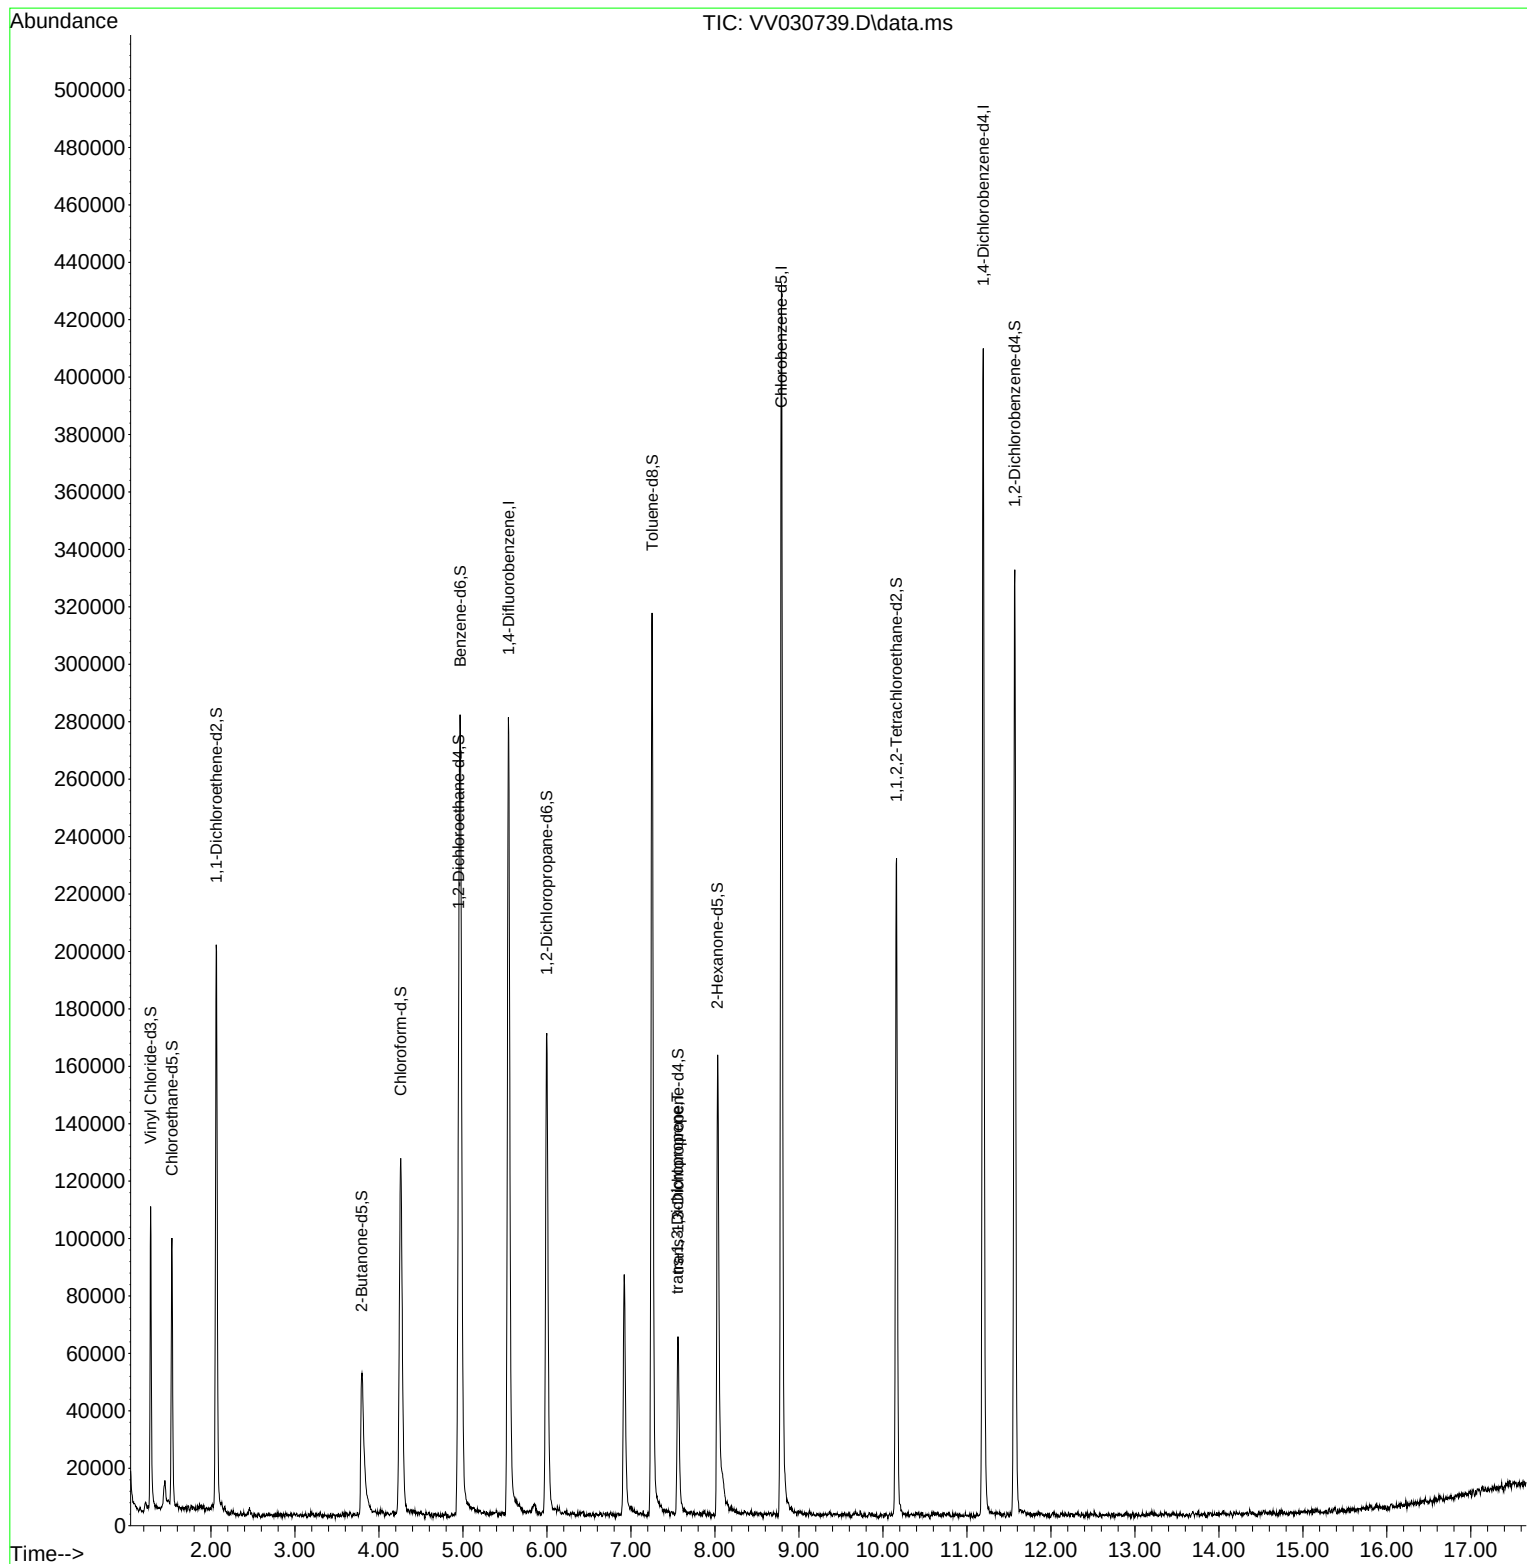

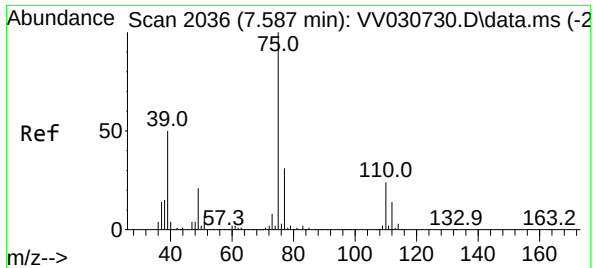

#44
 trans-1,3-Dichloropropene
 Concen: 0.763 ug/L
 RT: 7.555 min Scan# 20
 Delta R.T. -0.032 min
 Lab File: VV030739.D
 Acq: 21 Apr 2023 00:28

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ3

Tgt Ion: 75 Resp: 2073
 Ion Ratio Lower Upper
 75 100
 77 42.7 22.1 41.1#

