

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030742.D
 Acq On : 21 Apr 2023 01:40
 Operator : SY/MD
 Sample : 02440-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ6

Quant Time: Apr 21 06:14:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	230361	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	221703	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	106674	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	68318	40.455	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.920%		
7) Chloroethane-d5	1.535	69	55996	39.569	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.140%		
11) 1,1-Dichloroethene-d2	2.066	65	34002	42.458	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.920%		
21) 2-Butanone-d5	3.799	46	85884	92.593	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	92.590%		
24) Chloroform-d	4.259	84	128873	42.110	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.220%		
26) 1,2-Dichloroethane-d4	4.950	65	90814	46.155	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.320%		
32) Benzene-d6	4.969	84	235695	44.965	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.940%		
36) 1,2-Dichloropropane-d6	5.995	67	72440	44.491	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.980%		
41) Toluene-d8	7.252	98	208256	42.316	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.640%		
43) trans-1,3-Dichloroprop...	7.561	79	33997	41.427	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.860%		
47) 2-Hexanone-d5	8.033	63	53599	83.564	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.560%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	101989	43.168	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.340%		
66) 1,2-Dichlorobenzene-d4	11.570	152	83376	49.174	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.340%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	1999	0.748	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030742.D
Acq On : 21 Apr 2023 01:40
Operator : SY/MD
Sample : 02440-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ6

Quant Time: Apr 21 06:14:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

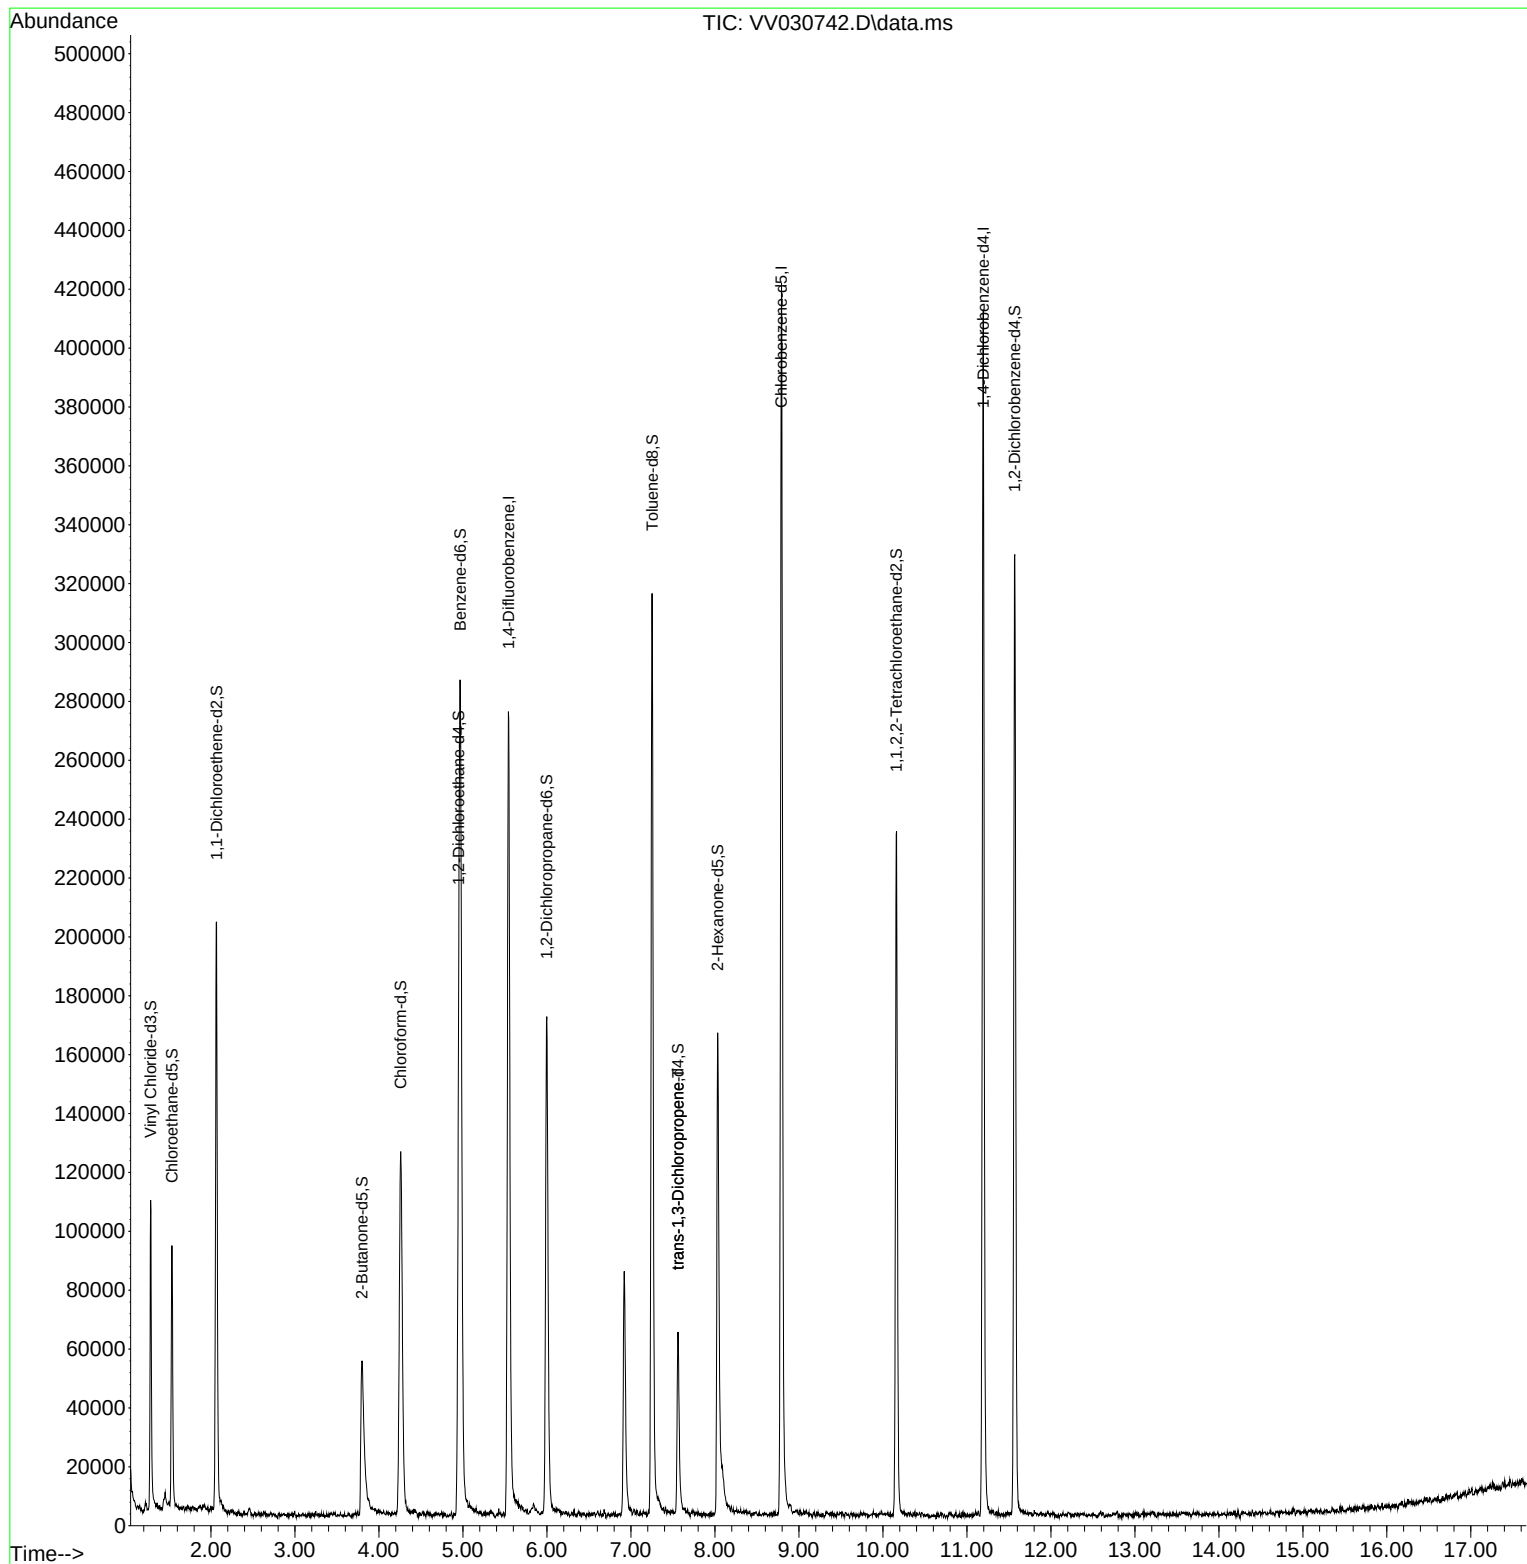

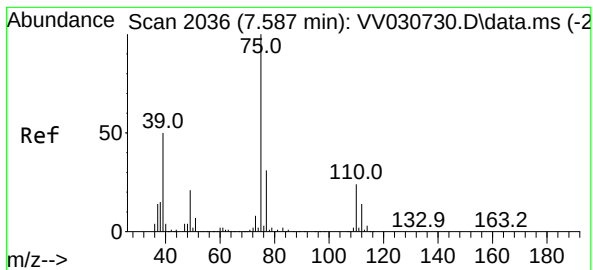

#44
 trans-1,3-Dichloropropene
 Concen: 0.748 ug/L
 RT: 7.561 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV030742.D
 Acq: 21 Apr 2023 01:40

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ6

Tgt Ion: 75 Resp: 1999
 Ion Ratio Lower Upper
 75 100
 77 43.6 22.1 41.1#

