

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030745.D
 Acq On : 21 Apr 2023 02:53
 Operator : SY/MD
 Sample : 02440-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ9

Quant Time: Apr 21 06:15:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 01:37:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	229863	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	222751	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108437	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	67113	39.828	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.660%
7) Chloroethane-d5	1.535	69	56905	40.299	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	2.063	65	33546	41.979	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.960%
21) 2-Butanone-d5	3.796	46	87554	94.598	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.600%
24) Chloroform-d	4.259	84	127004	41.589	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.180%
26) 1,2-Dichloroethane-d4	4.950	65	90296	45.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.980%
32) Benzene-d6	4.969	84	234571	44.540	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.080%
36) 1,2-Dichloropropane-d6	5.995	67	71244	43.550	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.100%
41) Toluene-d8	7.252	98	202595	40.972	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.940%
43) trans-1,3-Dichloroprop...	7.561	79	32461	39.369	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.740%
47) 2-Hexanone-d5	8.034	63	54182	84.075	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	84.080%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	99244	41.809	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.620%
66) 1,2-Dichlorobenzene-d4	11.570	152	84207	48.856	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.720%
Target Compounds						
44) trans-1,3-Dichloropropene	7.561	75	2046	0.762	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030745.D
Acq On : 21 Apr 2023 02:53
Operator : SY/MD
Sample : 02440-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ9

Quant Time: Apr 21 06:15:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 01:37:39 2023
Response via : Initial Calibration

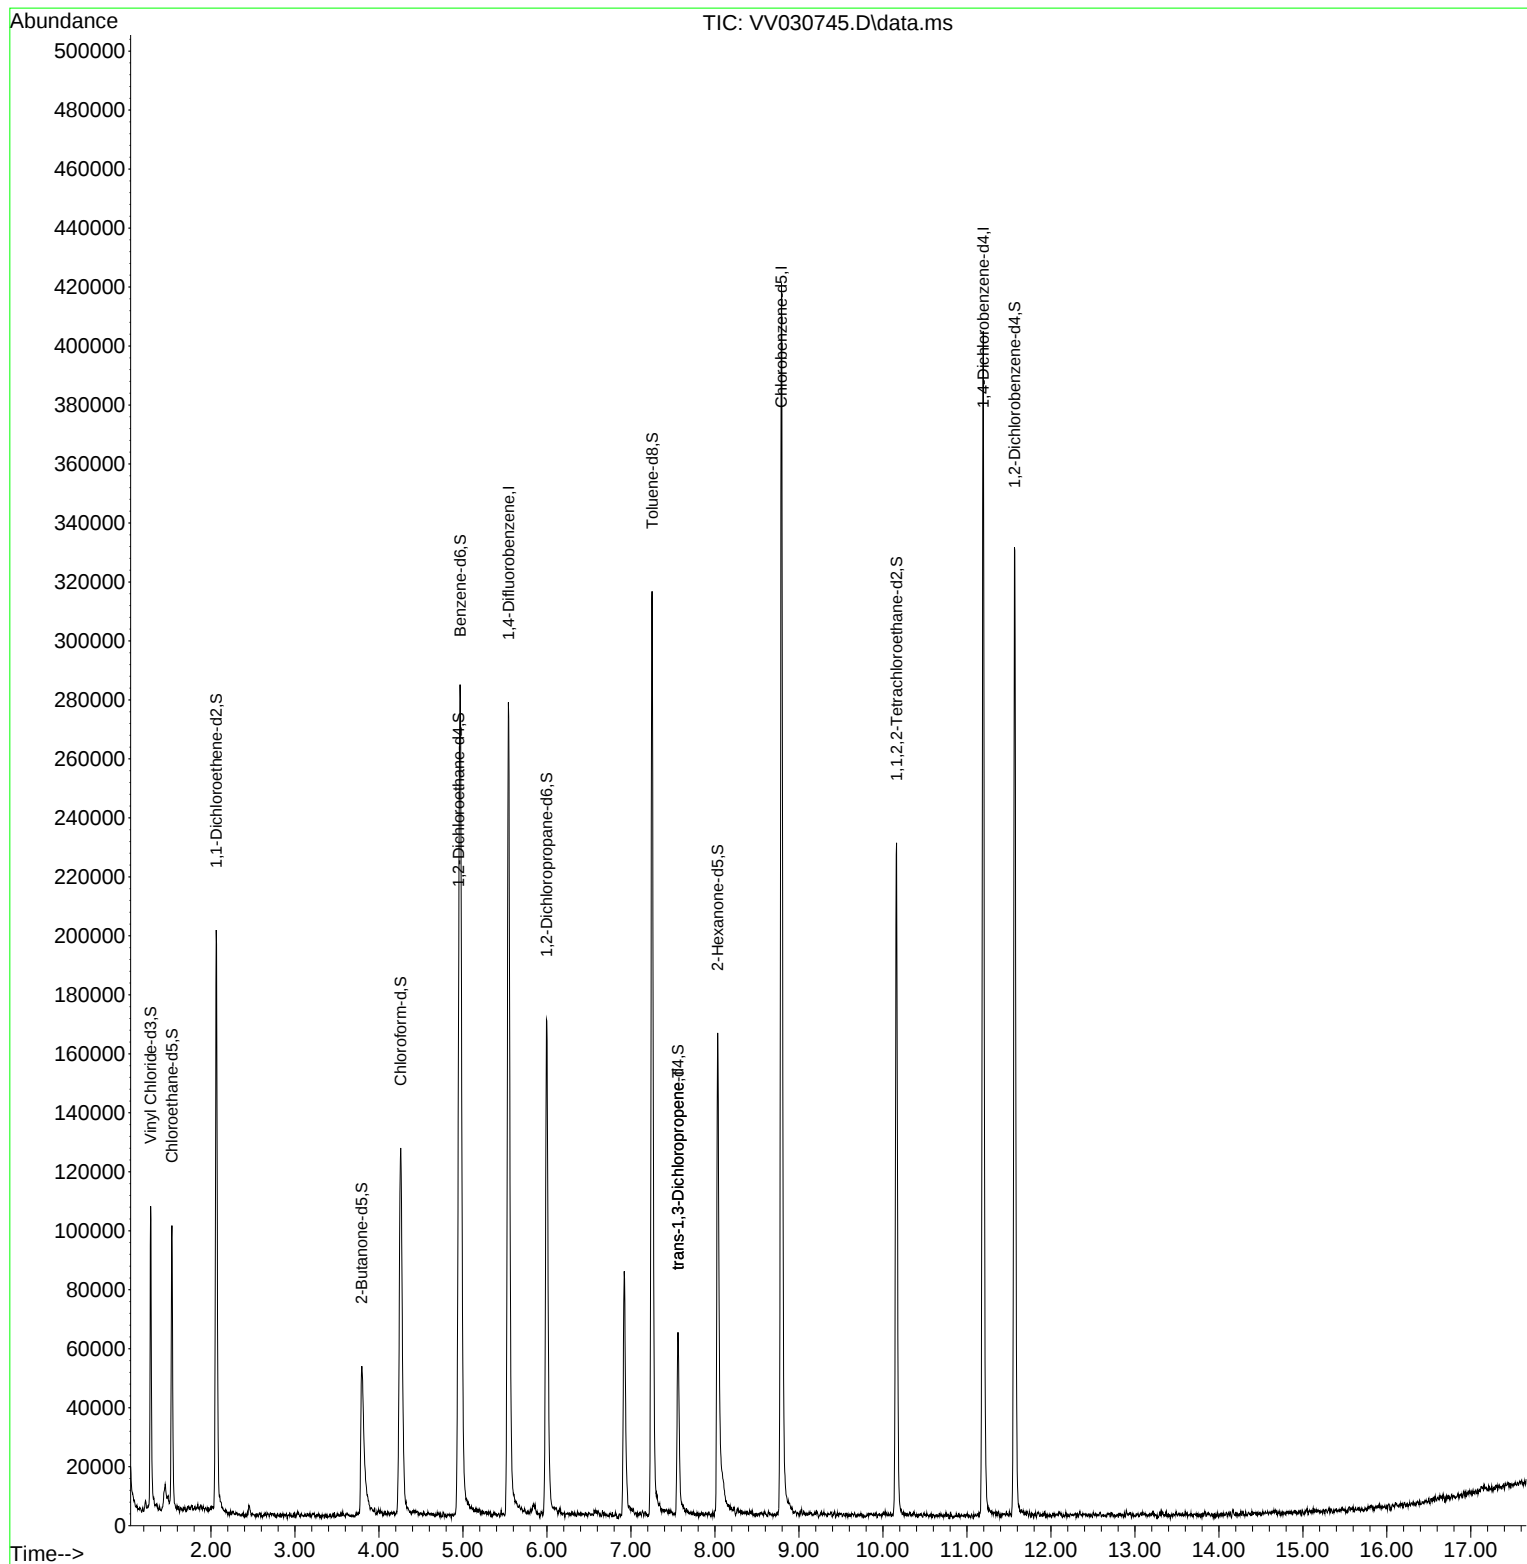

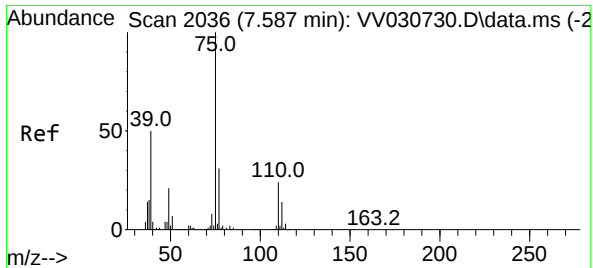

#44
 trans-1,3-Dichloropropene
 Concen: 0.762 ug/L
 RT: 7.561 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV030745.D
 Acq: 21 Apr 2023 02:53

Instrument :
 MSVOA_V
 ClientSampleId :
 C0MQ9

Tgt Ion: 75 Resp: 2046
 Ion Ratio Lower Upper
 75 100
 77 36.6 22.1 41.1

