




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:15:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
 Supervised By :Mahesh Dadoda 04/22/2023

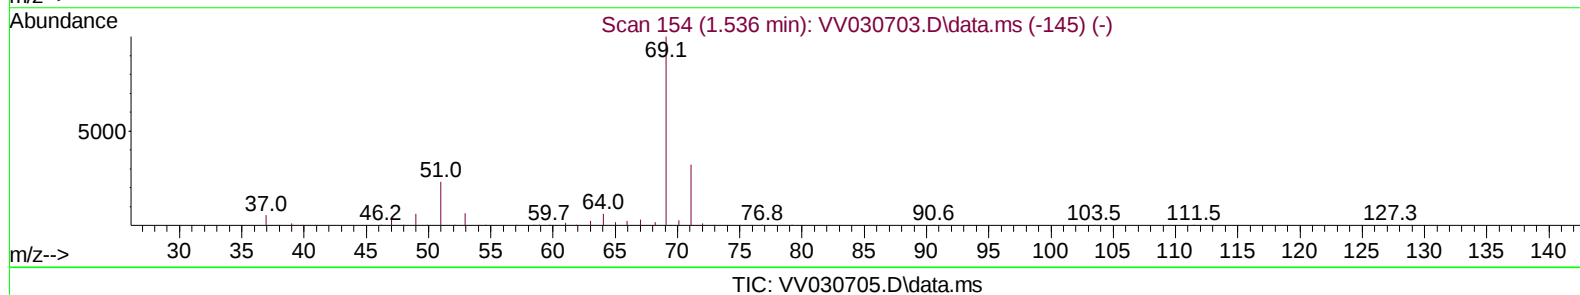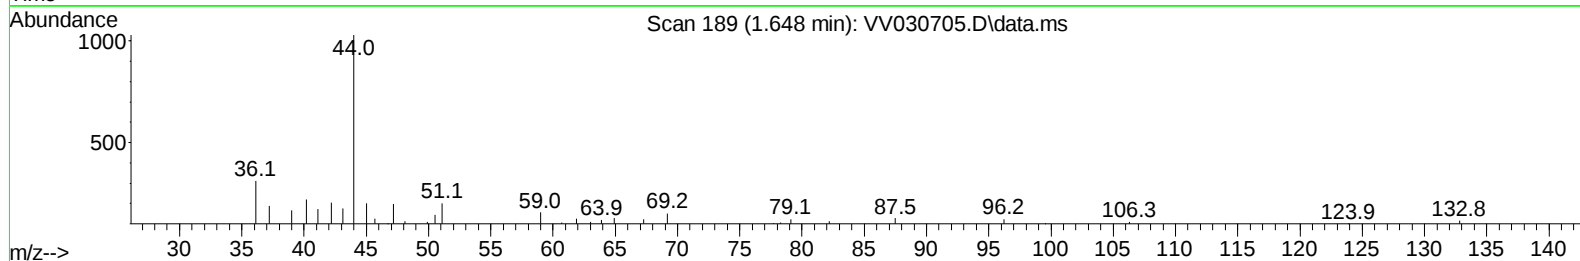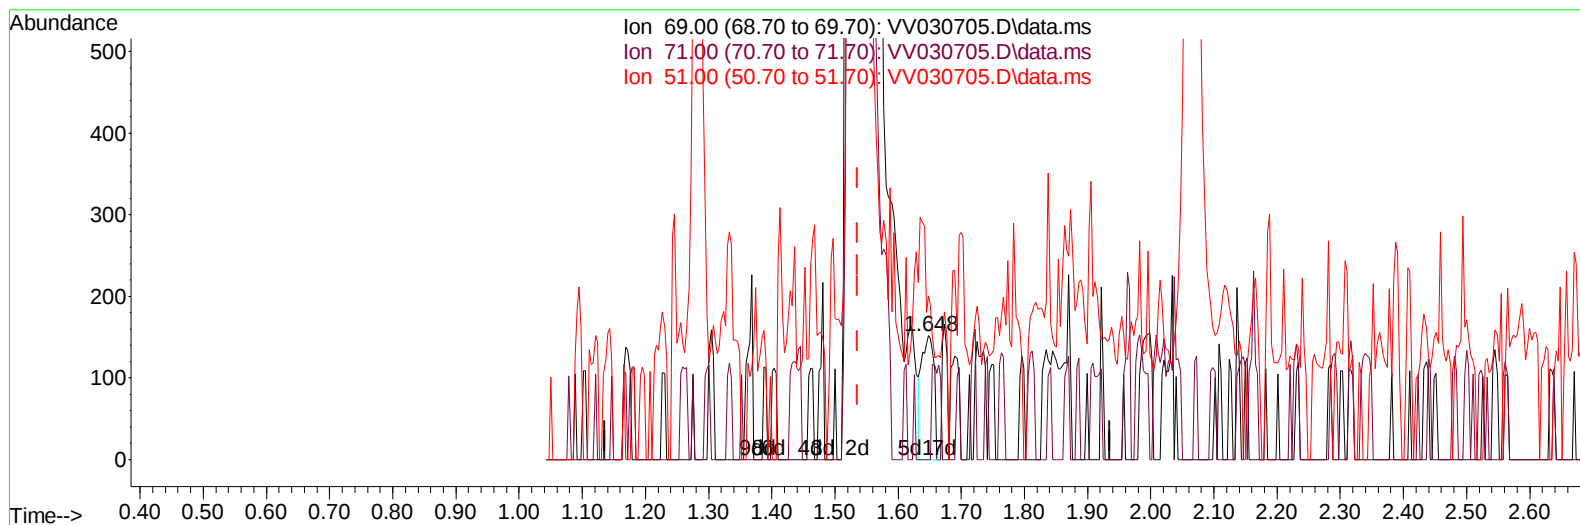

(7) Chloroethane-d5 (S)

1.648min (+ 0.113) 0.21 ug/L

response 204

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	31.86
51.00	30.70	35.78
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:15:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
 Supervised By :Mahesh Dadoda 04/22/2023

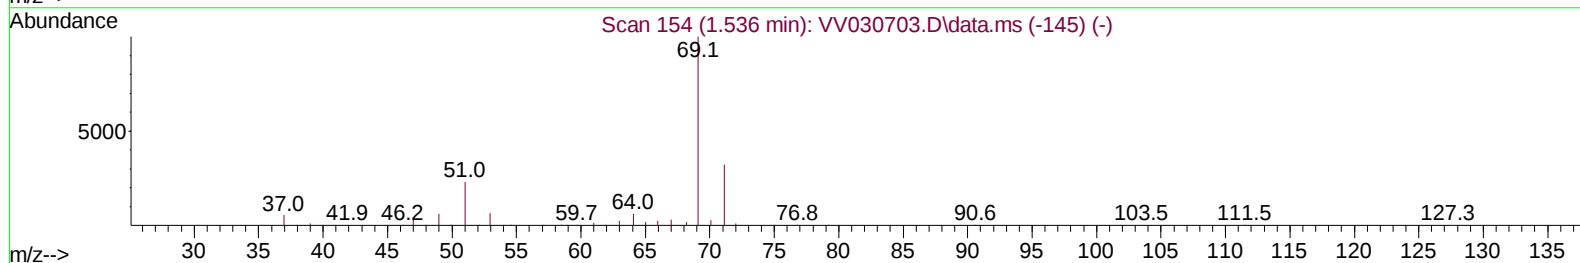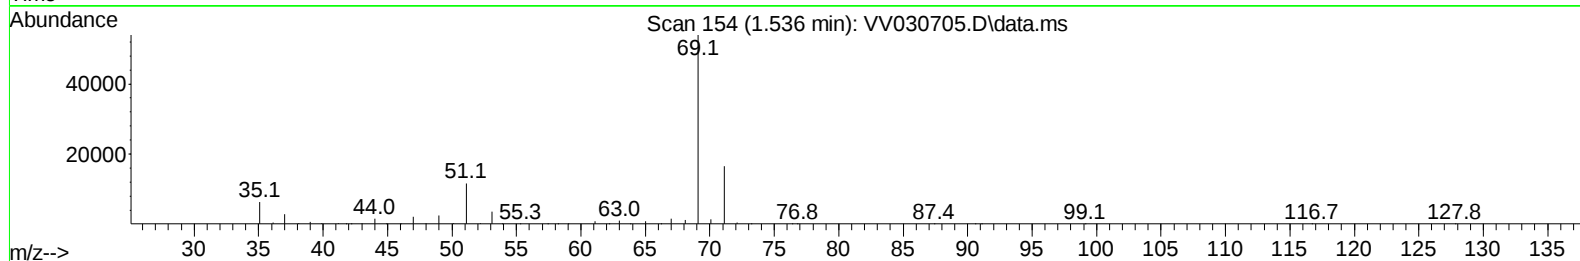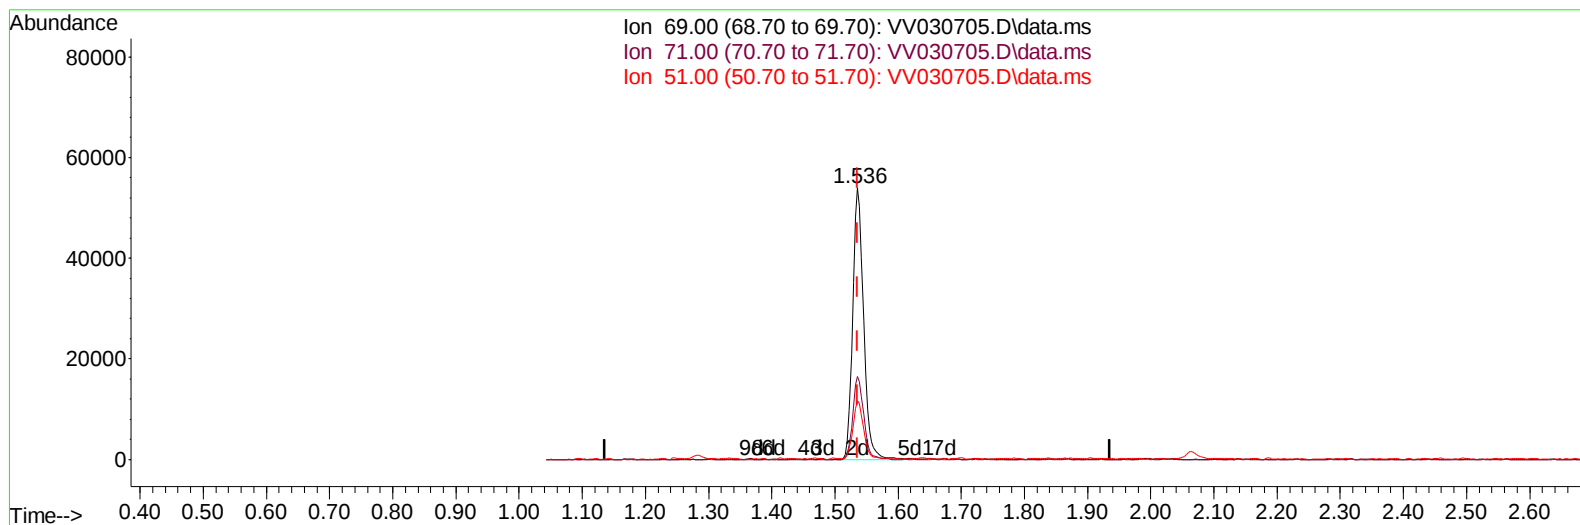

TIC: VV030705.D\data.ms

(7) Chloroethane-d5 (S)

1.536min (+ 0.000) 66.25 ug/L m

response 64955

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	0.10#
51.00	30.70	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:15:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
 Supervised By :Mahesh Dadoda 04/22/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	159599	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	153585	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	72415	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	80912	69.156	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	138.320%#	
7) Chloroethane-d5	1.536	69	64955m	66.251	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	132.500%#	
11) 1,1-Dichloroethene-d2	2.063	65	36506	65.795	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	131.600%#	
21) 2-Butanone-d5	3.799	46	79348	123.475	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	123.470%	
24) Chloroform-d	4.256	84	138924	65.521	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	131.040%#	
26) 1,2-Dichloroethane-d4	4.947	65	96677	70.921	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	141.840%#	
32) Benzene-d6	4.966	84	256365	70.601	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	141.200%#	
36) 1,2-Dichloropropane-d6	5.995	67	79157	70.178	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	140.360%#	
41) Toluene-d8	7.249	98	224219	65.766	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	131.540%#	
43) trans-1,3-Dichloroprop...	7.558	79	38109	67.034	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	134.060%#	
47) 2-Hexanone-d5	8.034	63	50159	112.884	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	112.880%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	96104	58.718	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	117.440%	
66) 1,2-Dichlorobenzene-d4	11.571	152	86335	75.008	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	150.020%#	
Target Compounds						
					Qvalue	
13) Acetone	2.124	43	6829	6.867	ug/L	95
20) cis-1,2-Dichloroethene	3.828	96	14042	11.442	ug/L	89
25) Chloroform	4.281	83	32531	13.664	ug/L	97
30) 1,1,1-Trichloroethane	4.519	97	11750	5.445	ug/L	99
34) Trichloroethene	5.838	95	125817	103.713	ug/L	98
38) Bromodichloromethane	6.442	83	2236	1.268	ug/L #	85
51) Chlorobenzene	8.828	112	2396	0.724	ug/L	98
65) 1,4-Dichlorobenzene	11.220	146	2529	1.061	ug/L	97
72) 1,2,3-Trichlorobenzene	13.689	180	1344	0.935	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030705.D
Acq On : 20 Apr 2023 10:36
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:15:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 00:14:50 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
Supervised By :Mahesh Dadoda 04/22/2023

