




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030713.D
Acq On : 20 Apr 2023 13:48
Operator : SY/MD
Sample : 02411-08 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:17:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 00:14:50 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
Supervised By :Mahesh Dadoda 04/22/2023

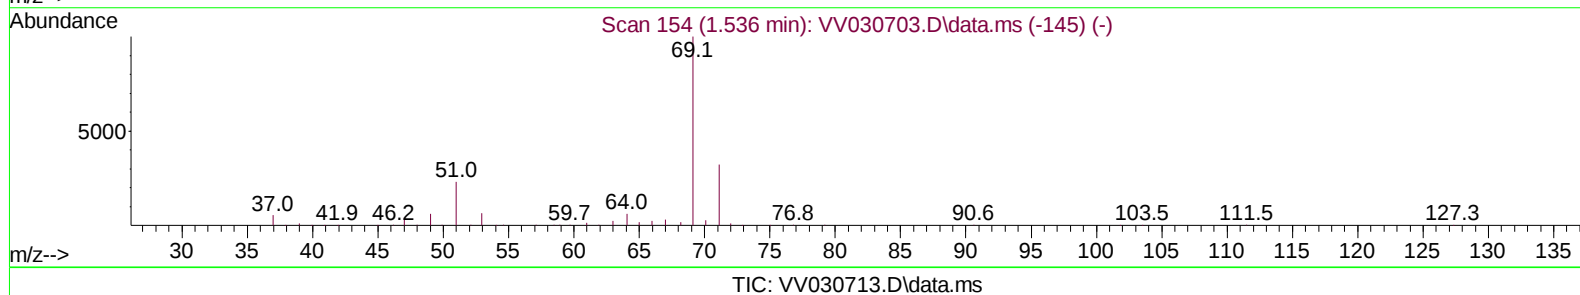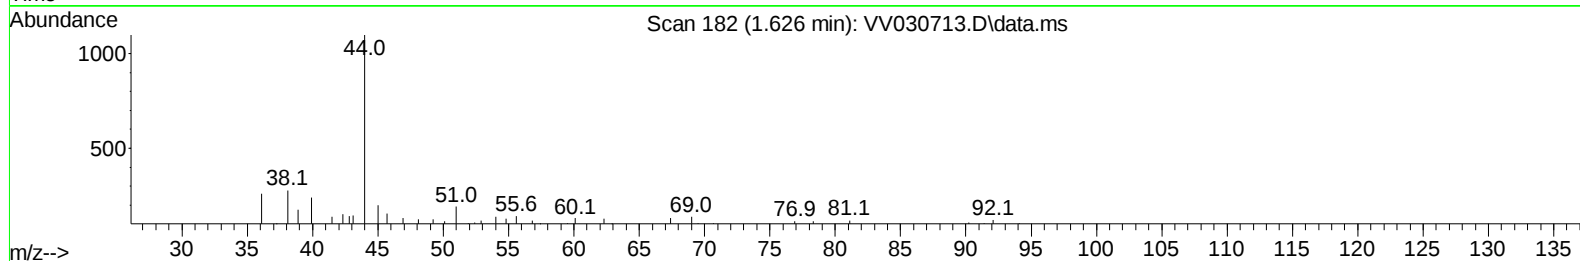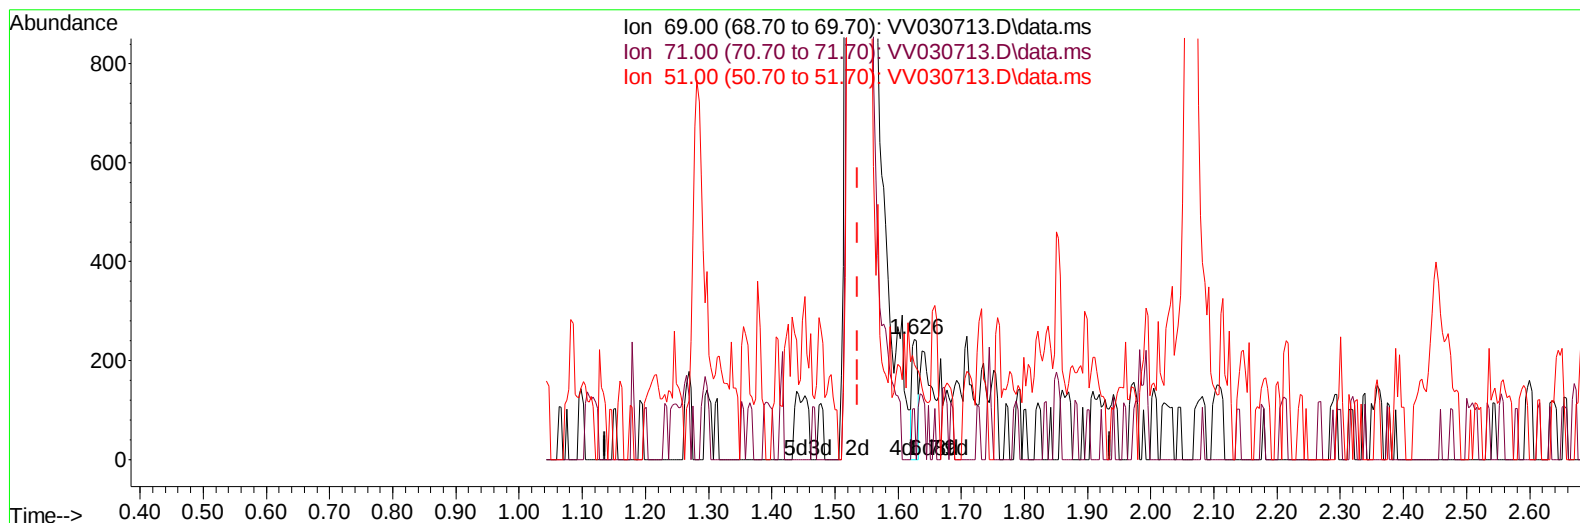

(7) Chloroethane-d5 (S)

1.626min (+ 0.090) 0.11 ug/L

response 162

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	24.07
51.00	30.70	22.22
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030713.D
 Acq On : 20 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02411-08 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:17:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
 Supervised By :Mahesh Dadoda 04/22/2023

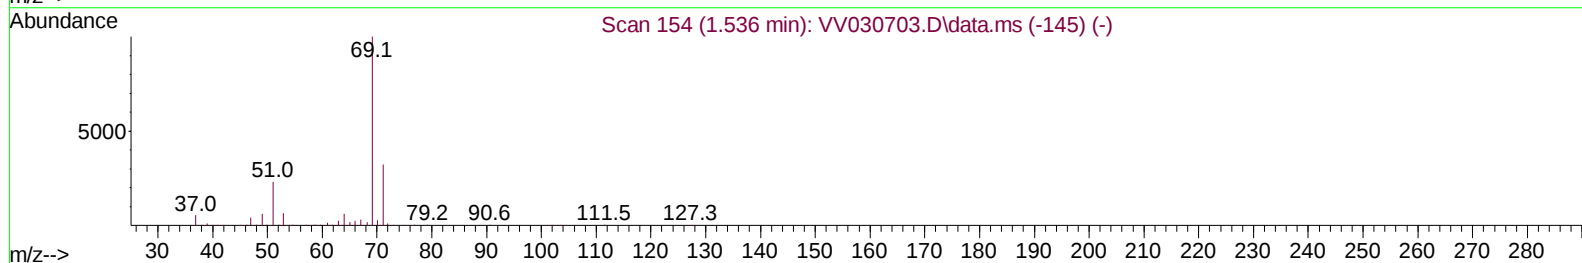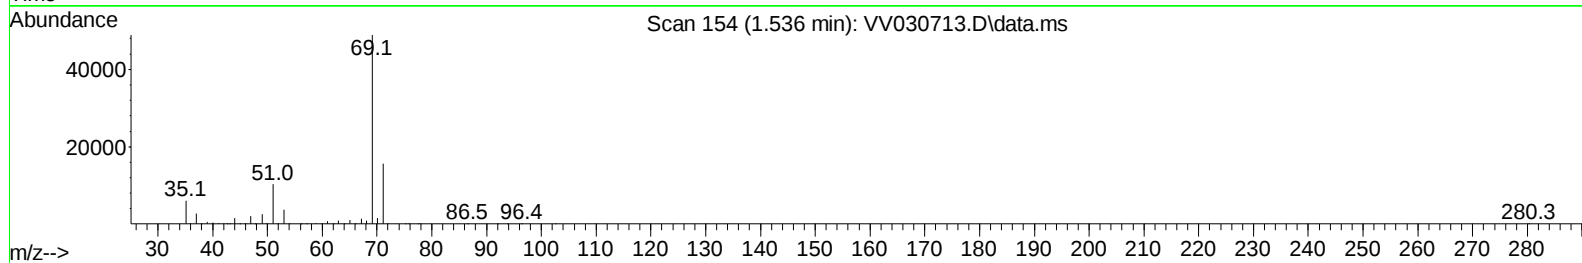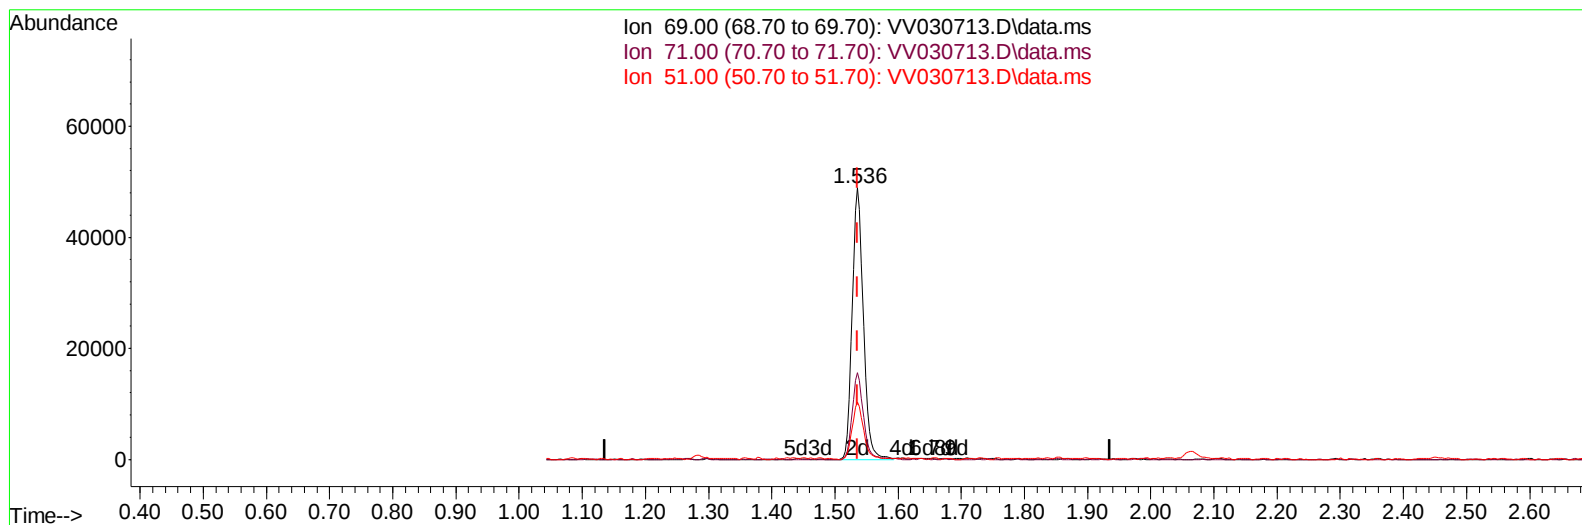

TIC: VV030713.D\data.ms

(7) Chloroethane-d5 (S)

1.536min (+ 0.000) 42.16 ug/L m

response 59666

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.00	0.07#
51.00	30.70	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030713.D
 Acq On : 20 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02411-08 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:17:46 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 21 00:14:50 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
 Supervised By :Mahesh Dadoda 04/22/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	230355	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	225744	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	108879	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	72089	42.689	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	85.380%	
7) Chloroethane-d5	1.536	69	59666m	42.164	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	84.320%	
11) 1,1-Dichloroethene-d2	2.063	65	35456	44.274	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	88.540%	
21) 2-Butanone-d5	3.796	46	83533	90.060	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.060%	
24) Chloroform-d	4.259	84	131273	42.896	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	85.800%	
26) 1,2-Dichloroethane-d4	4.950	65	92408	46.967	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	93.940%	
32) Benzene-d6	4.969	84	244051	45.726	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	91.460%	
36) 1,2-Dichloropropane-d6	5.998	67	74958	45.213	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.420%	
41) Toluene-d8	7.252	98	210823	42.071	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	84.140%	
43) trans-1,3-Dichloroprop...	7.558	79	36661	43.874	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	87.740%	
47) 2-Hexanone-d5	8.034	63	54330	83.187	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	83.190%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	103098	42.856	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	85.720%	
66) 1,2-Dichlorobenzene-d4	11.570	152	85079	49.162	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	98.320%	
Target Compounds						
30) 1,1,1-Trichloroethane	4.523	97	2256	0.711	ug/L #	78
34) Trichloroethene	5.841	95	148376	83.213	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030713.D
Acq On : 20 Apr 2023 13:48
Operator : SY/MD
Sample : 02411-08 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Manual IntegrationsAPPROVED

Quant Time: Apr 21 00:17:46 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 21 00:14:50 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/22/2023
Supervised By :Mahesh Dadoda 04/22/2023

