

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030704.D
 Acq On : 20 Apr 2023 10:06
 Operator : SY/MD
 Sample : VV0420WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	132734	146342	16.84%	2.169%
2	1.535	148	154	168	rVB	118990	139864	16.10%	2.073%
3	2.063	309	318	334	rVB	230189	339856	39.11%	5.037%
4	2.359	407	410	412	rBV4	1459	1116	0.13%	0.017%
5	2.545	465	468	469	rBV3	1140	714	0.08%	0.011%
6	2.574	473	477	478	rBV4	1379	1033	0.12%	0.015%
7	2.609	485	488	490	rBV4	1187	906	0.10%	0.013%
8	2.989	603	606	607	rBV3	1356	718	0.08%	0.011%
9	3.053	622	626	628	rVB5	1583	1155	0.13%	0.017%
10	3.162	656	660	661	rBV4	2111	1495	0.17%	0.022%
11	3.461	750	753	756	rBV4	1147	1010	0.12%	0.015%
12	3.567	783	786	789	rBV5	1728	1444	0.17%	0.021%
13	3.696	821	826	828	rVB5	2135	2012	0.23%	0.030%
14	3.738	836	839	840	rBV2	1301	784	0.09%	0.012%
15	3.799	849	858	885	rBV	51023	148801	17.12%	2.206%
16	4.059	937	939	941	rVB3	2180	771	0.09%	0.011%
17	4.256	981	1000	1022	rBV	137652	359775	41.40%	5.333%
18	4.484	1069	1071	1074	rVB4	1824	722	0.08%	0.011%
19	4.596	1103	1106	1107	rBV3	1097	740	0.09%	0.011%
20	4.609	1107	1110	1113	rVB6	1726	1122	0.13%	0.017%
21	4.715	1140	1143	1145	rBV3	1532	793	0.09%	0.012%
22	4.786	1162	1165	1171	rBV8	1754	2034	0.23%	0.030%
23	4.815	1171	1174	1177	rBV4	1593	979	0.11%	0.015%
24	4.963	1203	1220	1247	rVV2	326902	868931	100.00%	12.879%
25	5.387	1350	1352	1355	rVB4	1484	729	0.08%	0.011%
26	5.490	1382	1384	1386	rBV3	1388	798	0.09%	0.012%
27	5.538	1387	1399	1419	rVV	268254	557965	64.21%	8.270%
28	5.802	1477	1481	1482	rBV4	1631	1147	0.13%	0.017%
29	5.995	1529	1541	1565	rBV	186576	389998	44.88%	5.781%
30	6.233	1611	1615	1617	rBV4	1303	755	0.09%	0.011%
31	6.275	1625	1628	1630	rVB3	1801	1079	0.12%	0.016%
32	6.294	1630	1634	1638	rBV7	1633	1741	0.20%	0.026%
33	6.442	1677	1680	1685	rBV5	1986	1903	0.22%	0.028%
34	6.542	1709	1711	1714	rBV4	969	789	0.09%	0.012%
35	6.651	1742	1745	1747	rBV3	1929	1210	0.14%	0.018%
36	6.767	1777	1781	1782	rBV4	1652	1106	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030704.D
 Acq On : 20 Apr 2023 10:06
 Operator : SY/MD
 Sample : VV0420WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.918	1818	1828	1848	rVV	99238	187078	21.53%	2.773%
38	7.249	1920	1931	1950	rBV	367664	645196	74.25%	9.563%
39	7.558	2017	2027	2041	rBV	70359	128744	14.82%	1.908%
40	7.956	2147	2151	2153	rBV4	1325	943	0.11%	0.014%
41	7.989	2158	2161	2164	rBV5	1169	1160	0.13%	0.017%
42	8.034	2166	2175	2208	rVV	166611	340214	39.15%	5.043%
43	8.339	2267	2270	2274	rBV5	1311	1419	0.16%	0.021%
44	8.387	2282	2285	2289	rVB4	1854	1242	0.14%	0.018%
45	8.407	2289	2291	2292	rBV2	1685	938	0.11%	0.014%
46	8.525	2325	2328	2332	rBV4	1378	896	0.10%	0.013%
47	8.792	2398	2411	2431	rBV	406946	697781	80.30%	10.343%
48	8.947	2454	2459	2461	rBV5	1984	2096	0.24%	0.031%
49	9.017	2480	2481	2485	rVB3	1468	782	0.09%	0.012%
50	9.336	2577	2580	2583	rBV5	1338	1014	0.12%	0.015%
51	9.619	2665	2668	2670	rBV3	1145	784	0.09%	0.012%
52	9.670	2680	2684	2685	rBV4	2126	1042	0.12%	0.015%
53	9.702	2691	2694	2696	rVB3	2236	1100	0.13%	0.016%
54	9.751	2708	2709	2713	rVB4	1824	917	0.11%	0.014%
55	9.773	2713	2716	2719	rBV5	1706	1236	0.14%	0.018%
56	9.879	2744	2749	2756	rBV9	3043	3293	0.38%	0.049%
57	10.024	2792	2794	2798	rBV6	1334	1342	0.15%	0.020%
58	10.159	2825	2836	2854	rBV	243475	394713	45.43%	5.851%
59	10.442	2921	2924	2926	rVB4	1791	1000	0.12%	0.015%
60	10.464	2927	2931	2932	rBV4	1591	901	0.10%	0.013%
61	10.641	2980	2986	2988	rBV7	1534	1139	0.13%	0.017%
62	10.786	3027	3031	3033	rBV5	1454	881	0.10%	0.013%
63	10.799	3033	3035	3039	rVV5	1444	693	0.08%	0.010%
64	10.850	3048	3051	3052	rBV3	2259	1172	0.13%	0.017%
65	10.943	3076	3080	3082	rBV6	1433	1253	0.14%	0.019%
66	10.992	3091	3095	3098	rBV6	1200	1043	0.12%	0.015%
67	11.194	3147	3158	3180	rBV	389732	632715	72.82%	9.378%
68	11.352	3205	3207	3209	rBV4	1518	829	0.10%	0.012%
69	11.432	3230	3232	3235	rVB4	1534	723	0.08%	0.011%
70	11.567	3262	3274	3296	rVV	365136	593779	68.33%	8.801%
71	11.747	3325	3330	3332	rBV5	2188	1871	0.22%	0.028%
72	12.008	3408	3411	3412	rBV3	2108	1179	0.14%	0.017%
73	12.062	3426	3428	3434	rVB7	2007	1785	0.21%	0.026%
74	12.088	3434	3436	3439	rBV4	1450	974	0.11%	0.014%
75	12.162	3456	3459	3462	rVB5	1321	987	0.11%	0.015%
76	12.213	3473	3475	3479	rVB5	1479	849	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030704.D
 Acq On : 20 Apr 2023 10:06
 Operator : SY/MD
 Sample : VV0420WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK327

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.300	3501	3502	3508	rVB5	1432	909	0.10%	0.013%
78	12.438	3543	3545	3547	rBV3	1332	742	0.09%	0.011%
79	12.496	3560	3563	3566	rBV5	1361	943	0.11%	0.014%
80	12.792	3653	3655	3658	rBV5	1554	1107	0.13%	0.016%
81	12.956	3702	3706	3707	rBV3	1236	715	0.08%	0.011%
82	12.995	3715	3718	3720	rBV4	1387	1000	0.12%	0.015%
83	13.075	3740	3743	3747	rBV4	1157	1114	0.13%	0.017%
84	13.104	3751	3752	3757	rVB4	1440	872	0.10%	0.013%
85	13.162	3769	3770	3775	rVB4	1716	930	0.11%	0.014%
86	13.210	3775	3785	3796	rBV5	12527	20691	2.38%	0.307%
87	13.448	3847	3859	3872	rBV2	23015	41099	4.73%	0.609%
88	13.583	3898	3901	3903	rBV4	1111	828	0.10%	0.012%
89	13.692	3927	3935	3947	rVB5	13439	23893	2.75%	0.354%
90	13.863	3986	3988	3992	rBV5	1202	739	0.09%	0.011%
91	13.892	3994	3997	4000	rVV5	2189	1549	0.18%	0.023%
92	13.924	4004	4007	4009	rBV4	1841	1009	0.12%	0.015%
93	14.037	4038	4042	4044	rBV5	1647	1021	0.12%	0.015%
94	14.127	4065	4070	4074	rBV8	1607	1623	0.19%	0.024%
95	14.146	4074	4076	4079	rBV4	1114	706	0.08%	0.010%
96	14.236	4099	4104	4105	rBV5	1184	1001	0.12%	0.015%
97	14.274	4114	4116	4118	rBV3	1347	774	0.09%	0.011%
98	14.313	4125	4128	4129	rBV3	2020	1146	0.13%	0.017%
99	14.615	4219	4222	4223	rBV3	1826	1038	0.12%	0.015%
100	14.799	4278	4279	4286	rBV7	1329	1142	0.13%	0.017%




Sum of corrected areas: 6746631

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030704.D
Acq On : 20 Apr 2023 10:06
Operator : SY/MD
Sample : VV0420WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

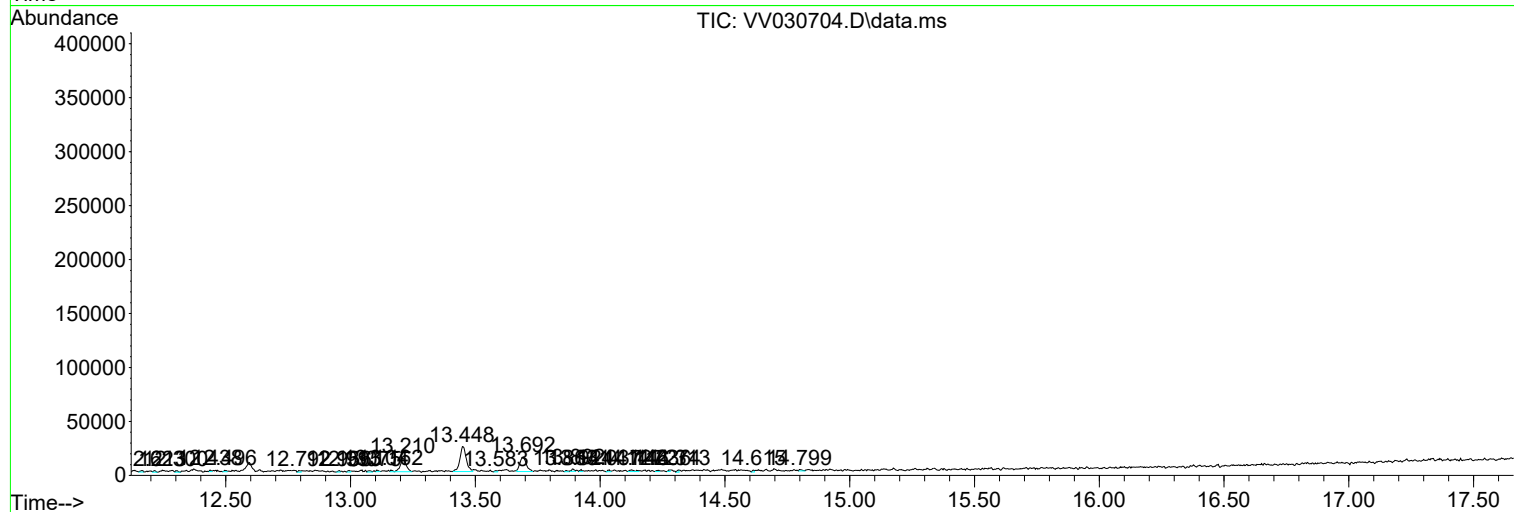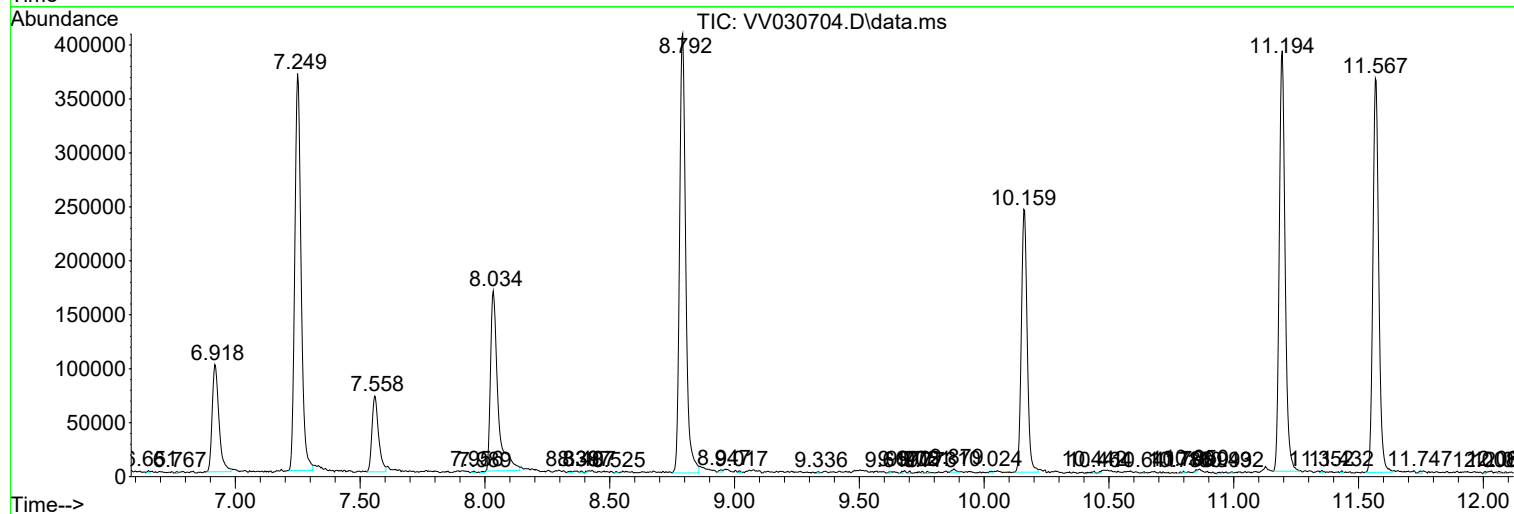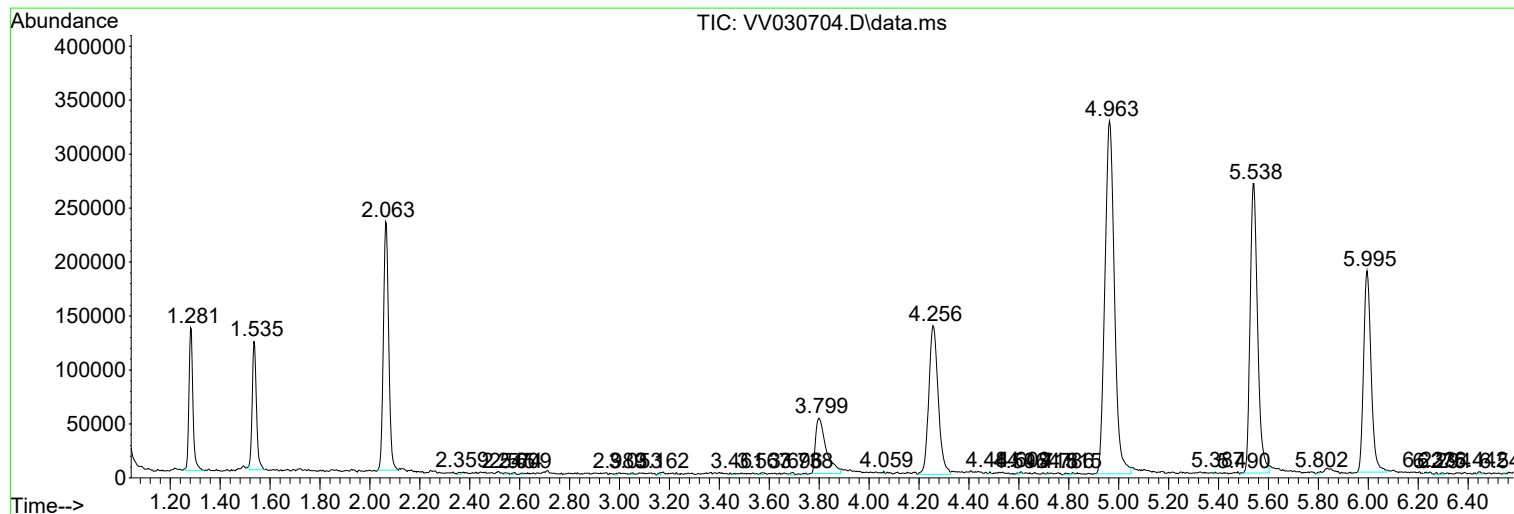

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030704.D
Acq On : 20 Apr 2023 10:06
Operator : SY/MD
Sample : VV0420WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030704.D
Acq On : 20 Apr 2023 10:06
Operator : SY/MD
Sample : VV0420WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK327

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc