

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	122936	131634	16.00%	1.938%
2	1.536	148	154	168	rVB	106986	127149	15.45%	1.872%
3	2.063	310	318	331	rBV	221189	322826	39.24%	4.752%
4	2.426	427	431	433	rBV5	1780	1258	0.15%	0.019%
5	2.532	462	464	466	rBV3	1059	581	0.07%	0.009%
6	2.571	471	476	481	rVB9	1642	1358	0.17%	0.020%
7	2.622	490	492	495	rBV4	843	553	0.07%	0.008%
8	2.683	509	511	513	rBV3	959	517	0.06%	0.008%
9	2.696	513	515	519	rVV5	1506	1260	0.15%	0.019%
10	2.799	545	547	552	rVB6	1327	649	0.08%	0.010%
11	2.825	552	555	558	rVB4	1974	975	0.12%	0.014%
12	2.867	565	568	570	rBV3	1333	891	0.11%	0.013%
13	2.902	577	579	581	rBV3	1338	585	0.07%	0.009%
14	2.989	603	606	610	rBV3	1430	1099	0.13%	0.016%
15	3.011	610	613	617	rBV5	1228	1118	0.14%	0.016%
16	3.095	635	639	641	rBV4	1584	1267	0.15%	0.019%
17	3.166	660	661	665	rVB5	1678	655	0.08%	0.010%
18	3.333	709	713	715	rBV5	1512	866	0.11%	0.013%
19	3.439	739	746	747	rBV6	1489	1426	0.17%	0.021%
20	3.478	754	758	759	rBV4	1065	548	0.07%	0.008%
21	3.519	766	771	772	rBV6	976	804	0.10%	0.012%
22	3.587	790	792	797	rBV6	1484	1141	0.14%	0.017%
23	3.677	818	820	824	rBV5	1494	1106	0.13%	0.016%
24	3.732	835	837	841	rVB4	1620	1150	0.14%	0.017%
25	3.809	848	861	885	rBV3	54481	197936	24.06%	2.914%
26	4.259	981	1001	1028	rBV3	140263	431379	52.43%	6.350%
27	4.468	1064	1066	1068	rBV4	1509	576	0.07%	0.008%
28	4.638	1117	1119	1124	rVB6	1499	779	0.09%	0.011%
29	4.806	1167	1171	1173	rBV5	1552	1090	0.13%	0.016%
30	4.851	1181	1185	1186	rBV4	886	595	0.07%	0.009%
31	4.963	1202	1220	1244	rBV2	304914	822780	100.00%	12.111%
32	5.227	1300	1302	1304	rBV3	1832	930	0.11%	0.014%
33	5.429	1361	1365	1368	rBV5	1416	1246	0.15%	0.018%
34	5.478	1378	1380	1387	rBV6	1885	2369	0.29%	0.035%
35	5.542	1387	1400	1420	rBV	189081	395443	48.06%	5.821%
36	5.838	1480	1492	1521	rBV	371867	750951	91.27%	11.054%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.995	1530	1541	1562	rVB	179468	360372	43.80%	5.305%
38	6.522	1703	1705	1709	rVB5	1333	917	0.11%	0.013%
39	6.648	1742	1744	1746	rBV3	1916	1049	0.13%	0.015%
40	6.822	1796	1798	1803	rBV6	875	579	0.07%	0.009%
41	6.844	1803	1805	1808	rVB4	1380	705	0.09%	0.010%
42	6.918	1817	1828	1849	rBV	95896	184699	22.45%	2.719%
43	7.140	1895	1897	1900	rBV3	1489	970	0.12%	0.014%
44	7.249	1920	1931	1951	rBV	351744	623932	75.83%	9.184%
45	7.503	2008	2010	2013	rBV4	1568	852	0.10%	0.013%
46	7.558	2018	2027	2040	rBV	68658	123060	14.96%	1.811%
47	7.886	2119	2129	2139	rBV2	14744	28029	3.41%	0.413%
48	8.034	2166	2175	2190	rBV	144112	273321	33.22%	4.023%
49	8.468	2308	2310	2312	rBV3	931	593	0.07%	0.009%
50	8.542	2330	2333	2334	rBV3	1185	587	0.07%	0.009%
51	8.600	2349	2351	2355	rBV5	1394	990	0.12%	0.015%
52	8.664	2366	2371	2376	rBV8	2057	2253	0.27%	0.033%
53	8.793	2399	2411	2434	rBV	277599	488188	59.33%	7.186%
54	9.037	2483	2487	2490	rBV5	2233	1826	0.22%	0.027%
55	9.172	2527	2529	2531	rBV3	1556	733	0.09%	0.011%
56	9.252	2552	2554	2558	rBV4	1384	1120	0.14%	0.016%
57	9.336	2577	2580	2582	rBV3	1352	754	0.09%	0.011%
58	9.497	2624	2630	2634	rBV7	3468	3612	0.44%	0.053%
59	9.600	2659	2662	2667	rVB6	1927	1683	0.20%	0.025%
60	9.622	2667	2669	2671	rBV4	1183	615	0.07%	0.009%
61	9.635	2671	2673	2675	rBV3	1210	679	0.08%	0.010%
62	9.841	2733	2737	2740	rBV5	1926	1486	0.18%	0.022%
63	9.866	2743	2745	2749	rVB4	1919	1305	0.16%	0.019%
64	9.915	2758	2760	2762	rBV3	1240	701	0.09%	0.010%
65	9.944	2766	2769	2770	rBV3	1415	775	0.09%	0.011%
66	10.095	2813	2816	2817	rBV2	1475	779	0.09%	0.011%
67	10.159	2824	2836	2859	rBV	217551	357378	43.44%	5.261%
68	10.333	2879	2890	2901	rBV	24644	43382	5.27%	0.639%
69	10.403	2909	2912	2917	rBV5	1684	1017	0.12%	0.015%
70	10.436	2920	2922	2924	rBV4	1393	508	0.06%	0.007%
71	10.564	2958	2962	2965	rBV6	1674	1558	0.19%	0.023%
72	10.818	3037	3041	3044	rBV6	1394	1335	0.16%	0.020%
73	11.194	3147	3158	3180	rBV	276333	452491	55.00%	6.661%
74	11.571	3264	3275	3292	rVB	338545	561243	68.21%	8.261%
75	12.027	3416	3417	3419	rBV2	1360	554	0.07%	0.008%
76	12.259	3487	3489	3490	rBV2	1542	717	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030705.D
 Acq On : 20 Apr 2023 10:36
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.529	3572	3573	3575	rBV2	1239	518	0.06%	0.008%
78	12.625	3600	3603	3605	rBV4	1188	704	0.09%	0.010%
79	13.069	3737	3741	3742	rBV4	1783	996	0.12%	0.015%
80	13.095	3747	3749	3753	rVB4	2002	1163	0.14%	0.017%
81	13.146	3763	3765	3768	rBV4	1281	730	0.09%	0.011%
82	13.214	3777	3786	3797	rBV4	5418	10956	1.33%	0.161%
83	13.307	3812	3815	3817	rBV3	1564	783	0.10%	0.012%
84	13.455	3852	3861	3872	rVB2	10158	17847	2.17%	0.263%
85	13.664	3923	3926	3928	rBV4	1611	1257	0.15%	0.019%
86	13.693	3928	3935	3944	rVB4	5553	9280	1.13%	0.137%
87	13.770	3957	3959	3962	rBV4	1691	1222	0.15%	0.018%
88	13.831	3976	3978	3983	rVB5	1455	951	0.12%	0.014%
89	13.959	4013	4018	4019	rBV4	1995	1312	0.16%	0.019%
90	14.050	4044	4046	4047	rBV2	1550	626	0.08%	0.009%
91	14.078	4053	4055	4056	rBV2	1214	618	0.08%	0.009%
92	14.149	4072	4077	4079	rBV4	2062	1549	0.19%	0.023%
93	14.207	4094	4095	4099	rVB3	1719	770	0.09%	0.011%
94	14.249	4104	4108	4109	rBV4	1532	968	0.12%	0.014%
95	14.490	4180	4183	4186	rVV5	1137	765	0.09%	0.011%
96	14.522	4191	4193	4199	rVB6	1933	1477	0.18%	0.022%
97	14.754	4262	4265	4267	rBV4	1961	1215	0.15%	0.018%
98	15.069	4361	4363	4364	rBV2	1587	776	0.09%	0.011%
99	15.104	4371	4374	4376	rBV3	1572	1161	0.14%	0.017%
100	15.281	4426	4429	4431	rBV4	1480	1003	0.12%	0.015%




Sum of corrected areas: 6793484

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030705.D
Acq On : 20 Apr 2023 10:36
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

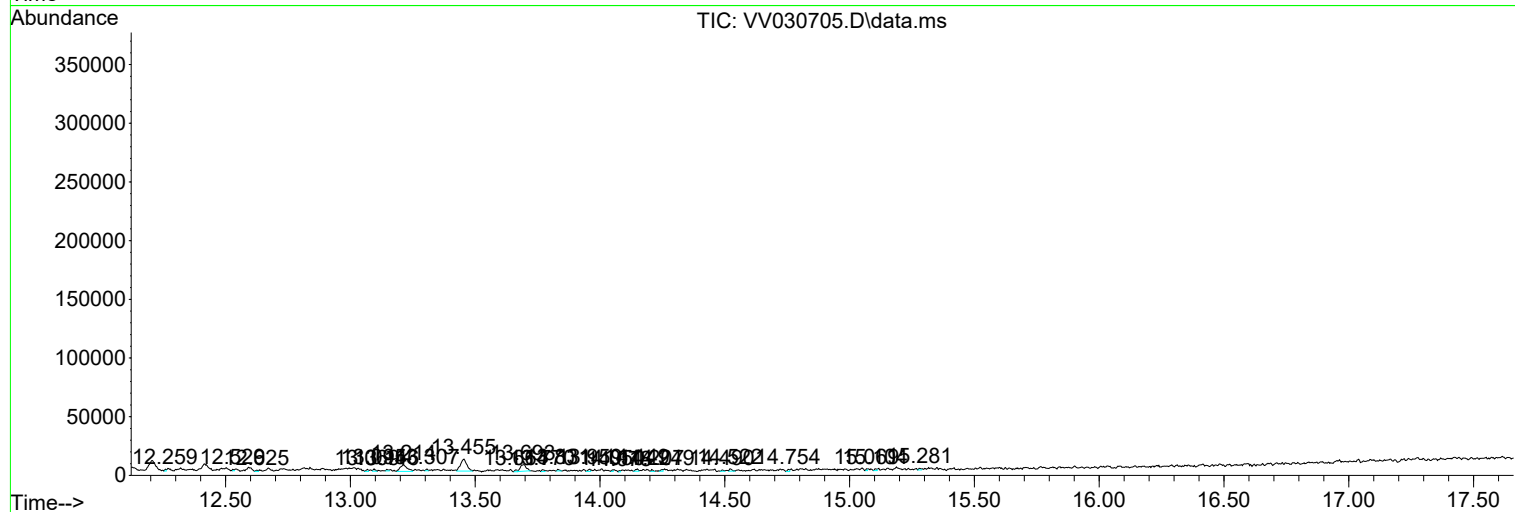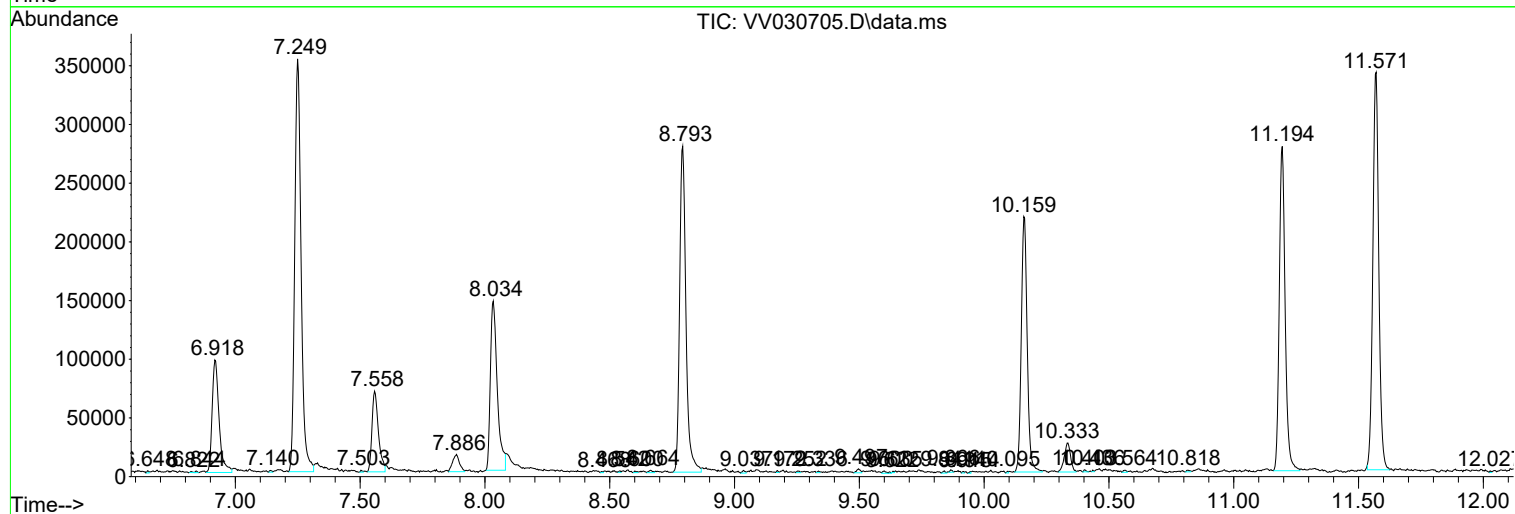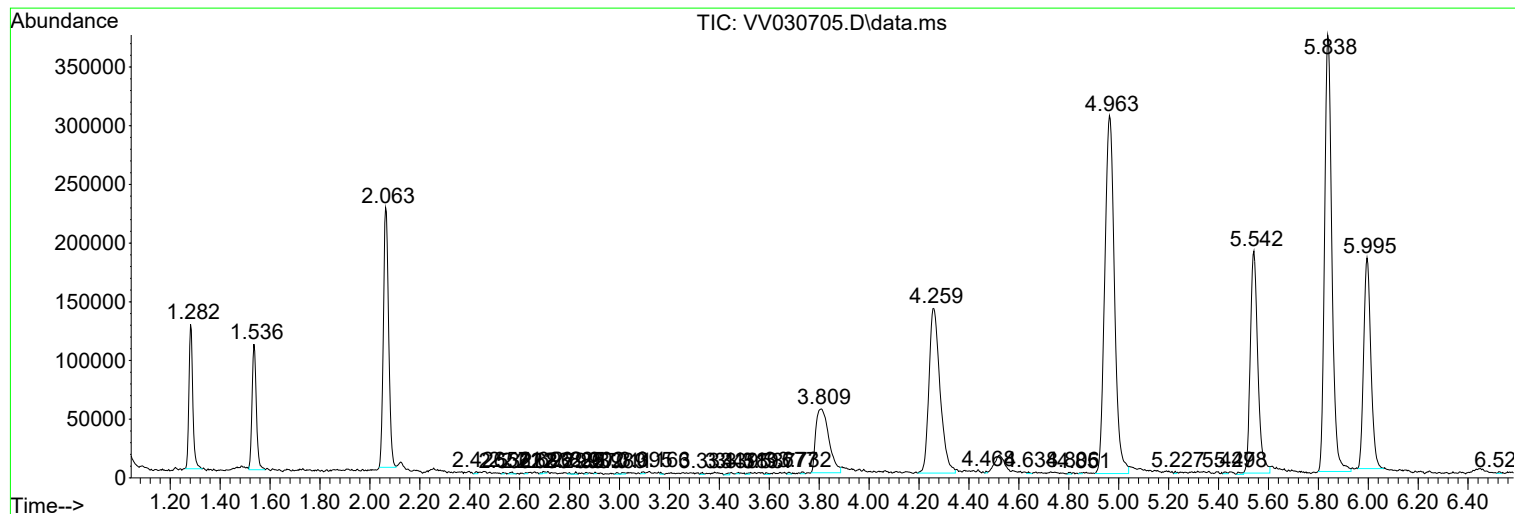

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030705.D
Acq On : 20 Apr 2023 10:36
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030705.D
Acq On : 20 Apr 2023 10:36
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc