

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030706.D
 Acq On : 20 Apr 2023 11:00
 Operator : SY/MD
 Sample : 02411-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	87025	95495	11.42%	1.402%
2	1.536	147	154	166	rVB	105032	125537	15.02%	1.843%
3	2.066	310	319	331	rBV	219352	317547	37.99%	4.661%
4	2.397	419	422	425	rBV4	994	749	0.09%	0.011%
5	2.433	428	433	434	rVB5	1092	818	0.10%	0.012%
6	2.481	446	448	451	rVB4	1333	766	0.09%	0.011%
7	2.818	550	553	556	rVB4	1069	764	0.09%	0.011%
8	2.889	571	575	577	rBV4	1527	1103	0.13%	0.016%
9	2.960	593	597	598	rBV4	1928	1161	0.14%	0.017%
10	3.130	647	650	653	rBV4	1615	1033	0.12%	0.015%
11	3.172	661	663	666	rVB3	1439	990	0.12%	0.015%
12	3.201	666	672	674	rBV7	2290	2095	0.25%	0.031%
13	3.259	686	690	693	rBV6	1291	1358	0.16%	0.020%
14	3.484	756	760	765	rVB7	1358	1063	0.13%	0.016%
15	3.593	791	794	798	rBV7	1711	1416	0.17%	0.021%
16	3.799	847	858	888	rBV	49697	150735	18.03%	2.212%
17	4.005	918	922	925	rBV4	2175	1996	0.24%	0.029%
18	4.137	959	963	965	rBV5	1119	869	0.10%	0.013%
19	4.259	988	1001	1024	rVB	136011	343019	41.04%	5.035%
20	4.683	1130	1133	1137	rBV6	1033	819	0.10%	0.012%
21	4.761	1154	1157	1160	rBV4	1212	895	0.11%	0.013%
22	4.809	1169	1172	1174	rVB5	2003	1280	0.15%	0.019%
23	4.860	1186	1188	1194	rBV6	1685	1686	0.20%	0.025%
24	4.966	1204	1221	1244	rBV2	311576	835851	100.00%	12.268%
25	5.542	1384	1400	1426	rBV	244920	518164	61.99%	7.605%
26	5.841	1482	1493	1516	rVV	256326	510870	61.12%	7.498%
27	5.998	1531	1542	1562	rVB	183631	373700	44.71%	5.485%
28	6.236	1614	1616	1618	rBV3	1312	748	0.09%	0.011%
29	6.297	1633	1635	1637	rBV3	1477	780	0.09%	0.011%
30	6.449	1678	1682	1687	rBV8	1411	1268	0.15%	0.019%
31	6.474	1687	1690	1691	rBV3	1663	896	0.11%	0.013%
32	6.629	1736	1738	1742	rBV4	1289	752	0.09%	0.011%
33	6.760	1775	1779	1781	rBV5	1745	1264	0.15%	0.019%
34	6.815	1794	1796	1798	rBV3	1236	720	0.09%	0.011%
35	6.921	1818	1829	1846	rBV2	75113	145641	17.42%	2.138%
36	7.133	1892	1895	1896	rBV2	1435	704	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030706.D
 Acq On : 20 Apr 2023 11:00
 Operator : SY/MD
 Sample : 02411-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1919	1932	1951	rBV	354286	640150	76.59%	9.396%
38	7.561	2020	2028	2040	rBV3	37221	65260	7.81%	0.958%
39	7.667	2059	2061	2065	rVB6	2106	1267	0.15%	0.019%
40	7.760	2084	2090	2093	rBV7	1449	1544	0.18%	0.023%
41	7.883	2120	2128	2140	rVB3	8936	16969	2.03%	0.249%
42	7.950	2146	2149	2150	rBV3	1368	812	0.10%	0.012%
43	7.973	2154	2156	2161	rVB6	1714	1062	0.13%	0.016%
44	8.002	2161	2165	2166	rBV4	1437	1138	0.14%	0.017%
45	8.034	2166	2175	2206	rBV	158404	325967	39.00%	4.784%
46	8.429	2296	2298	2301	rVB3	1887	1019	0.12%	0.015%
47	8.493	2315	2318	2319	rBV3	1348	775	0.09%	0.011%
48	8.555	2333	2337	2341	rBV6	1755	1637	0.20%	0.024%
49	8.580	2341	2345	2347	rBV5	1543	1301	0.16%	0.019%
50	8.722	2386	2389	2392	rVB5	1839	1229	0.15%	0.018%
51	8.793	2400	2411	2433	rBV	368238	623904	74.64%	9.157%
52	8.969	2463	2466	2469	rBV5	1737	990	0.12%	0.015%
53	9.037	2485	2487	2492	rVB4	1411	1270	0.15%	0.019%
54	9.082	2499	2501	2504	rBV4	1779	1030	0.12%	0.015%
55	9.156	2521	2524	2527	rBV5	1515	999	0.12%	0.015%
56	9.291	2564	2566	2570	rBV5	1113	854	0.10%	0.013%
57	9.432	2607	2610	2613	rBV5	1304	792	0.09%	0.012%
58	9.481	2618	2625	2626	rBV6	1998	1574	0.19%	0.023%
59	9.548	2644	2646	2650	rBV4	1377	968	0.12%	0.014%
60	9.567	2650	2652	2655	rBV4	1080	676	0.08%	0.010%
61	9.690	2684	2690	2692	rBV7	1694	1655	0.20%	0.024%
62	9.725	2698	2701	2705	rBV5	1376	1121	0.13%	0.016%
63	9.757	2709	2711	2713	rBV3	1638	904	0.11%	0.013%
64	9.863	2738	2744	2745	rBV6	1816	1426	0.17%	0.021%
65	9.921	2759	2762	2767	rBV6	1330	1302	0.16%	0.019%
66	10.111	2819	2821	2824	rBV4	1604	1044	0.12%	0.015%
67	10.162	2825	2837	2854	rVV	237738	389460	46.59%	5.716%
68	10.333	2880	2890	2902	rVB	21529	38562	4.61%	0.566%
69	10.378	2902	2904	2906	rBV3	1809	996	0.12%	0.015%
70	10.506	2941	2944	2948	rVB6	1412	1189	0.14%	0.017%
71	10.535	2948	2953	2955	rBV5	1585	1245	0.15%	0.018%
72	10.616	2974	2978	2981	rBV6	1524	1458	0.17%	0.021%
73	10.757	3019	3022	3025	rBV4	981	802	0.10%	0.012%
74	10.789	3030	3032	3034	rBV2	1545	797	0.10%	0.012%
75	10.834	3043	3046	3048	rBV3	1916	1008	0.12%	0.015%
76	11.101	3125	3129	3137	rBV10	4251	4970	0.59%	0.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030706.D
 Acq On : 20 Apr 2023 11:00
 Operator : SY/MD
 Sample : 02411-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3145	3158	3176	rBV	361332	587956	70.34%	8.630%
78	11.333	3197	3201	3203	rBV4	2189	1464	0.18%	0.021%
79	11.567	3262	3274	3295	rBV	363614	599527	71.73%	8.800%
80	11.744	3327	3329	3332	rVB3	1488	834	0.10%	0.012%
81	11.767	3332	3336	3340	rBV7	949	1026	0.12%	0.015%
82	11.873	3365	3369	3370	rBV5	1472	921	0.11%	0.014%
83	11.931	3383	3387	3389	rBV5	1202	968	0.12%	0.014%
84	12.079	3430	3433	3437	rBV6	1432	1019	0.12%	0.015%
85	12.300	3492	3502	3512	rBV6	8022	13651	1.63%	0.200%
86	12.509	3564	3567	3572	rBV7	1511	1231	0.15%	0.018%
87	12.583	3587	3590	3591	rBV3	1831	1011	0.12%	0.015%
88	12.863	3674	3677	3678	rBV3	1385	691	0.08%	0.010%
89	12.953	3699	3705	3710	rVB9	1602	2205	0.26%	0.032%
90	13.037	3725	3731	3732	rBV5	1672	1461	0.17%	0.021%
91	13.175	3771	3774	3776	rBV4	1380	770	0.09%	0.011%
92	13.201	3776	3782	3783	rBV5	1990	2003	0.24%	0.029%
93	13.548	3888	3890	3892	rVB2	1558	687	0.08%	0.010%
94	13.773	3957	3960	3964	rVB5	1402	1178	0.14%	0.017%
95	13.976	4018	4023	4026	rBV7	1656	1673	0.20%	0.025%
96	14.156	4075	4079	4082	rBV4	2572	2004	0.24%	0.029%
97	14.406	4153	4157	4160	rBV6	937	690	0.08%	0.010%
98	14.898	4304	4310	4314	rBV8	2172	2620	0.31%	0.038%
99	15.127	4377	4381	4382	rBV3	1652	1017	0.12%	0.015%
100	15.271	4423	4426	4427	rBV3	1797	887	0.11%	0.013%




Sum of corrected areas: 6813172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030706.D
Acq On : 20 Apr 2023 11:00
Operator : SY/MD
Sample : 02411-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

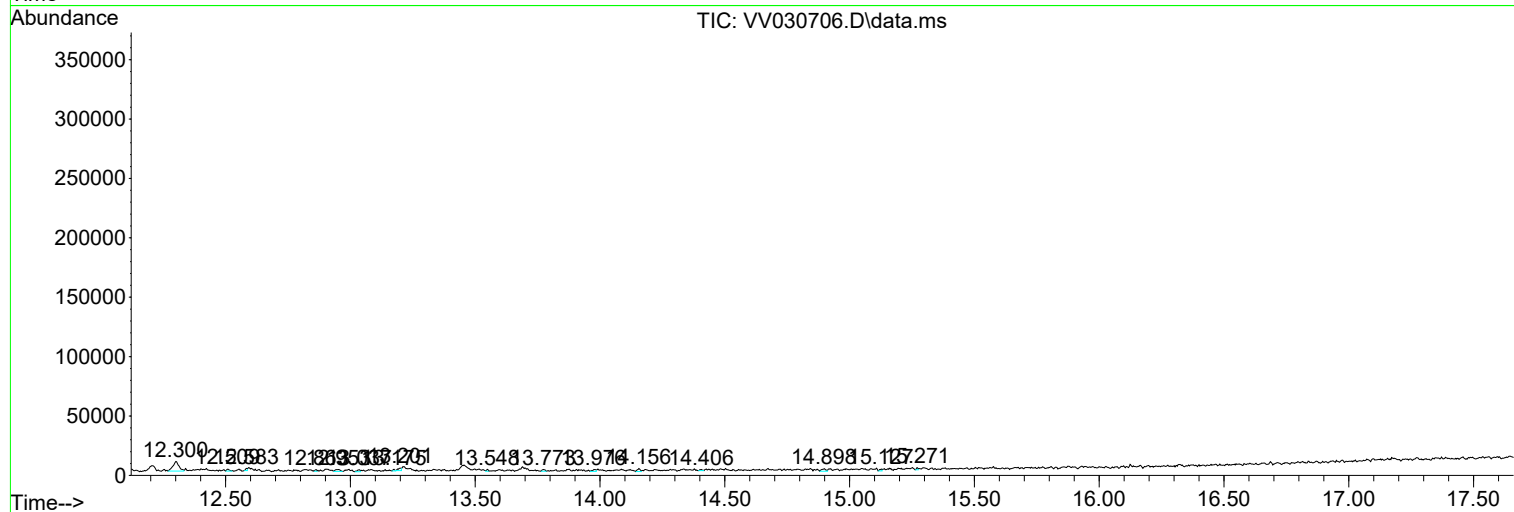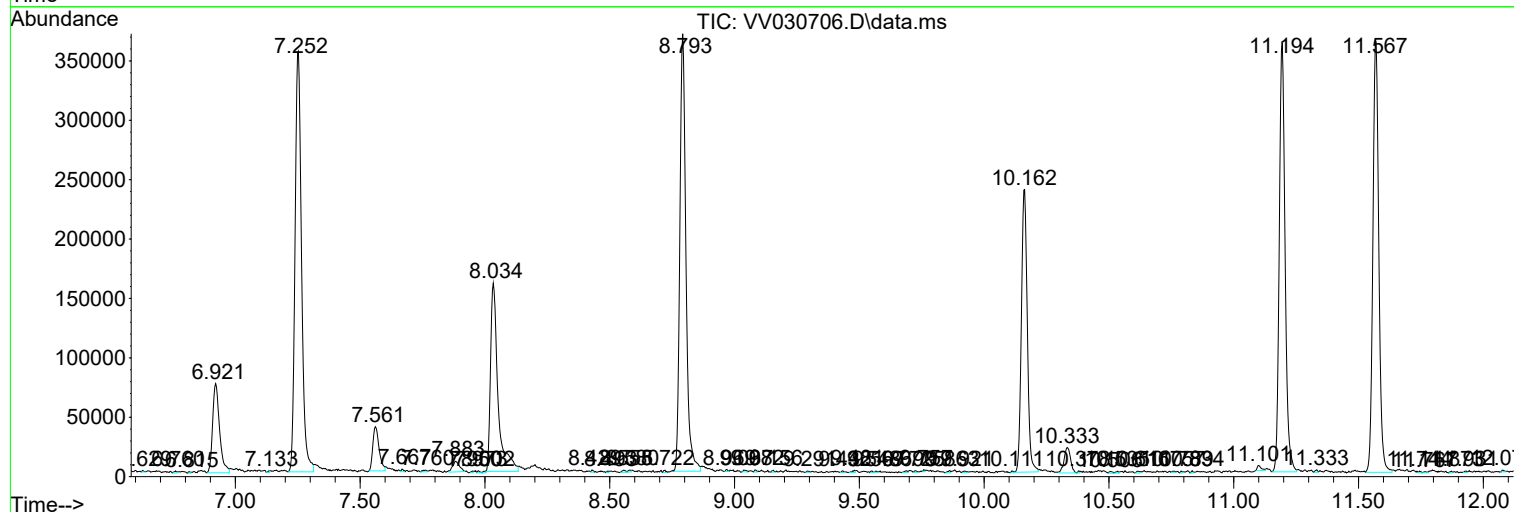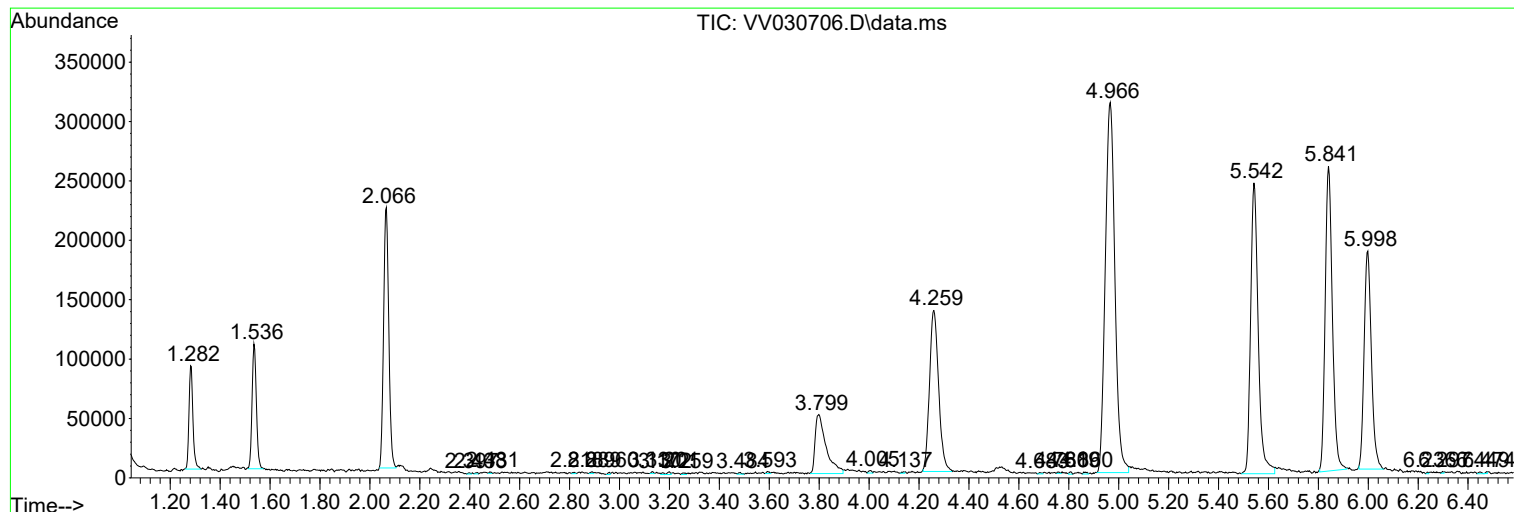

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030706.D
Acq On : 20 Apr 2023 11:00
Operator : SY/MD
Sample : 02411-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030706.D
Acq On : 20 Apr 2023 11:00
Operator : SY/MD
Sample : 02411-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc