

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030707.D
 Acq On : 20 Apr 2023 11:24
 Operator : SY/MD
 Sample : 02411-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	70	75	84	rVB	58634	62035	8.93%	0.987%
2	1.535	148	154	167	rVB	80241	94152	13.55%	1.498%
3	2.063	310	318	333	rBV	152798	220318	31.70%	3.506%
4	2.432	431	433	435	rBV3	1009	561	0.08%	0.009%
5	2.510	455	457	460	rBV4	1095	861	0.12%	0.014%
6	2.796	544	546	549	rBV3	1211	858	0.12%	0.014%
7	3.072	629	632	633	rBV2	1655	839	0.12%	0.013%
8	3.204	669	673	676	rBV5	945	852	0.12%	0.014%
9	3.246	682	686	689	rBV5	1246	958	0.14%	0.015%
10	3.265	689	692	693	rBV3	1370	827	0.12%	0.013%
11	3.487	758	761	765	rBV5	1812	1370	0.20%	0.022%
12	3.545	777	779	783	rBV4	1343	1018	0.15%	0.016%
13	3.683	819	822	824	rBV4	1613	1013	0.15%	0.016%
14	3.799	849	858	882	rBV	53190	151133	21.75%	2.405%
15	4.259	988	1001	1022	rVB	118977	299418	43.09%	4.764%
16	4.487	1069	1072	1073	rBV3	1933	1222	0.18%	0.019%
17	4.966	1206	1221	1249	rBV2	261455	694910	100.00%	11.058%
18	5.198	1290	1293	1295	rBV4	1644	1136	0.16%	0.018%
19	5.458	1369	1374	1377	rBV6	2669	2245	0.32%	0.036%
20	5.542	1389	1400	1423	rBV	242746	499354	71.86%	7.946%
21	5.837	1481	1492	1512	rBV	292936	576911	83.02%	9.180%
22	5.998	1532	1542	1559	rVB	168384	333150	47.94%	5.301%
23	6.342	1648	1649	1650	rBV	1398	427	0.06%	0.007%
24	6.857	1806	1809	1812	rBV4	1235	992	0.14%	0.016%
25	6.921	1820	1829	1847	rBV2	69645	132941	19.13%	2.115%
26	7.252	1920	1932	1950	rBV	292034	511470	73.60%	8.139%
27	7.564	2021	2029	2046	rVB	40194	74315	10.69%	1.183%
28	8.034	2166	2175	2203	rBV	169907	350379	50.42%	5.575%
29	8.792	2400	2411	2436	rBV	373502	632064	90.96%	10.058%
30	9.262	2555	2557	2560	rVB4	1579	696	0.10%	0.011%
31	9.278	2560	2562	2566	rBV5	1653	1380	0.20%	0.022%
32	9.686	2687	2689	2690	rBV2	1710	814	0.12%	0.013%
33	9.963	2773	2775	2776	rBV2	1765	731	0.11%	0.012%
34	10.078	2808	2811	2815	rBV6	1485	1001	0.14%	0.016%
35	10.098	2815	2817	2818	rBV2	1487	502	0.07%	0.008%
36	10.120	2822	2824	2825	rVB2	1371	506	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030707.D
 Acq On : 20 Apr 2023 11:24
 Operator : SY/MD
 Sample : 02411-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	10.159	2825	2836	2853	rBV	247778	406903	58.55%	6.475%
38	10.332	2882	2890	2900	rVB	14256	23298	3.35%	0.371%
39	10.403	2905	2912	2914	rBV9	2551	2579	0.37%	0.041%
40	10.525	2943	2950	2953	rBV7	2108	2755	0.40%	0.044%
41	10.731	3012	3014	3018	rBV5	1931	1315	0.19%	0.021%
42	10.908	3064	3069	3071	rBV5	1868	1703	0.25%	0.027%
43	11.194	3147	3158	3177	rBV	368317	591814	85.16%	9.417%
44	11.567	3263	3274	3297	rBV	344724	557340	80.20%	8.869%
45	12.297	3491	3501	3510	rBV6	15687	27274	3.92%	0.434%
46	12.561	3579	3583	3584	rBV5	1336	910	0.13%	0.014%
47	12.779	3648	3651	3658	rBV8	2001	2661	0.38%	0.042%
48	12.902	3687	3689	3690	rBV2	1206	412	0.06%	0.007%
49	12.940	3699	3701	3703	rBV3	1217	716	0.10%	0.011%
50	13.049	3731	3735	3736	rBV5	1465	928	0.13%	0.015%
51	13.107	3752	3753	3755	rBV2	1045	505	0.07%	0.008%
52	13.207	3779	3784	3787	rBV6	3650	3940	0.57%	0.063%
53	13.445	3853	3858	3859	rBV4	3765	2720	0.39%	0.043%
54	13.490	3869	3872	3874	rBV4	2174	1522	0.22%	0.024%
55	14.065	4049	4051	4052	rBV2	986	535	0.08%	0.009%
56	14.525	4193	4194	4195	rBV	1363	472	0.07%	0.008%
57	14.815	4282	4284	4287	rBV4	1500	808	0.12%	0.013%


Sum of corrected areas: 6284469

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030707.D
Acq On : 20 Apr 2023 11:24
Operator : SY/MD
Sample : 02411-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

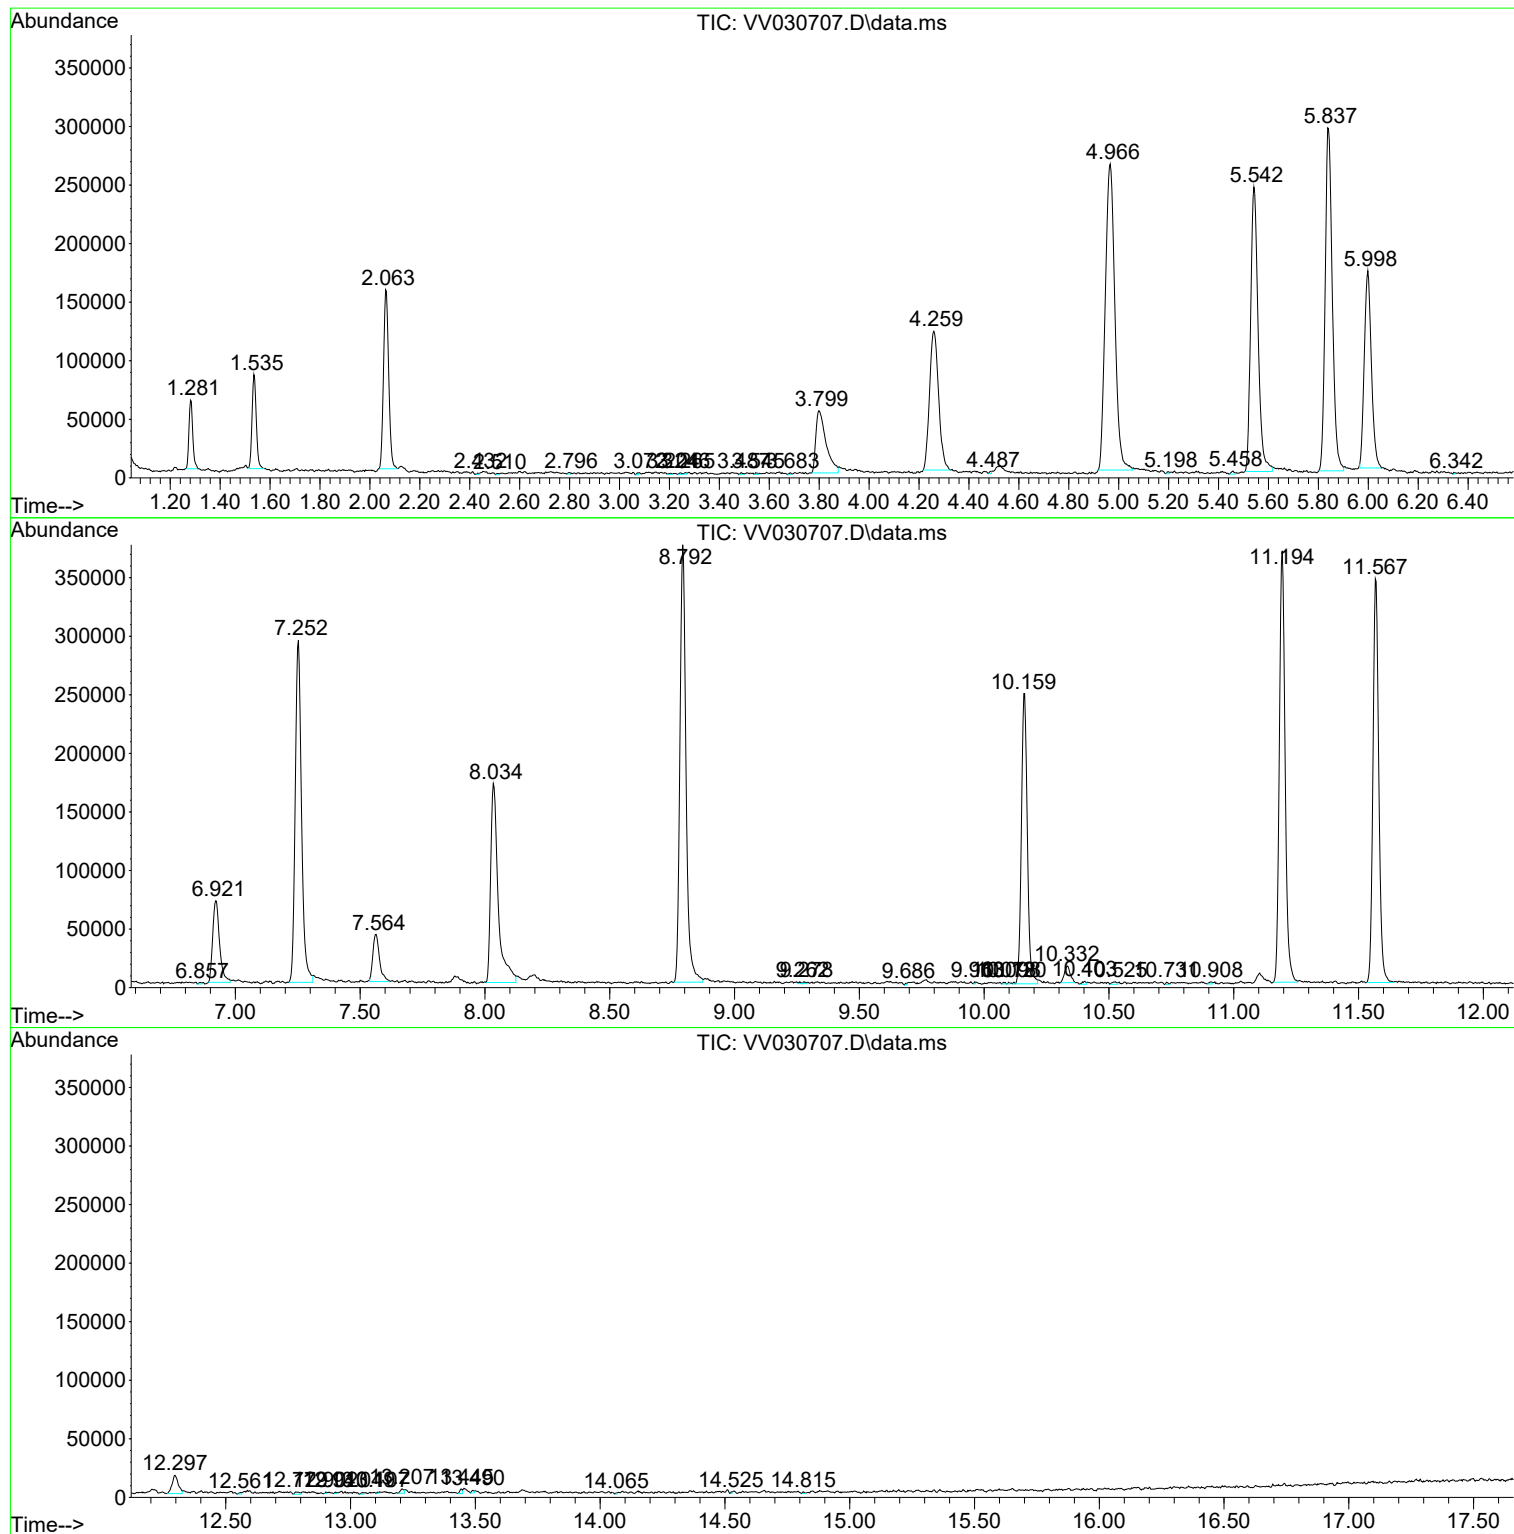

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030707.D
Acq On : 20 Apr 2023 11:24
Operator : SY/MD
Sample : 02411-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030707.D
Acq On : 20 Apr 2023 11:24
Operator : SY/MD
Sample : 02411-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc