

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030708.D
 Acq On : 20 Apr 2023 11:48
 Operator : SY/MD
 Sample : 02411-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	85	rBV	72431	78677	11.20%	1.359%
2	1.535	148	154	167	rVB	75851	88951	12.66%	1.537%
3	2.066	310	319	330	rBV	159345	221348	31.50%	3.824%
4	2.400	420	423	427	rVB5	1603	1019	0.15%	0.018%
5	2.423	427	430	433	rBV4	1489	950	0.14%	0.016%
6	2.442	433	436	438	rBV4	1780	983	0.14%	0.017%
7	2.577	476	478	480	rBV3	1437	731	0.10%	0.013%
8	2.648	498	500	504	rBV5	905	765	0.11%	0.013%
9	2.716	519	521	522	rBV2	1313	586	0.08%	0.010%
10	2.796	545	546	551	rBV5	1759	865	0.12%	0.015%
11	2.818	551	553	556	rVB4	1130	737	0.10%	0.013%
12	2.941	588	591	592	rBV3	1232	655	0.09%	0.011%
13	2.966	597	599	602	rBV4	1365	689	0.10%	0.012%
14	3.005	609	611	613	rVB3	1406	621	0.09%	0.011%
15	3.056	624	627	628	rBV3	1155	699	0.10%	0.012%
16	3.082	631	635	638	rBV5	1517	1159	0.16%	0.020%
17	3.288	695	699	702	rBV5	1898	1315	0.19%	0.023%
18	3.317	702	708	711	rBV7	1807	2258	0.32%	0.039%
19	3.413	735	738	741	rBV4	1678	1018	0.14%	0.018%
20	3.436	743	745	749	rVB4	1396	895	0.13%	0.015%
21	3.455	749	751	755	rBV6	1265	1052	0.15%	0.018%
22	3.590	790	793	794	rBV2	1786	1025	0.15%	0.018%
23	3.674	815	819	822	rBV6	1420	1091	0.16%	0.019%
24	3.699	825	827	828	rBV3	1145	566	0.08%	0.010%
25	3.796	848	857	888	rBV2	56648	166364	23.67%	2.874%
26	4.063	938	940	945	rBV6	1553	1416	0.20%	0.024%
27	4.259	983	1001	1026	rBV2	121039	315812	44.94%	5.455%
28	4.580	1099	1101	1106	rBV5	1367	907	0.13%	0.016%
29	4.696	1134	1137	1141	rBV6	1689	1349	0.19%	0.023%
30	4.783	1161	1164	1167	rBV5	1034	888	0.13%	0.015%
31	4.847	1177	1184	1187	rBV8	2132	2228	0.32%	0.038%
32	4.912	1202	1204	1205	rBV2	1339	568	0.08%	0.010%
33	4.966	1205	1221	1247	rVV3	262014	702756	100.00%	12.140%
34	5.542	1389	1400	1417	rBV	234475	477627	67.96%	8.251%
35	5.844	1482	1494	1508	rBV2	39462	83353	11.86%	1.440%
36	5.998	1531	1542	1563	rVB	164170	327125	46.55%	5.651%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030708.D
 Acq On : 20 Apr 2023 11:48
 Operator : SY/MD
 Sample : 02411-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.429	1672	1676	1681	rBV8	1511	1965	0.28%	0.034%
38	6.510	1699	1701	1705	rBV5	1362	780	0.11%	0.013%
39	6.622	1734	1736	1738	rBV3	1283	737	0.10%	0.013%
40	6.921	1818	1829	1852	rVV2	82856	161634	23.00%	2.792%
41	7.172	1903	1907	1908	rBV3	1680	1003	0.14%	0.017%
42	7.252	1920	1932	1959	rBV	278930	506561	72.08%	8.750%
43	7.561	2017	2028	2047	rBV	60584	111109	15.81%	1.919%
44	7.751	2085	2087	2091	rBV5	1262	948	0.13%	0.016%
45	7.783	2096	2097	2099	rVB2	1591	552	0.08%	0.010%
46	7.818	2104	2108	2111	rBV5	2090	1348	0.19%	0.023%
47	7.847	2115	2117	2120	rBV4	1001	858	0.12%	0.015%
48	8.034	2165	2175	2192	rBV	179878	337354	48.00%	5.828%
49	8.426	2292	2297	2299	rBV6	1245	1281	0.18%	0.022%
50	8.661	2367	2370	2373	rBV4	1781	1267	0.18%	0.022%
51	8.677	2373	2375	2376	rBV	1545	577	0.08%	0.010%
52	8.792	2400	2411	2432	rBV	363002	605931	86.22%	10.467%
53	9.226	2543	2546	2549	rBV5	1263	766	0.11%	0.013%
54	9.262	2554	2557	2559	rBV4	996	648	0.09%	0.011%
55	9.490	2626	2628	2630	rBV2	949	607	0.09%	0.010%
56	9.577	2653	2655	2660	rVB4	1537	1113	0.16%	0.019%
57	9.599	2660	2662	2664	rBV3	829	560	0.08%	0.010%
58	10.008	2787	2789	2790	rBV2	1222	644	0.09%	0.011%
59	10.030	2794	2796	2799	rVV4	2243	1393	0.20%	0.024%
60	10.043	2799	2800	2804	rVB4	2205	1112	0.16%	0.019%
61	10.069	2804	2808	2811	rBV5	1717	1219	0.17%	0.021%
62	10.159	2824	2836	2858	rBV	245917	404076	57.50%	6.980%
63	10.262	2865	2868	2872	rBV5	1686	1373	0.20%	0.024%
64	10.336	2881	2891	2900	rBV3	8778	15871	2.26%	0.274%
65	10.381	2903	2905	2908	rVB4	1756	1158	0.16%	0.020%
66	10.400	2908	2911	2912	rBV3	1095	557	0.08%	0.010%
67	10.490	2937	2939	2942	rBV4	1716	1140	0.16%	0.020%
68	10.538	2951	2954	2957	rBV4	1065	661	0.09%	0.011%
69	10.664	2989	2993	2995	rBV5	2161	1809	0.26%	0.031%
70	10.779	3024	3029	3032	rBV6	1765	1678	0.24%	0.029%
71	10.911	3068	3070	3073	rVB4	1610	907	0.13%	0.016%
72	10.940	3075	3079	3083	rBV6	1678	1746	0.25%	0.030%
73	10.985	3091	3093	3097	rBV4	1060	795	0.11%	0.014%
74	11.194	3147	3158	3178	rBV	348657	556908	79.25%	9.620%
75	11.426	3228	3230	3232	rBV3	980	623	0.09%	0.011%
76	11.471	3241	3244	3248	rBV5	1636	1391	0.20%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030708.D
 Acq On : 20 Apr 2023 11:48
 Operator : SY/MD
 Sample : 02411-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.570	3263	3275	3291	rBV	332873	538175	76.58%	9.297%
78	11.792	3342	3344	3346	rBV3	1143	558	0.08%	0.010%
79	11.921	3380	3384	3385	rBV3	1256	596	0.08%	0.010%
80	12.104	3439	3441	3443	rVB3	1351	613	0.09%	0.011%
81	12.146	3451	3454	3456	rBV4	1562	799	0.11%	0.014%
82	12.191	3465	3468	3470	rBV4	1372	942	0.13%	0.016%
83	12.519	3568	3570	3574	rVB5	1957	898	0.13%	0.016%
84	12.554	3574	3581	3583	rBV8	1941	2070	0.29%	0.036%
85	12.635	3604	3606	3609	rBV3	1141	593	0.08%	0.010%
86	12.680	3615	3620	3626	rBV9	1391	2103	0.30%	0.036%
87	12.773	3646	3649	3650	rBV3	1094	575	0.08%	0.010%
88	12.934	3695	3699	3701	rBV5	1168	918	0.13%	0.016%
89	13.082	3742	3745	3747	rBV5	1556	944	0.13%	0.016%
90	13.120	3752	3757	3759	rBV5	1906	1662	0.24%	0.029%
91	13.204	3776	3783	3787	rBV7	3660	5034	0.72%	0.087%
92	13.336	3822	3824	3826	rBV3	1987	1031	0.15%	0.018%
93	13.390	3839	3841	3845	rVB5	1280	759	0.11%	0.013%
94	13.512	3875	3879	3883	rBV6	1816	1538	0.22%	0.027%
95	13.651	3919	3922	3924	rBV4	1863	1178	0.17%	0.020%
96	13.686	3931	3933	3934	rBV2	1541	703	0.10%	0.012%
97	13.776	3956	3961	3963	rBV5	1877	1554	0.22%	0.027%
98	14.400	4149	4155	4158	rBV6	1596	2066	0.29%	0.036%
99	14.500	4184	4186	4190	rVB5	1890	1143	0.16%	0.020%
100	14.532	4194	4196	4200	rVB5	1398	819	0.12%	0.014%




Sum of corrected areas: 5788979

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030708.D
Acq On : 20 Apr 2023 11:48
Operator : SY/MD
Sample : 02411-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

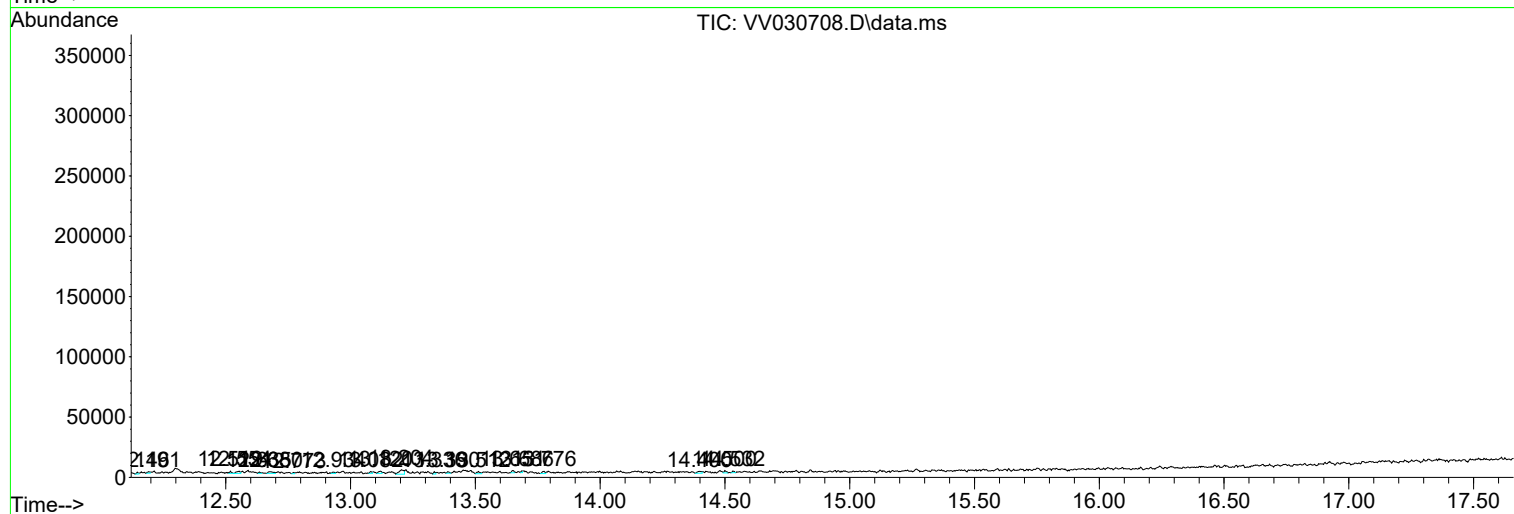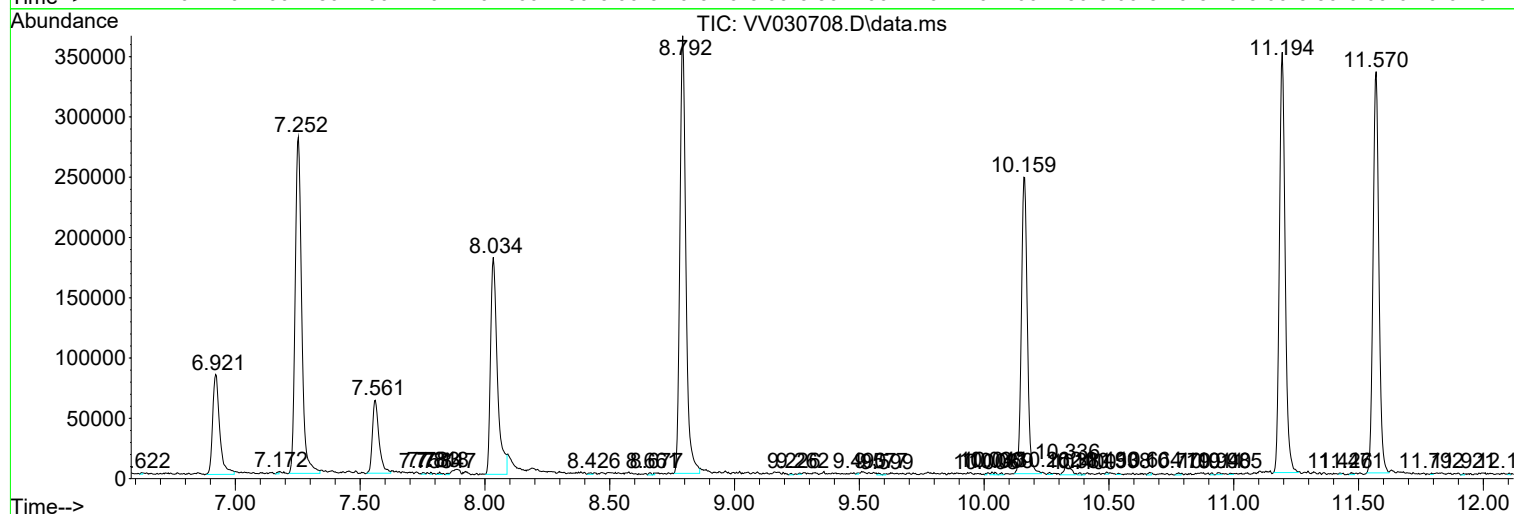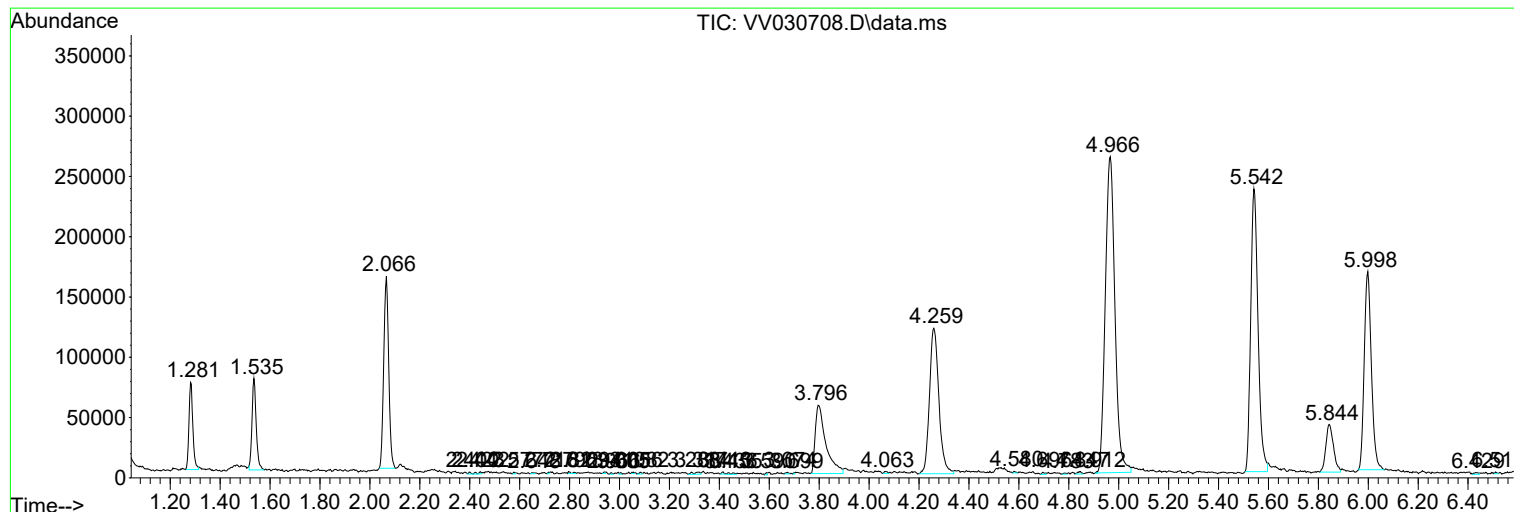

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030708.D
Acq On : 20 Apr 2023 11:48
Operator : SY/MD
Sample : 02411-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030708.D
Acq On : 20 Apr 2023 11:48
Operator : SY/MD
Sample : 02411-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc