

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030709.D
 Acq On : 20 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02411-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	75817	79726	11.25%	1.351%
2	1.535	147	154	168	rVB	81939	97051	13.70%	1.644%
3	2.066	310	319	333	rBV	153747	224680	31.71%	3.807%
4	2.378	414	416	419	rVB4	1464	621	0.09%	0.011%
5	2.696	511	515	517	rVB5	966	642	0.09%	0.011%
6	2.760	532	535	538	rBV4	1897	1435	0.20%	0.024%
7	2.818	550	553	559	rBV7	970	1067	0.15%	0.018%
8	2.895	573	577	580	rBV5	1534	981	0.14%	0.017%
9	2.928	584	587	590	rVB5	1431	787	0.11%	0.013%
10	2.947	590	593	595	rBV4	1716	1300	0.18%	0.022%
11	2.985	601	605	608	rBV6	941	728	0.10%	0.012%
12	3.063	624	629	631	rBV6	1312	1221	0.17%	0.021%
13	3.140	651	653	656	rBV4	1010	650	0.09%	0.011%
14	3.178	662	665	666	rBV3	1364	723	0.10%	0.012%
15	3.339	710	715	717	rBV6	1763	1454	0.21%	0.025%
16	3.522	770	772	777	rBV5	1356	965	0.14%	0.016%
17	3.561	780	784	787	rBV6	1438	1204	0.17%	0.020%
18	3.584	788	791	794	rBV4	1185	652	0.09%	0.011%
19	3.799	848	858	881	rBV	56470	156636	22.11%	2.654%
20	4.172	971	974	977	rBV5	1366	1112	0.16%	0.019%
21	4.259	988	1001	1020	rBV2	119379	295682	41.74%	5.010%
22	4.725	1142	1146	1149	rBV5	1103	997	0.14%	0.017%
23	4.870	1188	1191	1194	rBV4	1429	926	0.13%	0.016%
24	4.966	1204	1221	1248	rBV2	265172	708448	100.00%	12.004%
25	5.542	1388	1400	1425	rBV	243380	515803	72.81%	8.740%
26	5.844	1482	1494	1513	rBV5	27059	61095	8.62%	1.035%
27	5.998	1527	1542	1559	rBV	167587	349207	49.29%	5.917%
28	6.265	1623	1625	1628	rBV3	1405	779	0.11%	0.013%
29	6.345	1648	1650	1652	rBV4	1993	863	0.12%	0.015%
30	6.400	1661	1667	1669	rBV7	1304	1431	0.20%	0.024%
31	6.458	1682	1685	1687	rBV4	1487	1000	0.14%	0.017%
32	6.548	1712	1713	1716	rBV3	1201	639	0.09%	0.011%
33	6.632	1731	1739	1740	rBV6	1997	2321	0.33%	0.039%
34	6.921	1818	1829	1850	rBV	84255	161625	22.81%	2.739%
35	7.072	1873	1876	1878	rBV4	1402	867	0.12%	0.015%
36	7.252	1920	1932	1952	rBV	281053	507456	71.63%	8.598%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030709.D
 Acq On : 20 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02411-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.455	1993	1995	1997	rBV3	1320	656	0.09%	0.011%
38	7.561	2020	2028	2049	rVB2	58281	102749	14.50%	1.741%
39	7.683	2063	2066	2068	rBV3	2347	1323	0.19%	0.022%
40	7.767	2090	2092	2095	rBV3	1400	1031	0.15%	0.017%
41	8.033	2166	2175	2210	rBV	180799	366778	51.77%	6.215%
42	8.416	2292	2294	2296	rBV2	1881	1008	0.14%	0.017%
43	8.728	2386	2391	2395	rBV7	1944	1901	0.27%	0.032%
44	8.792	2400	2411	2433	rVV	372308	638941	90.19%	10.826%
45	9.185	2531	2533	2534	rBV2	1609	642	0.09%	0.011%
46	9.255	2552	2555	2558	rBV5	1216	887	0.13%	0.015%
47	9.275	2558	2561	2564	rVB5	1698	1103	0.16%	0.019%
48	9.300	2564	2569	2572	rBV5	1355	1201	0.17%	0.020%
49	9.384	2593	2595	2598	rBV3	1298	844	0.12%	0.014%
50	9.464	2616	2620	2621	rBV4	1903	1255	0.18%	0.021%
51	9.506	2631	2633	2639	rBV7	1160	1497	0.21%	0.025%
52	9.631	2669	2672	2674	rBV4	1460	843	0.12%	0.014%
53	9.689	2688	2690	2693	rBV3	1551	860	0.12%	0.015%
54	9.831	2727	2734	2736	rBV9	1503	1988	0.28%	0.034%
55	9.844	2736	2738	2741	rVV4	1830	1015	0.14%	0.017%
56	9.876	2743	2748	2751	rVB7	1786	1870	0.26%	0.032%
57	9.911	2756	2759	2762	rVV5	1424	950	0.13%	0.016%
58	10.004	2785	2788	2789	rBV3	1124	777	0.11%	0.013%
59	10.072	2806	2809	2812	rBV4	1283	1029	0.15%	0.017%
60	10.162	2826	2837	2855	rVB	249342	401398	56.66%	6.801%
61	10.332	2884	2890	2891	rBV4	5430	4804	0.68%	0.081%
62	10.397	2908	2910	2914	rBV4	1943	1214	0.17%	0.021%
63	10.422	2914	2918	2922	rVV6	2128	1792	0.25%	0.030%
64	10.455	2924	2928	2931	rVV4	1282	953	0.13%	0.016%
65	10.538	2950	2954	2955	rBV3	1295	944	0.13%	0.016%
66	10.631	2980	2983	2986	rBV5	1068	751	0.11%	0.013%
67	10.895	3061	3065	3069	rVB6	2127	1625	0.23%	0.028%
68	10.950	3080	3082	3087	rVB6	1011	635	0.09%	0.011%
69	11.049	3107	3113	3114	rBV5	1730	1515	0.21%	0.026%
70	11.104	3128	3130	3133	rBV4	1226	788	0.11%	0.013%
71	11.123	3133	3136	3137	rBV4	2354	947	0.13%	0.016%
72	11.194	3144	3158	3176	rBV	370442	596923	84.26%	10.114%
73	11.374	3211	3214	3219	rVB5	1817	1572	0.22%	0.027%
74	11.471	3241	3244	3247	rBV3	1172	851	0.12%	0.014%
75	11.570	3264	3275	3292	rBV	335589	545169	76.95%	9.237%
76	11.744	3325	3329	3332	rBV6	1803	1537	0.22%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030709.D
 Acq On : 20 Apr 2023 12:12
 Operator : SY/MD
 Sample : 02411-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.795	3343	3345	3350	rBV6	1138	760	0.11%	0.013%
78	11.837	3356	3358	3363	rVB4	1795	1183	0.17%	0.020%
79	11.873	3364	3369	3372	rVB6	1480	1151	0.16%	0.020%
80	11.914	3379	3382	3387	rBV7	1938	1825	0.26%	0.031%
81	12.037	3417	3420	3422	rBV4	1449	936	0.13%	0.016%
82	12.069	3428	3430	3433	rBV3	947	649	0.09%	0.011%
83	12.130	3445	3449	3451	rBV4	944	718	0.10%	0.012%
84	12.348	3513	3517	3521	rBV7	1611	1366	0.19%	0.023%
85	12.445	3545	3547	3553	rBV6	912	694	0.10%	0.012%
86	12.528	3569	3573	3576	rBV6	1767	1468	0.21%	0.025%
87	12.580	3586	3589	3591	rBV3	1197	869	0.12%	0.015%
88	12.670	3614	3617	3619	rBV4	1016	753	0.11%	0.013%
89	12.782	3649	3652	3655	rBB4	918	633	0.09%	0.011%
90	12.844	3668	3671	3673	rBV4	1357	847	0.12%	0.014%
91	12.969	3707	3710	3713	rVB6	1150	789	0.11%	0.013%
92	13.149	3764	3766	3769	rVV4	1221	905	0.13%	0.015%
93	13.172	3769	3773	3777	rVB6	1601	1370	0.19%	0.023%
94	13.339	3821	3825	3828	rBV5	2080	1800	0.25%	0.030%
95	13.442	3854	3857	3858	rBV3	1648	982	0.14%	0.017%
96	13.557	3891	3893	3896	rBV4	999	664	0.09%	0.011%
97	13.734	3943	3948	3949	rBV5	1410	808	0.11%	0.014%
98	13.969	4018	4021	4024	rVB5	1885	1077	0.15%	0.018%
99	14.033	4037	4041	4045	rVV7	1320	1350	0.19%	0.023%
100	15.159	4389	4391	4393	rBV3	1798	1004	0.14%	0.017%




Sum of corrected areas: 5901941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030709.D
Acq On : 20 Apr 2023 12:12
Operator : SY/MD
Sample : 02411-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

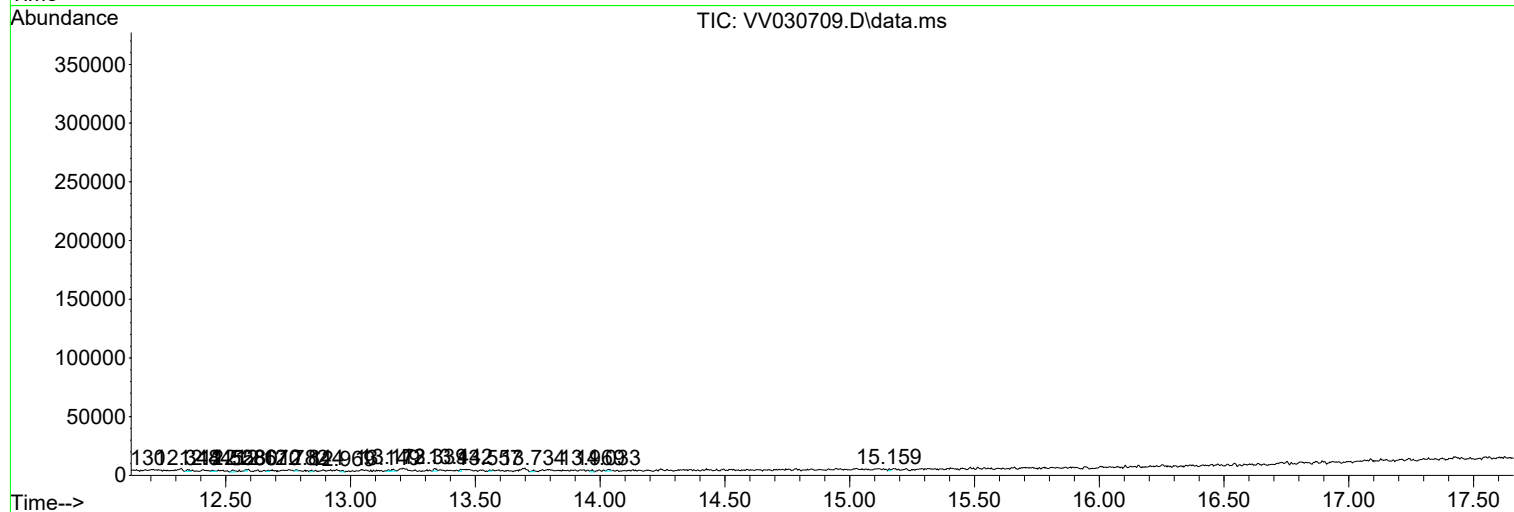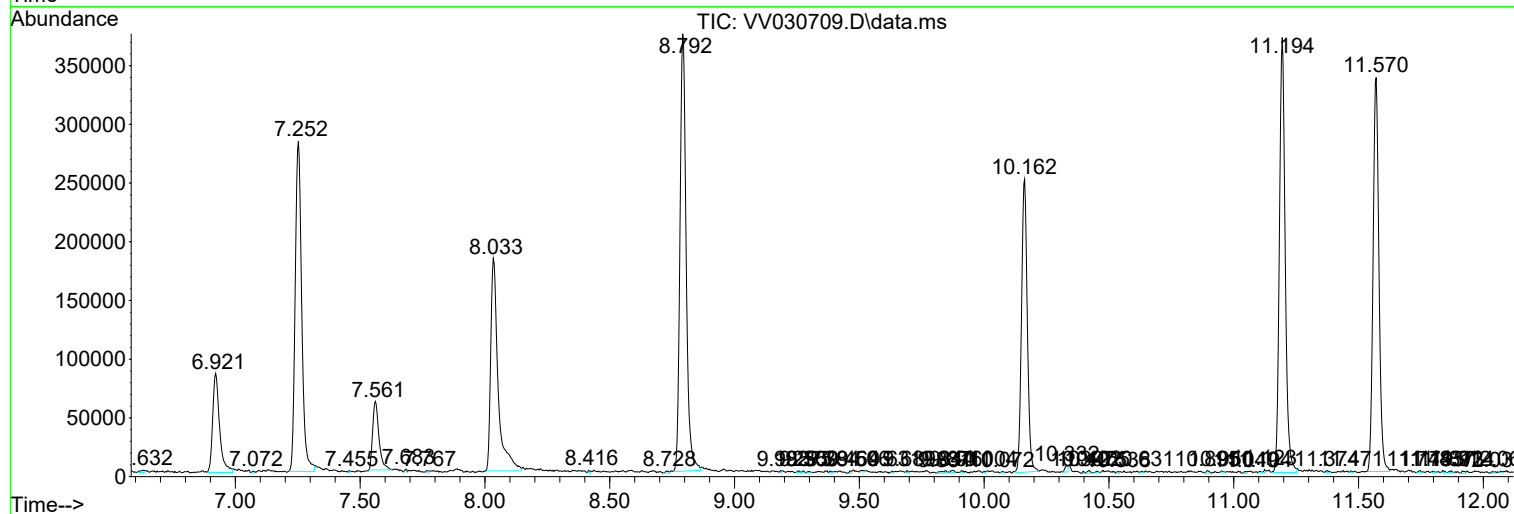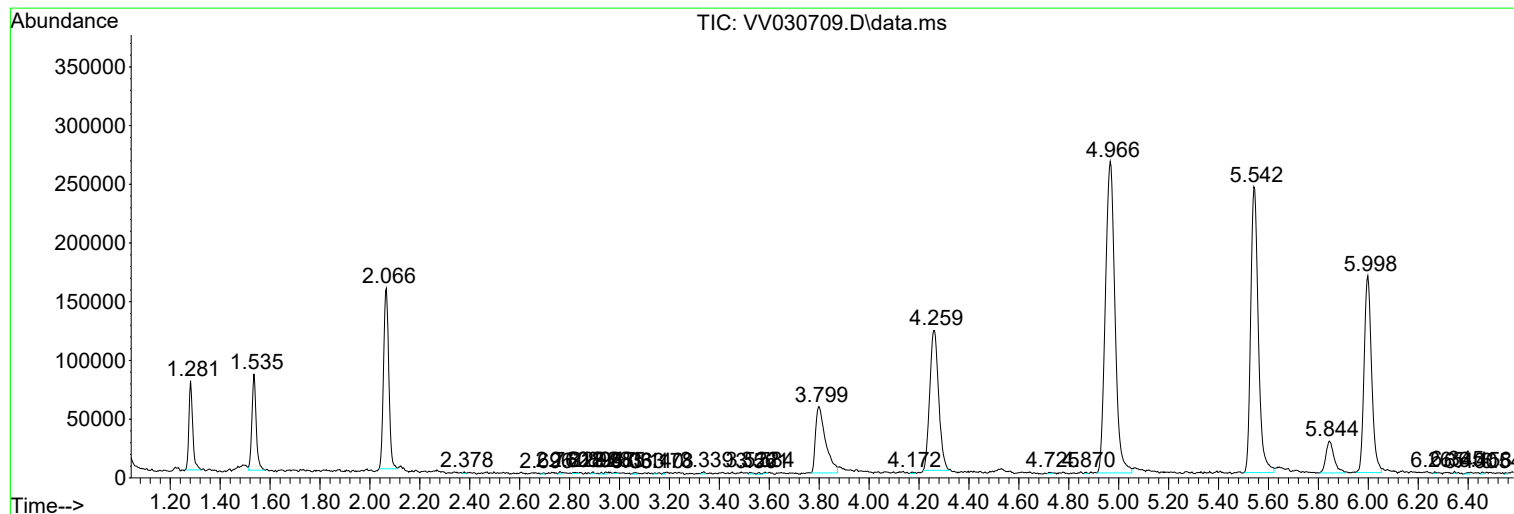

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030709.D
Acq On : 20 Apr 2023 12:12
Operator : SY/MD
Sample : 02411-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030709.D
Acq On : 20 Apr 2023 12:12
Operator : SY/MD
Sample : 02411-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc