

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030710.D
 Acq On : 20 Apr 2023 12:36
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rVB	118686	132694	16.49%	2.147%
2	1.536	148	154	165	rVB	98335	118414	14.72%	1.916%
3	2.066	310	319	332	rBV	215913	313117	38.91%	5.065%
4	2.388	414	419	420	rBV6	1845	1606	0.20%	0.026%
5	2.629	489	494	497	rBV5	1507	1468	0.18%	0.024%
6	2.738	524	528	530	rBV5	1364	938	0.12%	0.015%
7	2.777	536	540	541	rBV2	1183	917	0.11%	0.015%
8	2.790	541	544	550	rVB7	1465	1438	0.18%	0.023%
9	2.970	598	600	604	rVB5	1661	818	0.10%	0.013%
10	3.044	622	623	626	rVB3	1576	692	0.09%	0.011%
11	3.063	626	629	634	rBV6	2121	2174	0.27%	0.035%
12	3.085	634	636	640	rVB6	1294	733	0.09%	0.012%
13	3.163	658	660	662	rBV3	1056	694	0.09%	0.011%
14	3.237	680	683	686	rVB5	1597	790	0.10%	0.013%
15	3.465	749	754	755	rBV5	1670	1343	0.17%	0.022%
16	3.651	809	812	816	rVB5	1078	708	0.09%	0.011%
17	3.677	816	820	823	rBV6	1648	1224	0.15%	0.020%
18	3.764	841	847	848	rBV5	1643	1268	0.16%	0.021%
19	3.799	848	858	885	rVV	52573	160676	19.97%	2.599%
20	4.259	985	1001	1028	rBV	130198	332140	41.27%	5.373%
21	4.719	1140	1144	1145	rBV4	1363	839	0.10%	0.014%
22	4.841	1178	1182	1184	rBV4	1142	927	0.12%	0.015%
23	4.905	1197	1202	1204	rBV6	1859	1571	0.20%	0.025%
24	4.966	1204	1221	1246	rVV2	304642	804712	100.00%	13.017%
25	5.256	1309	1311	1313	rBV3	1670	925	0.11%	0.015%
26	5.542	1388	1400	1420	rBV	197987	412215	51.23%	6.668%
27	5.841	1480	1493	1515	rBV2	122502	255835	31.79%	4.139%
28	5.998	1531	1542	1558	rBV	172730	344800	42.85%	5.578%
29	6.384	1660	1662	1666	rVB5	1792	1116	0.14%	0.018%
30	6.410	1666	1670	1671	rBV4	1363	1024	0.13%	0.017%
31	6.449	1680	1682	1686	rVB4	1453	754	0.09%	0.012%
32	6.539	1707	1710	1712	rBV3	1581	912	0.11%	0.015%
33	6.568	1716	1719	1720	rBV3	1378	767	0.10%	0.012%
34	6.812	1788	1795	1799	rBV9	2024	2577	0.32%	0.042%
35	6.847	1803	1806	1810	rBV6	1850	1811	0.23%	0.029%
36	6.921	1818	1829	1848	rBV	92858	179221	22.27%	2.899%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030710.D
 Acq On : 20 Apr 2023 12:36
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.031	1861	1863	1866	rBV3	1418	716	0.09%	0.012%
38	7.252	1918	1932	1953	rBV	341351	614023	76.30%	9.933%
39	7.474	1999	2001	2002	rBV2	1761	790	0.10%	0.013%
40	7.561	2017	2028	2042	rBV2	68730	124445	15.46%	2.013%
41	7.677	2062	2064	2070	rVB7	1830	1197	0.15%	0.019%
42	8.034	2166	2175	2206	rBV	165784	338248	42.03%	5.472%
43	8.400	2285	2289	2294	rBV6	1999	1529	0.19%	0.025%
44	8.654	2366	2368	2371	rBV3	1292	795	0.10%	0.013%
45	8.793	2400	2411	2432	rBV	304203	517643	64.33%	8.374%
46	8.957	2460	2462	2463	rBV2	1532	726	0.09%	0.012%
47	9.002	2472	2476	2478	rBV4	1212	884	0.11%	0.014%
48	9.053	2489	2492	2495	rBV5	1030	902	0.11%	0.015%
49	9.095	2502	2505	2510	rBV7	1274	1271	0.16%	0.021%
50	9.297	2566	2568	2571	rBV5	1526	764	0.09%	0.012%
51	9.449	2613	2615	2620	rVB4	1599	927	0.12%	0.015%
52	9.481	2620	2625	2627	rBV6	1319	1107	0.14%	0.018%
53	9.953	2770	2772	2774	rBV3	1255	749	0.09%	0.012%
54	10.056	2800	2804	2806	rBV4	1155	863	0.11%	0.014%
55	10.092	2811	2815	2816	rBV4	1238	968	0.12%	0.016%
56	10.162	2825	2837	2854	rBV	239378	383851	47.70%	6.209%
57	10.387	2903	2907	2910	rBV6	1958	2116	0.26%	0.034%
58	10.481	2933	2936	2939	rBV5	1046	838	0.10%	0.014%
59	10.529	2947	2951	2956	rBV6	1414	1592	0.20%	0.026%
60	10.751	3016	3020	3026	rBV8	1646	1337	0.17%	0.022%
61	10.831	3043	3045	3049	rVB5	1182	805	0.10%	0.013%
62	10.976	3087	3090	3092	rBV4	1604	835	0.10%	0.014%
63	10.998	3092	3097	3100	rBV7	1405	1113	0.14%	0.018%
64	11.194	3146	3158	3177	rBV	307552	495590	61.59%	8.017%
65	11.571	3264	3275	3291	rVB	348607	560938	69.71%	9.074%
66	11.902	3374	3378	3380	rBV5	1364	1056	0.13%	0.017%
67	11.953	3393	3394	3399	rBV5	1448	899	0.11%	0.015%
68	12.037	3416	3420	3421	rBV4	1449	1182	0.15%	0.019%
69	12.120	3445	3446	3452	rBV6	1325	1283	0.16%	0.021%
70	12.204	3469	3472	3474	rBV4	1285	739	0.09%	0.012%
71	12.493	3557	3562	3565	rBV6	1498	1505	0.19%	0.024%
72	12.545	3576	3578	3580	rBV2	1215	733	0.09%	0.012%
73	12.577	3583	3588	3590	rBV5	1231	1088	0.14%	0.018%
74	12.596	3590	3594	3598	rBV6	2058	1871	0.23%	0.030%
75	12.751	3639	3642	3645	rBV4	1025	817	0.10%	0.013%
76	12.792	3651	3655	3657	rVB4	966	745	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030710.D
 Acq On : 20 Apr 2023 12:36
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.844	3668	3671	3672	rBV3	1125	731	0.09%	0.012%
78	12.876	3678	3681	3684	rBV5	1124	963	0.12%	0.016%
79	12.911	3690	3692	3696	rVB5	1481	992	0.12%	0.016%
80	13.017	3721	3725	3728	rVB5	1125	790	0.10%	0.013%
81	13.072	3740	3742	3746	rBV4	1766	1495	0.19%	0.024%
82	13.108	3750	3753	3757	rBV6	1610	1325	0.16%	0.021%
83	13.252	3797	3798	3801	rBV3	1263	740	0.09%	0.012%
84	13.333	3820	3823	3826	rBV3	1379	729	0.09%	0.012%
85	13.352	3826	3829	3830	rBV2	1382	864	0.11%	0.014%
86	13.448	3853	3859	3862	rBV7	2854	3263	0.41%	0.053%
87	13.574	3896	3898	3901	rBV4	1839	1132	0.14%	0.018%
88	13.686	3927	3933	3937	rBV9	2019	2055	0.26%	0.033%
89	13.747	3949	3952	3953	rBV3	1446	962	0.12%	0.016%
90	13.969	4019	4021	4024	rBV4	1234	788	0.10%	0.013%
91	14.034	4037	4041	4042	rBV5	1182	868	0.11%	0.014%
92	14.107	4061	4064	4068	rBV4	1321	1009	0.13%	0.016%
93	14.191	4087	4090	4093	rVB4	2091	1176	0.15%	0.019%
94	14.249	4104	4108	4110	rBV6	913	727	0.09%	0.012%
95	14.291	4118	4121	4124	rBV5	1624	1217	0.15%	0.020%
96	14.333	4132	4134	4140	rBV7	1489	1737	0.22%	0.028%
97	14.538	4195	4198	4201	rBV5	1443	938	0.12%	0.015%
98	14.638	4225	4229	4232	rBV5	1827	1814	0.23%	0.029%
99	14.728	4254	4257	4261	rBV4	1288	1213	0.15%	0.020%
100	15.410	4466	4469	4470	rBV3	1615	957	0.12%	0.015%




Sum of corrected areas: 6181823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030710.D
Acq On : 20 Apr 2023 12:36
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

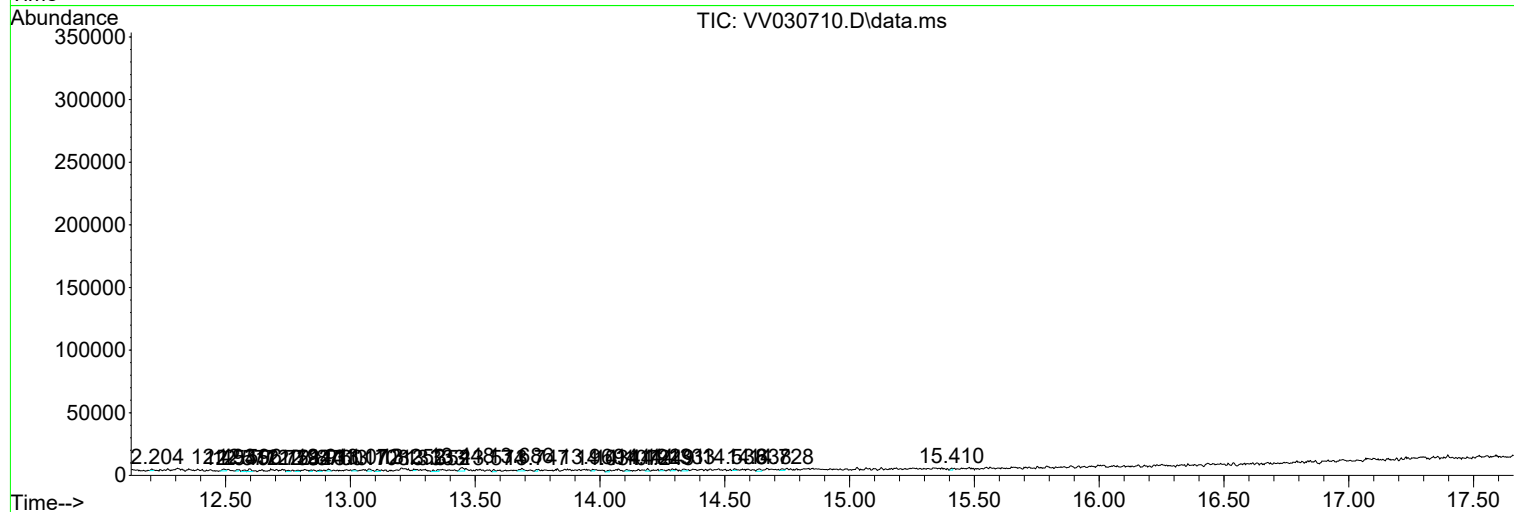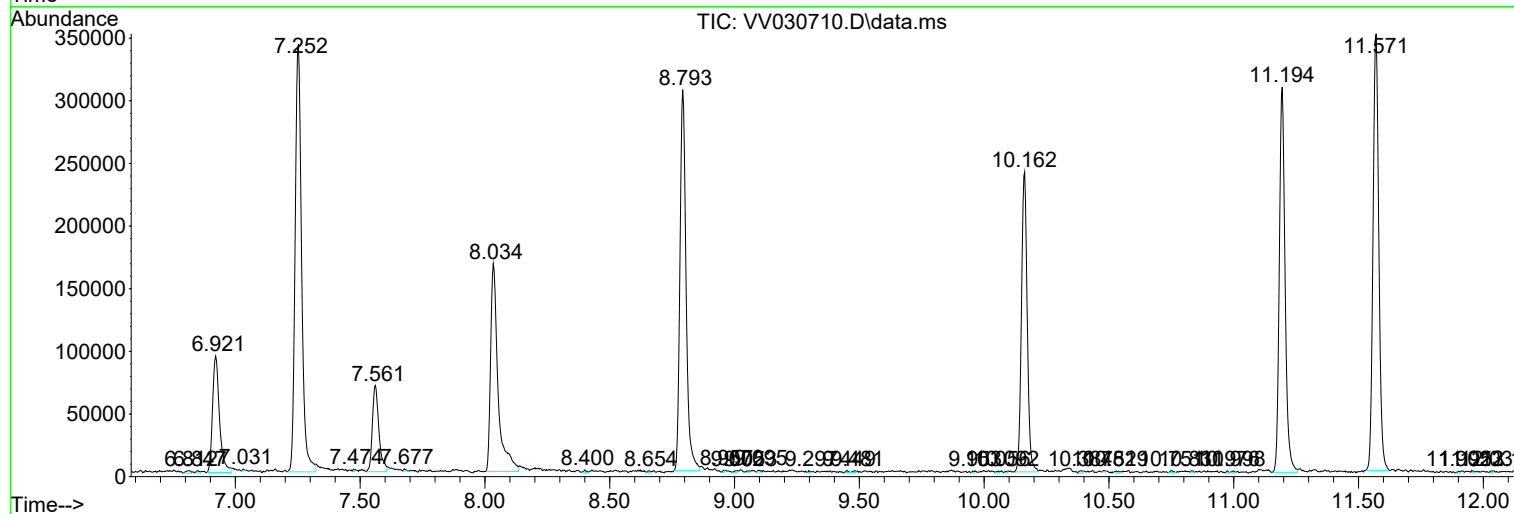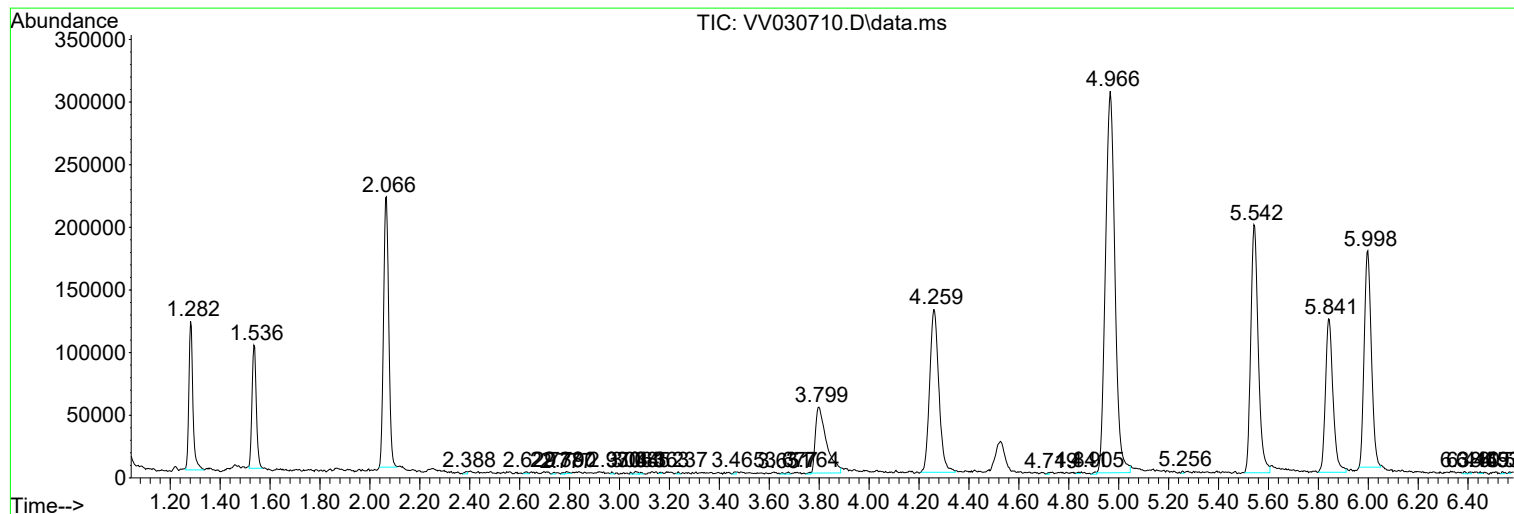

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030710.D
Acq On : 20 Apr 2023 12:36
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030710.D
Acq On : 20 Apr 2023 12:36
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc