

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030712.D
 Acq On : 20 Apr 2023 13:24
 Operator : SY/MD
 Sample : 02411-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rVB	121213	128440	16.11%	2.083%
2	1.535	148	154	166	rVB	109801	129194	16.20%	2.095%
3	2.063	310	318	334	rVB	212981	309662	38.84%	5.021%
4	2.207	362	363	368	rVB4	2163	1202	0.15%	0.019%
5	2.526	459	462	466	rBV4	1469	1034	0.13%	0.017%
6	2.667	505	506	508	rBV2	1244	539	0.07%	0.009%
7	2.683	509	511	514	rVV3	1207	744	0.09%	0.012%
8	2.699	514	516	517	rBV2	1423	542	0.07%	0.009%
9	2.905	572	580	582	rBV8	1496	1849	0.23%	0.030%
10	2.953	593	595	597	rBV3	1484	584	0.07%	0.009%
11	3.005	609	611	615	rBV5	867	580	0.07%	0.009%
12	3.285	695	698	699	rBV2	1077	596	0.07%	0.010%
13	3.304	701	704	706	rBV3	1504	866	0.11%	0.014%
14	3.336	711	714	717	rBV5	1449	1197	0.15%	0.019%
15	3.433	742	744	748	rVB4	1556	616	0.08%	0.010%
16	3.471	753	756	759	rBV5	1456	1011	0.13%	0.016%
17	3.510	766	768	772	rBV5	1243	1009	0.13%	0.016%
18	3.619	798	802	805	rBV6	1688	1303	0.16%	0.021%
19	3.664	810	816	818	rVB6	1391	1048	0.13%	0.017%
20	3.725	834	835	838	rBV2	1084	596	0.07%	0.010%
21	3.805	850	860	884	rBV2	47050	137887	17.29%	2.236%
22	4.259	988	1001	1024	rVB	126699	322445	40.44%	5.229%
23	4.670	1127	1129	1132	rVB4	1562	676	0.08%	0.011%
24	4.777	1160	1162	1164	rBV3	953	580	0.07%	0.009%
25	4.863	1187	1189	1194	rVB6	1356	803	0.10%	0.013%
26	4.966	1205	1221	1244	rBV2	300639	797325	100.00%	12.929%
27	5.481	1378	1381	1386	rBV5	1652	1650	0.21%	0.027%
28	5.542	1388	1400	1421	rBV2	248307	521672	65.43%	8.459%
29	5.998	1530	1542	1562	rBV	173505	356290	44.69%	5.778%
30	6.201	1603	1605	1607	rBV3	1444	808	0.10%	0.013%
31	6.378	1656	1660	1661	rBV4	1295	685	0.09%	0.011%
32	6.603	1726	1730	1732	rBV5	1142	877	0.11%	0.014%
33	6.921	1819	1829	1851	rBV	90984	173201	21.72%	2.809%
34	7.252	1920	1932	1955	rBV	332432	601938	75.49%	9.761%
35	7.561	2020	2028	2044	rBV	63858	109093	13.68%	1.769%
36	7.712	2073	2075	2077	rBV3	1618	790	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030712.D
 Acq On : 20 Apr 2023 13:24
 Operator : SY/MD
 Sample : 02411-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.741	2082	2084	2090	rVB6	1570	1212	0.15%	0.020%
38	7.767	2090	2092	2094	rBV2	1579	925	0.12%	0.015%
39	7.841	2113	2115	2119	rVB5	1108	692	0.09%	0.011%
40	7.947	2146	2148	2150	rBV2	1028	581	0.07%	0.009%
41	8.037	2166	2176	2206	rBV	157712	325333	40.80%	5.276%
42	8.403	2288	2290	2292	rBV3	1537	708	0.09%	0.011%
43	8.680	2374	2376	2380	rVB5	1286	636	0.08%	0.010%
44	8.792	2400	2411	2431	rVV	379201	651187	81.67%	10.560%
45	9.172	2526	2529	2530	rBV3	1234	537	0.07%	0.009%
46	9.262	2554	2557	2560	rBV5	1645	1226	0.15%	0.020%
47	9.368	2587	2590	2594	rBV6	2365	1854	0.23%	0.030%
48	9.407	2600	2602	2604	rBV2	1608	870	0.11%	0.014%
49	9.452	2614	2616	2618	rVB3	1573	664	0.08%	0.011%
50	9.490	2626	2628	2631	rBV4	1426	801	0.10%	0.013%
51	9.574	2651	2654	2655	rBV3	1375	596	0.07%	0.010%
52	9.960	2771	2774	2776	rBV3	2047	1299	0.16%	0.021%
53	10.072	2807	2809	2812	rBV3	1564	890	0.11%	0.014%
54	10.162	2825	2837	2856	rBV	235609	379385	47.58%	6.152%
55	10.294	2875	2878	2879	rBV3	1244	587	0.07%	0.010%
56	10.410	2911	2914	2920	rBV8	1558	1595	0.20%	0.026%
57	10.734	3013	3015	3017	rBV3	1245	748	0.09%	0.012%
58	10.812	3033	3039	3040	rBV6	1208	1335	0.17%	0.022%
59	10.844	3044	3049	3051	rBV4	1446	1115	0.14%	0.018%
60	10.972	3087	3089	3094	rVB6	1467	1166	0.15%	0.019%
61	11.079	3120	3122	3127	rBV7	1805	1406	0.18%	0.023%
62	11.111	3127	3132	3135	rBV6	2701	2672	0.34%	0.043%
63	11.194	3147	3158	3176	rBV	368769	593960	74.49%	9.632%
64	11.570	3264	3275	3293	rVB	343176	547718	68.69%	8.882%
65	11.722	3319	3322	3323	rBV3	1482	806	0.10%	0.013%
66	11.834	3355	3357	3359	rBV2	1798	733	0.09%	0.012%
67	11.850	3359	3362	3364	rBV3	1306	732	0.09%	0.012%
68	11.882	3369	3372	3373	rBV3	1204	671	0.08%	0.011%
69	12.072	3429	3431	3433	rBV2	1215	766	0.10%	0.012%
70	12.104	3439	3441	3443	rBV3	1174	705	0.09%	0.011%
71	12.152	3454	3456	3459	rBV4	894	636	0.08%	0.010%
72	12.474	3551	3556	3557	rBV5	1480	1175	0.15%	0.019%
73	12.532	3572	3574	3576	rBV3	1572	679	0.09%	0.011%
74	12.638	3603	3607	3610	rBV5	1621	1726	0.22%	0.028%
75	12.677	3614	3619	3621	rBV5	1569	1659	0.21%	0.027%
76	12.705	3626	3628	3630	rVB3	1920	770	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030712.D
 Acq On : 20 Apr 2023 13:24
 Operator : SY/MD
 Sample : 02411-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.792	3651	3655	3657	rBV4	1484	1083	0.14%	0.018%
78	12.876	3680	3681	3685	rVB3	1262	629	0.08%	0.010%
79	12.911	3690	3692	3696	rBV5	1369	660	0.08%	0.011%
80	12.934	3696	3699	3701	rBV4	1333	628	0.08%	0.010%
81	12.969	3706	3710	3712	rVB4	2453	1692	0.21%	0.027%
82	12.985	3712	3715	3718	rBV5	2645	2301	0.29%	0.037%
83	13.088	3744	3747	3749	rVB4	1405	689	0.09%	0.011%
84	13.181	3773	3776	3777	rBV4	1023	557	0.07%	0.009%
85	13.281	3803	3807	3813	rBV8	1432	1617	0.20%	0.026%
86	13.320	3816	3819	3822	rBV5	1291	857	0.11%	0.014%
87	13.374	3834	3836	3839	rVB4	1339	669	0.08%	0.011%
88	13.461	3861	3863	3867	rVB4	2059	907	0.11%	0.015%
89	13.635	3915	3917	3921	rVB5	1260	888	0.11%	0.014%
90	13.657	3921	3924	3927	rBV5	2004	1370	0.17%	0.022%
91	13.689	3932	3934	3936	rBV3	1766	807	0.10%	0.013%
92	13.763	3955	3957	3958	rBV2	1479	607	0.08%	0.010%
93	13.998	4026	4030	4031	rBV4	1630	1269	0.16%	0.021%
94	14.107	4059	4064	4065	rBV5	1328	1061	0.13%	0.017%
95	14.217	4095	4098	4100	rBV4	1652	988	0.12%	0.016%
96	14.422	4160	4162	4167	rBV5	840	830	0.10%	0.013%
97	14.490	4180	4183	4186	rBV5	1981	1495	0.19%	0.024%
98	14.805	4279	4281	4285	rBV4	1372	803	0.10%	0.013%
99	15.011	4343	4345	4347	rBV3	1279	581	0.07%	0.009%
100	15.065	4358	4362	4366	rBV6	2003	1684	0.21%	0.027%




Sum of corrected areas: 6166760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030712.D
Acq On : 20 Apr 2023 13:24
Operator : SY/MD
Sample : 02411-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

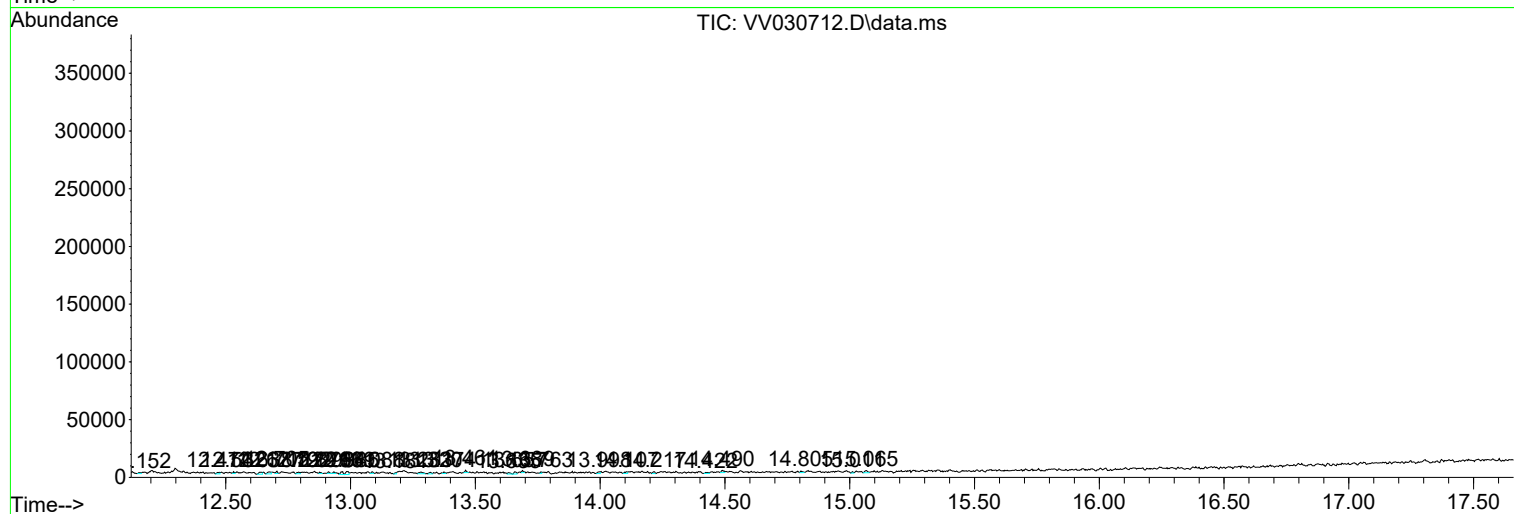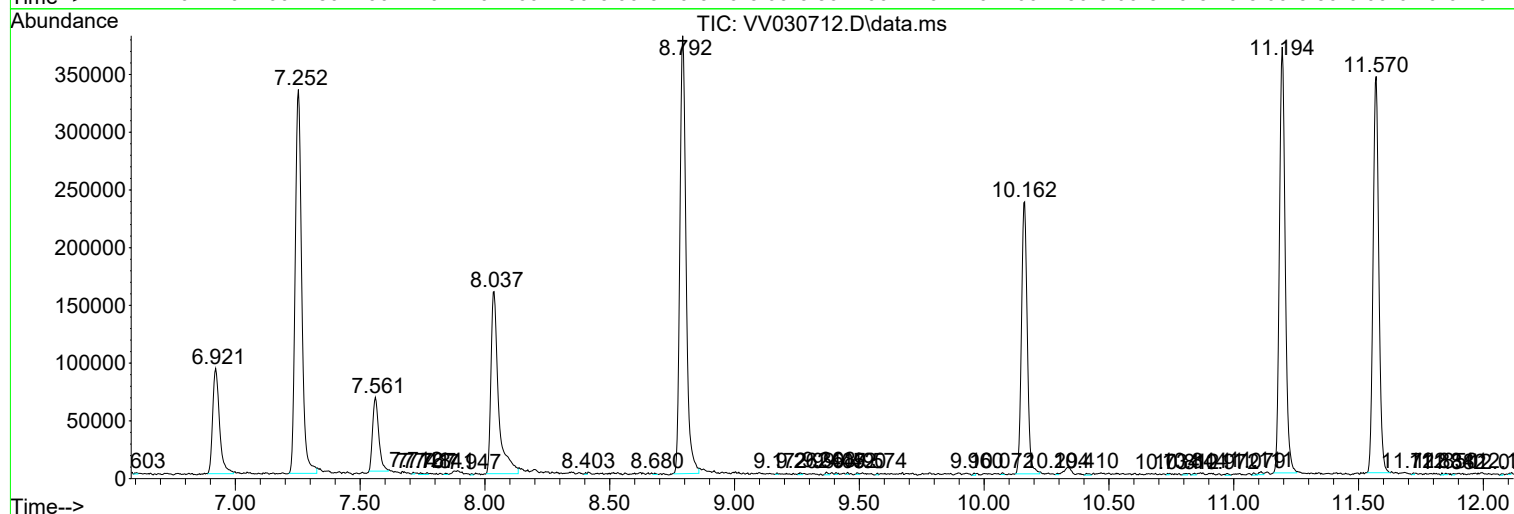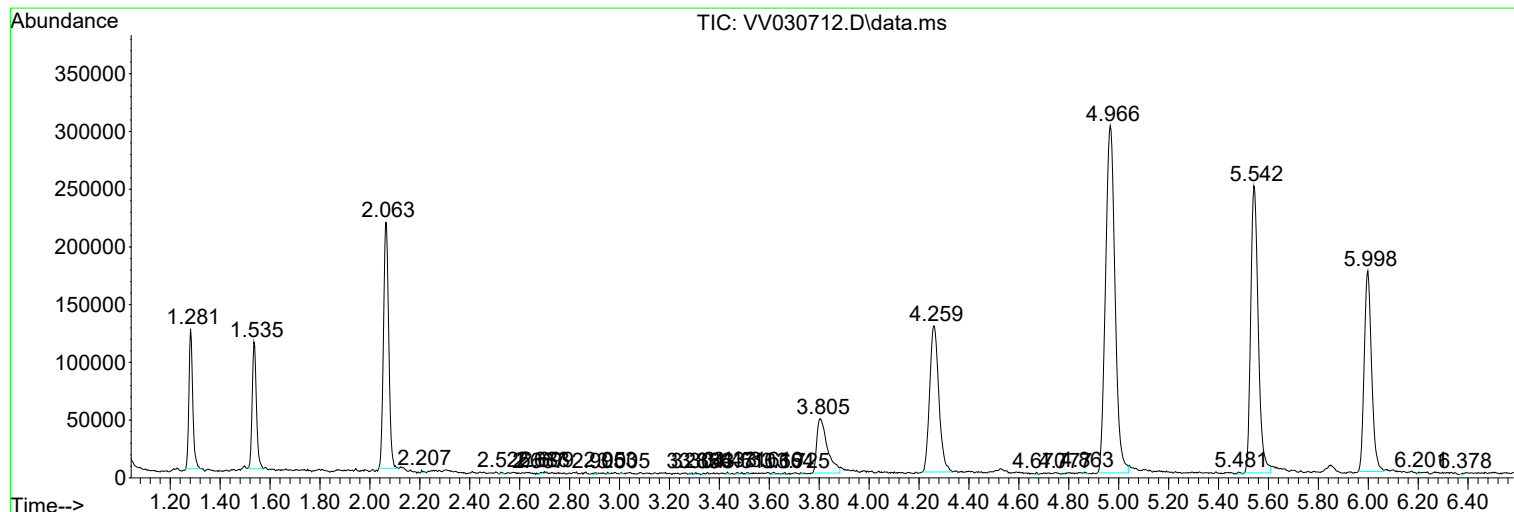

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030712.D
Acq On : 20 Apr 2023 13:24
Operator : SY/MD
Sample : 02411-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030712.D
Acq On : 20 Apr 2023 13:24
Operator : SY/MD
Sample : 02411-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc