

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030713.D
 Acq On : 20 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02411-08 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rBV	111055	120931	13.38%	1.697%
2	1.536	148	154	166	rVB	99130	114099	12.63%	1.601%
3	2.063	310	318	332	rVB	207436	300251	33.23%	4.213%
4	2.809	547	550	553	rBV5	1679	1430	0.16%	0.020%
5	2.838	555	559	561	rBV5	946	690	0.08%	0.010%
6	2.883	569	573	576	rBV7	2068	1591	0.18%	0.022%
7	2.934	588	589	592	rBV3	1318	530	0.06%	0.007%
8	3.050	623	625	627	rBV3	802	263	0.03%	0.004%
9	3.111	639	644	648	rBV7	1953	2310	0.26%	0.032%
10	3.130	648	650	652	rVV3	961	463	0.05%	0.006%
11	3.175	662	664	669	rVB5	1941	1450	0.16%	0.020%
12	3.195	669	670	671	rBV	913	189	0.02%	0.003%
13	3.207	672	674	676	rVB3	1267	345	0.04%	0.005%
14	3.294	699	701	703	rBV2	1658	741	0.08%	0.010%
15	3.326	708	711	716	rBV6	1254	1103	0.12%	0.015%
16	3.468	751	755	756	rBV3	992	660	0.07%	0.009%
17	3.500	762	765	770	rBV6	1573	1329	0.15%	0.019%
18	3.584	787	791	792	rBV4	1173	785	0.09%	0.011%
19	3.625	801	804	805	rBV2	1672	865	0.10%	0.012%
20	3.696	823	826	829	rBV5	1678	1230	0.14%	0.017%
21	3.796	847	857	879	rBV	52662	150925	16.70%	2.118%
22	4.259	986	1001	1025	rBV2	126569	323368	35.79%	4.537%
23	4.825	1176	1177	1180	rBV3	954	333	0.04%	0.005%
24	4.863	1187	1189	1193	rBV4	1340	824	0.09%	0.012%
25	4.966	1205	1221	1247	rBV2	292851	778211	86.13%	10.919%
26	5.307	1325	1327	1328	rBV2	1381	631	0.07%	0.009%
27	5.542	1389	1400	1420	rBV	276574	557970	61.75%	7.829%
28	5.841	1479	1493	1522	rBV	449837	903570	100.00%	12.678%
29	5.998	1532	1542	1560	rVB	169237	340649	37.70%	4.780%
30	6.500	1697	1698	1699	rBV	1450	471	0.05%	0.007%
31	6.555	1710	1715	1717	rBV6	2079	1731	0.19%	0.024%
32	6.703	1759	1761	1762	rBV2	1686	792	0.09%	0.011%
33	6.863	1809	1811	1814	rBV3	1422	833	0.09%	0.012%
34	6.921	1820	1829	1847	rBV	86335	158748	17.57%	2.227%
35	7.252	1921	1932	1961	rBV	327505	581188	64.32%	8.155%
36	7.561	2019	2028	2046	rBV	63948	114478	12.67%	1.606%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030713.D
 Acq On : 20 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02411-08 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.847	2115	2117	2121	rBV5	1251	734	0.08%	0.010%
38	7.995	2161	2163	2165	rBV3	1204	594	0.07%	0.008%
39	8.034	2165	2175	2208	rVV	159953	330629	36.59%	4.639%
40	8.603	2350	2352	2353	rBV2	1487	600	0.07%	0.008%
41	8.670	2372	2373	2374	rBV	659	182	0.02%	0.003%
42	8.792	2400	2411	2432	rBV	423114	712636	78.87%	9.999%
43	9.313	2569	2573	2577	rBV5	2207	2048	0.23%	0.029%
44	9.403	2596	2601	2605	rBV7	1965	2078	0.23%	0.029%
45	9.728	2700	2702	2703	rBV2	1520	669	0.07%	0.009%
46	9.908	2756	2758	2762	rVB5	1466	892	0.10%	0.013%
47	9.931	2762	2765	2767	rBV4	1636	1075	0.12%	0.015%
48	10.037	2796	2798	2801	rBV5	1533	1022	0.11%	0.014%
49	10.162	2826	2837	2850	rBV	231042	368151	40.74%	5.166%
50	10.390	2904	2908	2910	rBV4	1465	1202	0.13%	0.017%
51	10.673	2994	2996	2997	rBV2	655	185	0.02%	0.003%
52	10.702	3003	3005	3007	rBV3	1177	624	0.07%	0.009%
53	10.808	3037	3038	3039	rVB	1017	196	0.02%	0.003%
54	10.837	3045	3047	3049	rBV3	1064	554	0.06%	0.008%
55	10.908	3067	3069	3072	rVB3	1535	579	0.06%	0.008%
56	10.953	3081	3083	3087	rVB4	1514	1136	0.13%	0.016%
57	11.008	3097	3100	3103	rBV4	1943	1651	0.18%	0.023%
58	11.066	3113	3118	3120	rBV5	1932	1419	0.16%	0.020%
59	11.091	3124	3126	3127	rBV2	1257	582	0.06%	0.008%
60	11.194	3146	3158	3175	rBV	409787	661364	73.19%	9.280%
61	11.423	3227	3229	3230	rBV2	1894	855	0.09%	0.012%
62	11.570	3263	3275	3294	rBV	336582	548775	60.73%	7.700%
63	11.921	3378	3384	3386	rBV7	2068	1975	0.22%	0.028%
64	12.091	3433	3437	3438	rBV4	1280	909	0.10%	0.013%
65	12.101	3438	3440	3442	rVV3	1440	766	0.08%	0.011%
66	12.210	3472	3474	3475	rBV2	1393	608	0.07%	0.009%
67	12.439	3542	3545	3548	rBV5	2270	1809	0.20%	0.025%
68	12.461	3549	3552	3553	rVV2	1679	753	0.08%	0.011%
69	12.574	3585	3587	3589	rBV3	1759	1065	0.12%	0.015%
70	12.641	3605	3608	3611	rBV5	1982	1356	0.15%	0.019%
71	12.754	3642	3643	3646	rBV4	1145	466	0.05%	0.007%
72	12.940	3700	3701	3702	rBV2	915	209	0.02%	0.003%
73	12.998	3716	3719	3722	rBV4	1521	990	0.11%	0.014%
74	13.168	3770	3772	3774	rBV4	1507	708	0.08%	0.010%
75	13.316	3816	3818	3822	rVB4	1162	660	0.07%	0.009%
76	13.361	3829	3832	3837	rVB6	911	797	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030713.D
 Acq On : 20 Apr 2023 13:48
 Operator : SY/MD
 Sample : 02411-08 40X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

77	13.384	3837	3839	3843	rVB5	1204	876	0.10%	0.012%
78	13.410	3843	3847	3848	rBV5	1469	1145	0.13%	0.016%
79	13.641	3916	3919	3920	rBV3	1828	817	0.09%	0.011%
80	13.815	3971	3973	3976	rBV4	1291	690	0.08%	0.010%
81	13.902	3997	4000	4004	rBV5	1932	1623	0.18%	0.023%
82	14.149	4072	4077	4078	rBV5	1236	885	0.10%	0.012%
83	14.355	4139	4141	4142	rBV2	1261	592	0.07%	0.008%
84	14.747	4260	4263	4264	rBV3	1844	976	0.11%	0.014%




Sum of corrected areas: 7127084

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030713.D
Acq On : 20 Apr 2023 13:48
Operator : SY/MD
Sample : 02411-08 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

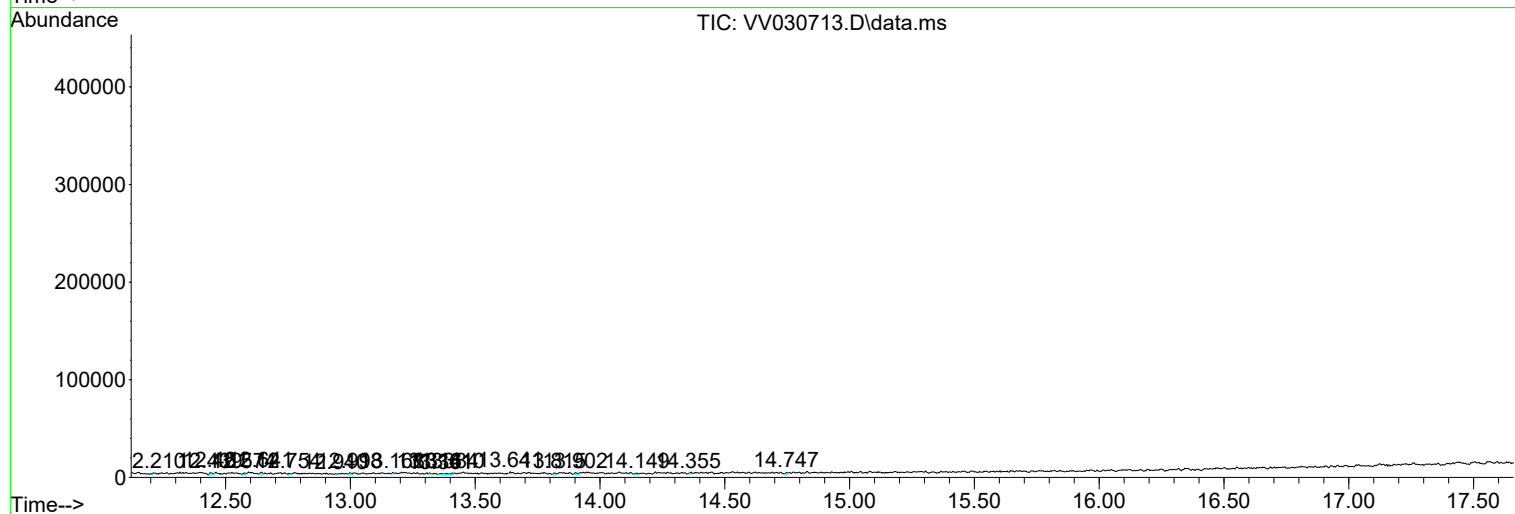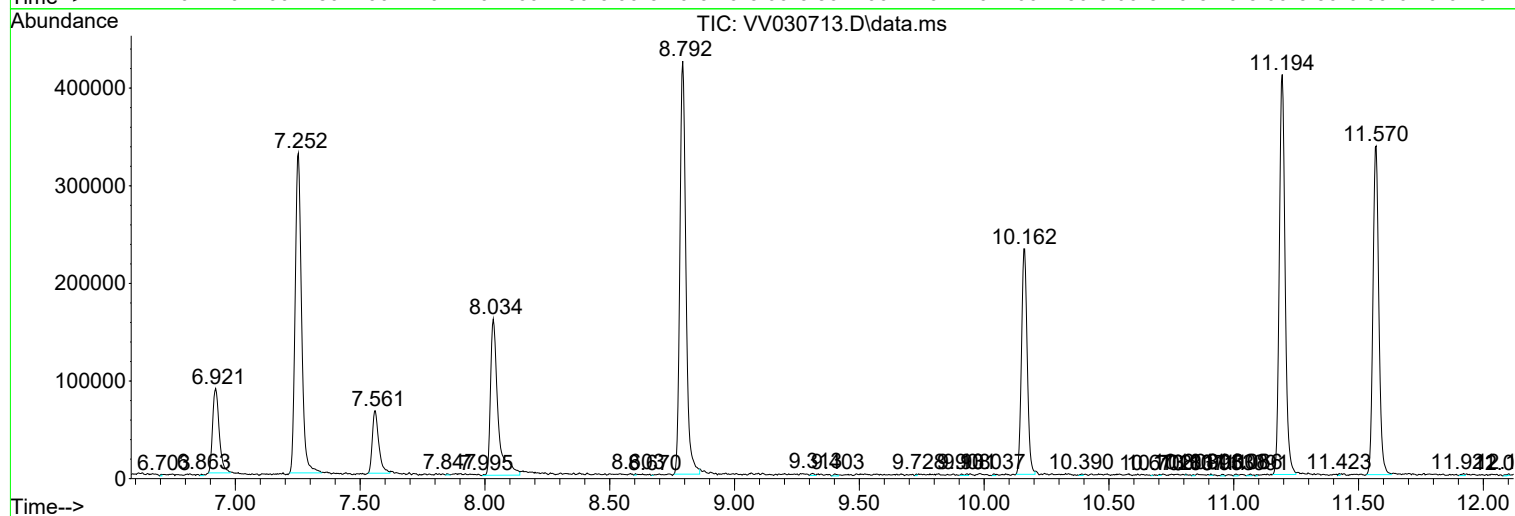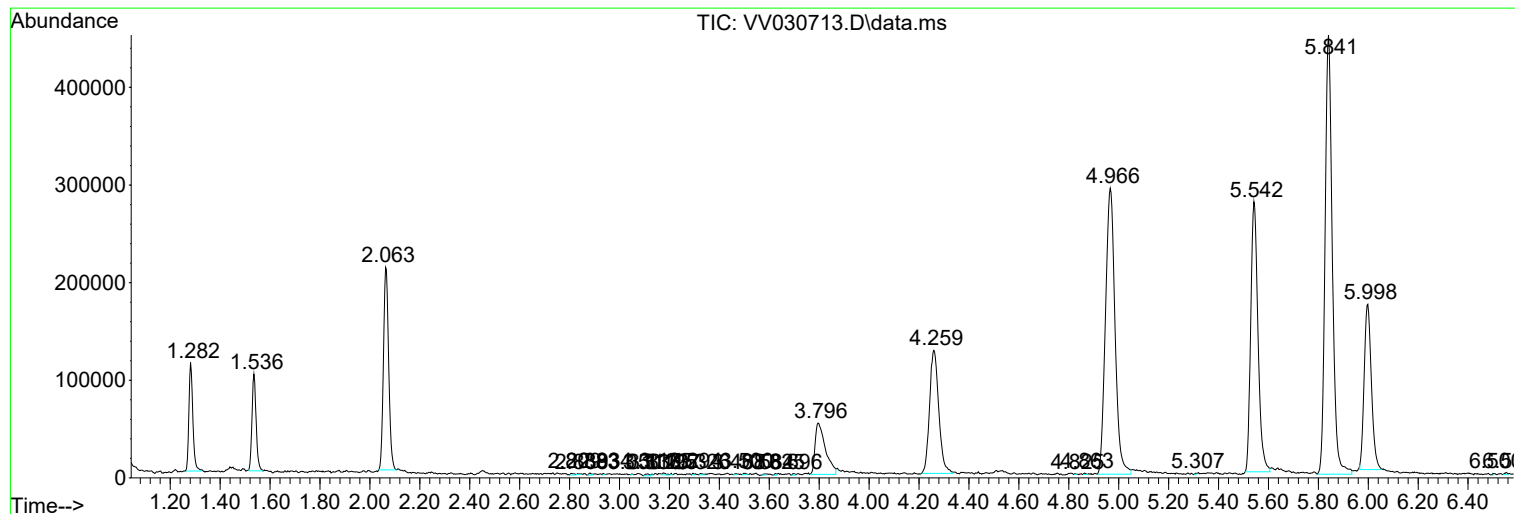

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030713.D
Acq On : 20 Apr 2023 13:48
Operator : SY/MD
Sample : 02411-08 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030713.D
Acq On : 20 Apr 2023 13:48
Operator : SY/MD
Sample : 02411-08 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------