

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030714.D
 Acq On : 20 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02411-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rVB	69378	74645	10.55%	1.171%
2	1.535	148	154	166	rVB	72252	87490	12.37%	1.372%
3	2.066	309	319	333	rBV	155764	231391	32.71%	3.630%
4	2.381	414	417	420	rVB4	1672	929	0.13%	0.015%
5	2.423	426	430	433	rVB6	1653	1356	0.19%	0.021%
6	2.449	434	438	441	rBV6	1884	1690	0.24%	0.027%
7	2.616	488	490	494	rVB5	1241	687	0.10%	0.011%
8	2.648	497	500	505	rVB7	1520	1081	0.15%	0.017%
9	3.108	641	643	646	rBV4	1106	787	0.11%	0.012%
10	3.330	709	712	715	rBV5	1769	1401	0.20%	0.022%
11	3.403	732	735	738	rVB5	1962	1297	0.18%	0.020%
12	3.423	738	741	742	rBV3	1227	688	0.10%	0.011%
13	3.432	742	744	749	rVV5	1122	941	0.13%	0.015%
14	3.481	758	759	763	rBV4	930	679	0.10%	0.011%
15	3.658	811	814	817	rBV4	1260	899	0.13%	0.014%
16	3.677	817	820	821	rBV3	1360	664	0.09%	0.010%
17	3.686	821	823	827	rBV4	1041	810	0.11%	0.013%
18	3.796	846	857	893	rBV	62025	207084	29.28%	3.248%
19	4.259	988	1001	1021	rBV	120955	300972	42.55%	4.721%
20	4.834	1177	1180	1184	rBV6	1247	1153	0.16%	0.018%
21	4.886	1194	1196	1199	rBV3	1253	678	0.10%	0.011%
22	4.966	1205	1221	1246	rBV2	261843	707357	100.00%	11.095%
23	5.439	1366	1368	1371	rBV4	1228	688	0.10%	0.011%
24	5.477	1378	1380	1383	rBV4	1100	865	0.12%	0.014%
25	5.542	1389	1400	1418	rBV	247277	511147	72.26%	8.018%
26	5.841	1482	1493	1517	rVB	232554	459733	64.99%	7.211%
27	5.998	1531	1542	1563	rVB	165050	335618	47.45%	5.264%
28	6.567	1712	1719	1723	rBV9	2116	2795	0.40%	0.044%
29	6.876	1812	1815	1817	rBV5	1478	935	0.13%	0.015%
30	6.921	1818	1829	1844	rBV	83032	155392	21.97%	2.437%
31	7.252	1920	1932	1954	rBV	280180	506868	71.66%	7.951%
32	7.561	2020	2028	2045	rBV	57864	98613	13.94%	1.547%
33	7.780	2094	2096	2100	rBV5	1393	852	0.12%	0.013%
34	8.034	2161	2175	2208	rBV	194268	393211	55.59%	6.168%
35	8.484	2313	2315	2319	rBV4	1723	1188	0.17%	0.019%
36	8.792	2400	2411	2432	rBV	380862	651494	92.10%	10.219%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030714.D
 Acq On : 20 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02411-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.995	2470	2474	2476	rBV4	2037	1430	0.20%	0.022%
38	9.085	2499	2502	2507	rBV7	1508	1424	0.20%	0.022%
39	9.185	2529	2533	2536	rBV5	1742	1396	0.20%	0.022%
40	9.262	2553	2557	2558	rBV3	1858	1269	0.18%	0.020%
41	9.384	2593	2595	2599	rVB4	1588	953	0.13%	0.015%
42	9.403	2599	2601	2605	rBV6	1468	906	0.13%	0.014%
43	9.628	2669	2671	2674	rBV4	1568	910	0.13%	0.014%
44	9.709	2693	2696	2697	rBV2	1322	805	0.11%	0.013%
45	9.805	2723	2726	2729	rBV4	1458	1153	0.16%	0.018%
46	9.892	2751	2753	2757	rVB4	1731	1202	0.17%	0.019%
47	9.924	2760	2763	2768	rVV7	1407	1153	0.16%	0.018%
48	10.033	2795	2797	2800	rBV4	1226	674	0.10%	0.011%
49	10.162	2820	2837	2857	rBV	256646	420259	59.41%	6.592%
50	10.297	2875	2879	2882	rBV5	1739	1490	0.21%	0.023%
51	10.461	2926	2930	2932	rVB5	1409	1014	0.14%	0.016%
52	10.480	2932	2936	2938	rBV5	2147	1655	0.23%	0.026%
53	10.686	2995	3000	3001	rBV5	1118	863	0.12%	0.014%
54	10.731	3011	3014	3019	rBV4	1334	1475	0.21%	0.023%
55	10.760	3021	3023	3025	rVV3	1934	913	0.13%	0.014%
56	11.014	3101	3102	3106	rVB4	1388	999	0.14%	0.016%
57	11.040	3106	3110	3112	rBV5	1581	1198	0.17%	0.019%
58	11.066	3117	3118	3122	rBV4	1035	834	0.12%	0.013%
59	11.107	3127	3131	3132	rBV4	1633	949	0.13%	0.015%
60	11.194	3147	3158	3179	rBV	370847	599351	84.73%	9.401%
61	11.390	3213	3219	3222	rBV6	1145	1124	0.16%	0.018%
62	11.410	3222	3225	3227	rBV4	1104	826	0.12%	0.013%
63	11.570	3264	3275	3295	rVB	333226	544350	76.96%	8.538%
64	11.998	3405	3408	3412	rBV4	1601	962	0.14%	0.015%
65	12.024	3412	3416	3417	rBV4	1690	951	0.13%	0.015%
66	12.152	3453	3456	3460	rVB6	1644	1261	0.18%	0.020%
67	12.181	3460	3465	3466	rBV5	1365	853	0.12%	0.013%
68	12.252	3485	3487	3490	rVB4	1383	687	0.10%	0.011%
69	12.303	3498	3503	3508	rBV8	2803	3067	0.43%	0.048%
70	12.361	3517	3521	3523	rBV5	1481	1012	0.14%	0.016%
71	12.416	3535	3538	3541	rBV4	1346	1002	0.14%	0.016%
72	12.435	3541	3544	3546	rVB4	1240	684	0.10%	0.011%
73	12.464	3550	3553	3557	rVB5	1481	826	0.12%	0.013%
74	12.512	3565	3568	3572	rBV5	1029	963	0.14%	0.015%
75	12.686	3620	3622	3624	rBV3	1324	625	0.09%	0.010%
76	12.741	3635	3639	3644	rVB7	1229	1065	0.15%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030714.D
 Acq On : 20 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02411-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.766	3645	3647	3650	rBV3	1396	888	0.13%	0.014%
78	12.892	3684	3686	3688	rBV3	1261	675	0.10%	0.011%
79	13.017	3720	3725	3728	rBV6	1189	1187	0.17%	0.019%
80	13.091	3744	3748	3750	rBV5	1361	880	0.12%	0.014%
81	13.107	3750	3753	3758	rVB7	1230	1226	0.17%	0.019%
82	13.136	3758	3762	3763	rBV4	1363	1084	0.15%	0.017%
83	13.207	3780	3784	3788	rBV7	2133	2104	0.30%	0.033%
84	13.303	3806	3814	3818	rBV9	1623	2048	0.29%	0.032%
85	13.545	3886	3889	3892	rBV4	1504	740	0.10%	0.012%
86	13.699	3934	3937	3942	rBV7	1872	1251	0.18%	0.020%
87	13.795	3965	3967	3970	rBV3	1251	638	0.09%	0.010%
88	13.837	3978	3980	3982	rBV2	1336	659	0.09%	0.010%
89	13.914	4000	4004	4007	rVB5	1670	1270	0.18%	0.020%
90	13.946	4010	4014	4016	rBV5	1534	1114	0.16%	0.017%
91	13.963	4016	4019	4021	rBV3	1255	1010	0.14%	0.016%
92	14.098	4058	4061	4065	rVB7	1259	986	0.14%	0.015%
93	14.123	4065	4069	4071	rBV5	1285	929	0.13%	0.015%
94	14.220	4096	4099	4102	rBV4	1120	757	0.11%	0.012%
95	14.782	4271	4274	4276	rBV4	1763	1235	0.17%	0.019%
96	14.911	4310	4314	4316	rBV3	1823	1190	0.17%	0.019%
97	14.950	4324	4326	4330	rVB5	1770	1158	0.16%	0.018%
98	15.059	4358	4360	4364	rBV5	2349	1690	0.24%	0.027%
99	15.146	4384	4387	4388	rBV3	1365	688	0.10%	0.011%
100	15.281	4427	4429	4431	rBV3	2178	1261	0.18%	0.020%




Sum of corrected areas: 6375279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030714.D
Acq On : 20 Apr 2023 14:12
Operator : SY/MD
Sample : 02411-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

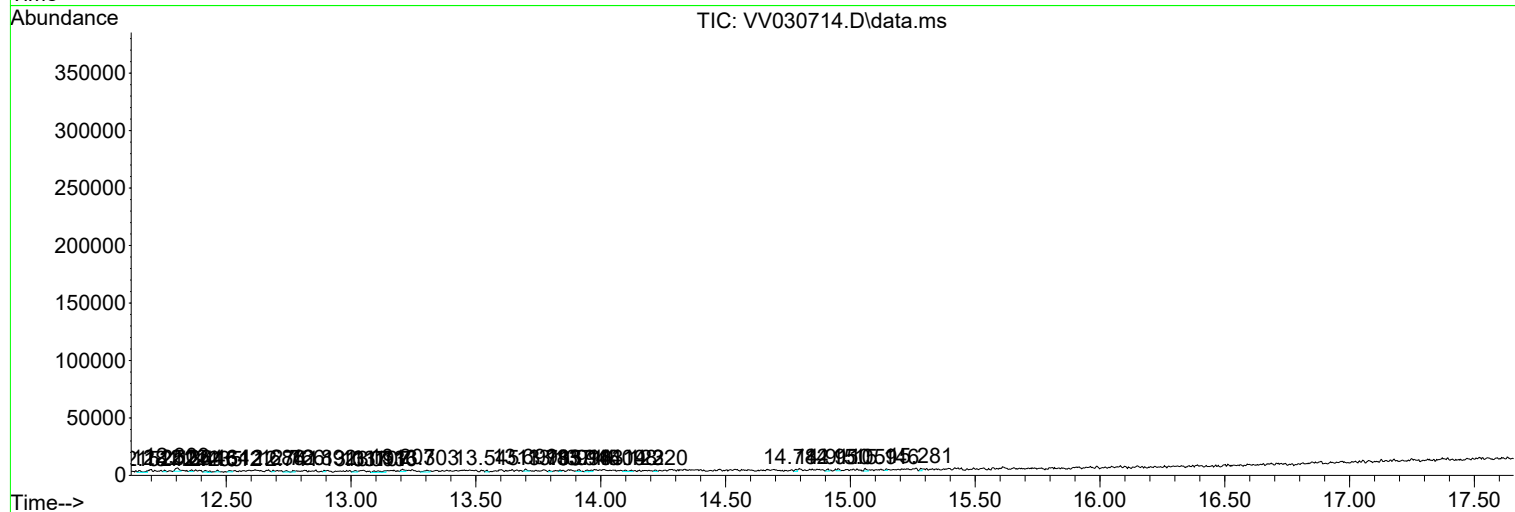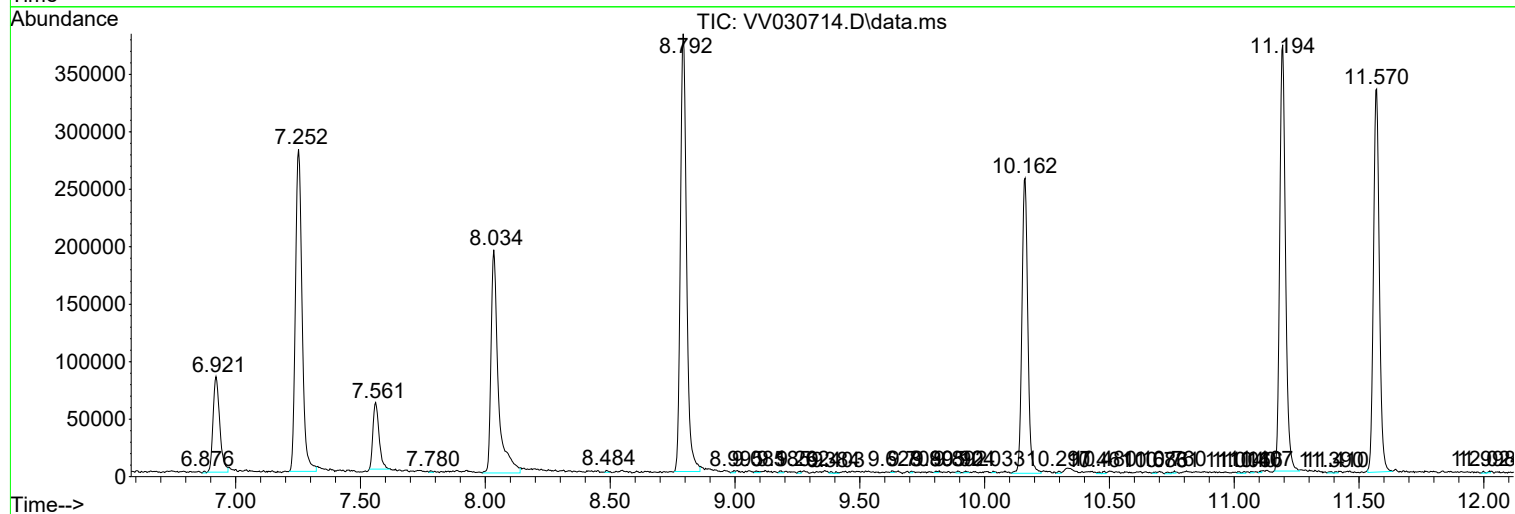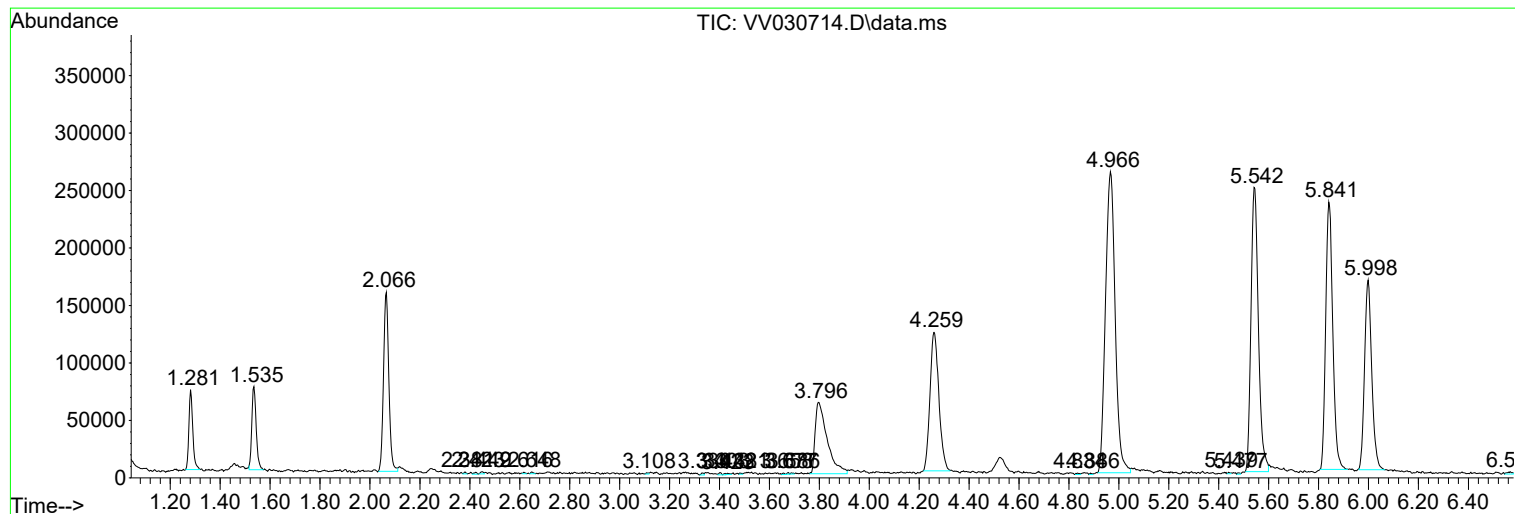

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030714.D
Acq On : 20 Apr 2023 14:12
Operator : SY/MD
Sample : 02411-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030714.D
Acq On : 20 Apr 2023 14:12
Operator : SY/MD
Sample : 02411-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc