

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030715.D
 Acq On : 20 Apr 2023 14:36
 Operator : SY/MD
 Sample : 02411-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030715.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rBV	71961	77793	10.67%	1.303%
2	1.539	147	155	167	rBV	82955	99483	13.65%	1.667%
3	2.066	310	319	335	rVB	156629	226745	31.10%	3.799%
4	2.516	455	459	462	rBV6	782	731	0.10%	0.012%
5	2.661	502	504	506	rBV3	1716	809	0.11%	0.014%
6	2.834	555	558	560	rVV4	1044	658	0.09%	0.011%
7	3.043	620	623	625	rBV3	1664	1168	0.16%	0.020%
8	3.105	639	642	646	rVB6	1712	1561	0.21%	0.026%
9	3.172	659	663	665	rBV4	971	763	0.10%	0.013%
10	3.285	693	698	700	rBV5	1067	891	0.12%	0.015%
11	3.310	704	706	710	rVB5	2371	1499	0.21%	0.025%
12	3.413	736	738	740	rBV2	1184	667	0.09%	0.011%
13	3.429	740	743	745	rVB4	1380	706	0.10%	0.012%
14	3.468	753	755	760	rBV7	1454	1388	0.19%	0.023%
15	3.613	798	800	807	rVB7	2033	1427	0.20%	0.024%
16	3.641	807	809	811	rBV3	1166	638	0.09%	0.011%
17	3.664	811	816	821	rBV5	1806	1882	0.26%	0.032%
18	3.805	850	860	885	rBV	58382	175965	24.14%	2.948%
19	4.259	988	1001	1024	rVB	124270	313659	43.02%	5.255%
20	4.510	1076	1079	1082	rBV6	1148	885	0.12%	0.015%
21	4.677	1129	1131	1135	rVB4	1537	817	0.11%	0.014%
22	4.831	1173	1179	1183	rBV7	1664	2153	0.30%	0.036%
23	4.883	1193	1195	1201	rBV6	856	719	0.10%	0.012%
24	4.966	1201	1221	1243	rBV3	269414	729018	100.00%	12.213%
25	5.346	1337	1339	1341	rBV3	1890	912	0.13%	0.015%
26	5.455	1368	1373	1376	rVB7	2330	2072	0.28%	0.035%
27	5.471	1376	1378	1380	rBV4	2003	1231	0.17%	0.021%
28	5.542	1388	1400	1424	rBV	246754	518863	71.17%	8.692%
29	5.937	1517	1523	1525	rBV5	1761	1643	0.23%	0.028%
30	5.998	1530	1542	1568	rVB	168702	354122	48.58%	5.933%
31	6.333	1644	1646	1649	rBV4	1193	857	0.12%	0.014%
32	6.493	1694	1696	1698	rVB3	1734	723	0.10%	0.012%
33	6.526	1704	1706	1710	rBV5	1431	1117	0.15%	0.019%
34	6.558	1713	1716	1717	rBV2	1620	970	0.13%	0.016%
35	6.831	1795	1801	1803	rBV6	1435	1567	0.21%	0.026%
36	6.921	1819	1829	1847	rBV	83264	157219	21.57%	2.634%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030715.D
 Acq On : 20 Apr 2023 14:36
 Operator : SY/MD
 Sample : 02411-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1919	1932	1950	rBV	288687	522570	71.68%	8.755%
38	7.561	2019	2028	2043	rBV2	62455	116294	15.95%	1.948%
39	7.844	2114	2116	2118	rBV3	1419	699	0.10%	0.012%
40	7.873	2123	2125	2127	rBV3	2132	1338	0.18%	0.022%
41	7.950	2146	2149	2150	rBV3	1353	873	0.12%	0.015%
42	8.034	2164	2175	2192	rBV	191613	369845	50.73%	6.196%
43	8.493	2316	2318	2320	rBV3	1391	738	0.10%	0.012%
44	8.583	2343	2346	2348	rBV3	1401	706	0.10%	0.012%
45	8.792	2399	2411	2427	rBV	385349	640829	87.90%	10.736%
46	9.198	2535	2537	2538	rBV2	1280	634	0.09%	0.011%
47	9.284	2562	2564	2571	rVB6	1642	1248	0.17%	0.021%
48	9.323	2571	2576	2578	rBV6	2090	1626	0.22%	0.027%
49	9.345	2580	2583	2586	rVV5	1565	1068	0.15%	0.018%
50	9.374	2590	2592	2594	rBV3	1558	841	0.12%	0.014%
51	9.423	2605	2607	2610	rBV4	1860	950	0.13%	0.016%
52	9.599	2658	2662	2665	rBV5	1974	1803	0.25%	0.030%
53	9.616	2665	2667	2670	rVB3	1591	733	0.10%	0.012%
54	9.635	2670	2673	2676	rBV5	1571	1417	0.19%	0.024%
55	9.741	2704	2706	2710	rVB5	1553	918	0.13%	0.015%
56	9.815	2725	2729	2732	rVB5	1941	1493	0.20%	0.025%
57	9.834	2732	2735	2737	rBV4	1563	806	0.11%	0.014%
58	9.979	2777	2780	2784	rBV5	1728	1303	0.18%	0.022%
59	10.037	2794	2798	2799	rBV3	1128	749	0.10%	0.013%
60	10.098	2815	2817	2821	rBV4	1228	994	0.14%	0.017%
61	10.162	2825	2837	2852	rBV	260130	423255	58.06%	7.091%
62	10.381	2903	2905	2908	rBV3	1069	743	0.10%	0.012%
63	10.406	2910	2913	2916	rVV5	1060	903	0.12%	0.015%
64	10.548	2955	2957	2959	rVB3	1736	766	0.11%	0.013%
65	10.564	2959	2962	2964	rBV4	1944	1180	0.16%	0.020%
66	10.625	2980	2981	2984	rBV3	909	659	0.09%	0.011%
67	10.670	2992	2995	2999	rBV5	1389	1415	0.19%	0.024%
68	10.760	3021	3023	3026	rBV3	2257	1497	0.21%	0.025%
69	10.779	3026	3029	3032	rVV5	1730	1231	0.17%	0.021%
70	10.828	3040	3044	3047	rBV5	1342	1369	0.19%	0.023%
71	11.104	3127	3130	3133	rBV5	1171	899	0.12%	0.015%
72	11.194	3146	3158	3177	rBV	363746	591192	81.09%	9.904%
73	11.496	3250	3252	3256	rBV6	1364	1124	0.15%	0.019%
74	11.567	3263	3274	3292	rBV	346560	562624	77.18%	9.426%
75	11.857	3360	3364	3368	rVB7	1430	1175	0.16%	0.020%
76	11.882	3368	3372	3375	rBV6	2038	1755	0.24%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030715.D
 Acq On : 20 Apr 2023 14:36
 Operator : SY/MD
 Sample : 02411-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.095	3435	3438	3441	rBV5	1378	947	0.13%	0.016%
78	12.265	3487	3491	3494	rBV4	1557	1089	0.15%	0.018%
79	12.323	3506	3509	3513	rBV6	1548	1019	0.14%	0.017%
80	12.384	3525	3528	3531	rBV4	1075	855	0.12%	0.014%
81	12.445	3542	3547	3548	rBV4	1665	1426	0.20%	0.024%
82	12.467	3552	3554	3557	rVB4	1541	870	0.12%	0.015%
83	12.631	3601	3605	3607	rBV5	1499	1011	0.14%	0.017%
84	12.770	3645	3648	3651	rBV5	849	721	0.10%	0.012%
85	12.837	3665	3669	3673	rBV6	1142	926	0.13%	0.016%
86	12.934	3696	3699	3702	rBV7	1210	943	0.13%	0.016%
87	13.168	3770	3772	3776	rVB5	1555	933	0.13%	0.016%
88	13.255	3797	3799	3803	rBV5	1186	785	0.11%	0.013%
89	13.297	3809	3812	3816	rBV5	1549	1475	0.20%	0.025%
90	13.377	3835	3837	3839	rBV3	1275	632	0.09%	0.011%
91	13.455	3858	3861	3863	rBV4	2260	1259	0.17%	0.021%
92	13.506	3875	3877	3880	rVV4	1274	639	0.09%	0.011%
93	13.612	3907	3910	3911	rBV3	1288	649	0.09%	0.011%
94	13.763	3955	3957	3962	rBV5	1521	875	0.12%	0.015%
95	13.924	4001	4007	4011	rBV9	1297	1465	0.20%	0.025%
96	13.995	4026	4029	4032	rBV5	1119	959	0.13%	0.016%
97	14.156	4076	4079	4084	rBV5	2037	1359	0.19%	0.023%
98	14.310	4123	4127	4128	rBV4	1681	1226	0.17%	0.021%
99	14.480	4178	4180	4182	rBV3	1196	752	0.10%	0.013%
100	14.725	4252	4256	4257	rBV4	1196	756	0.10%	0.013%




Sum of corrected areas: 5969154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030715.D
Acq On : 20 Apr 2023 14:36
Operator : SY/MD
Sample : 02411-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

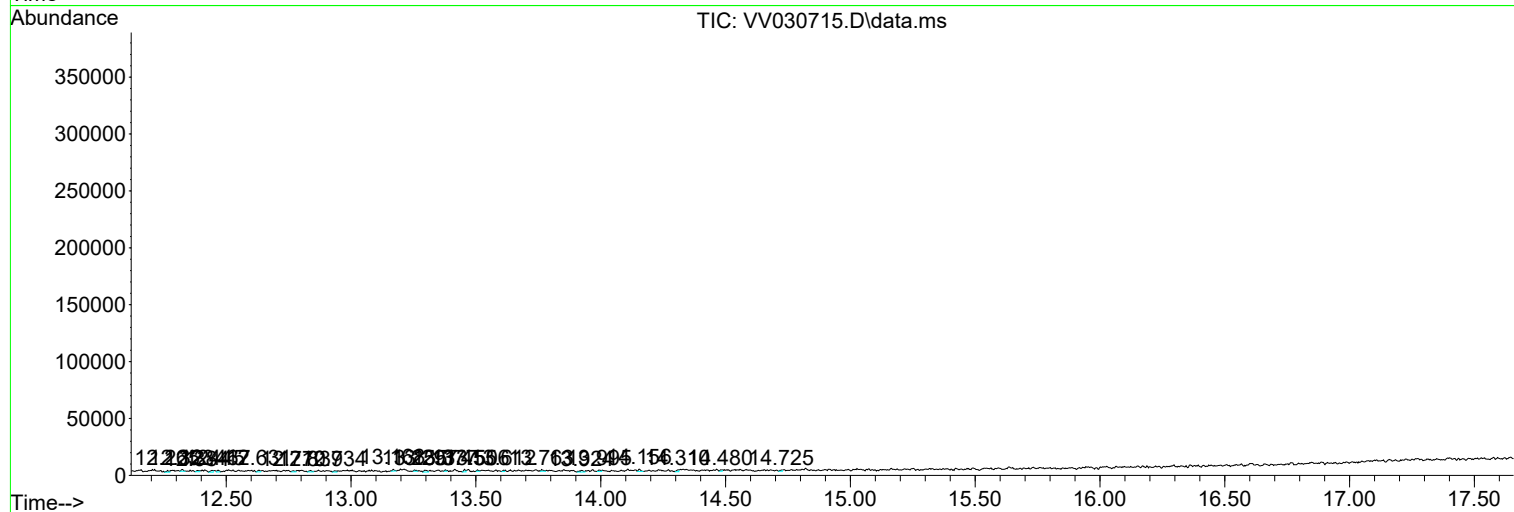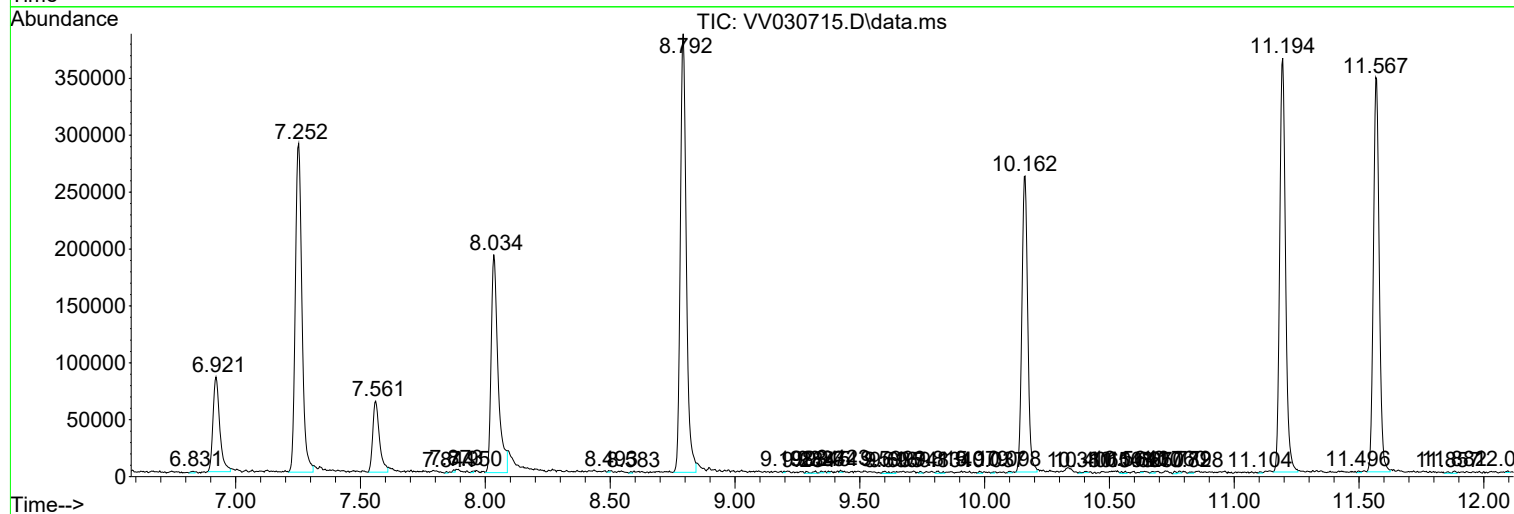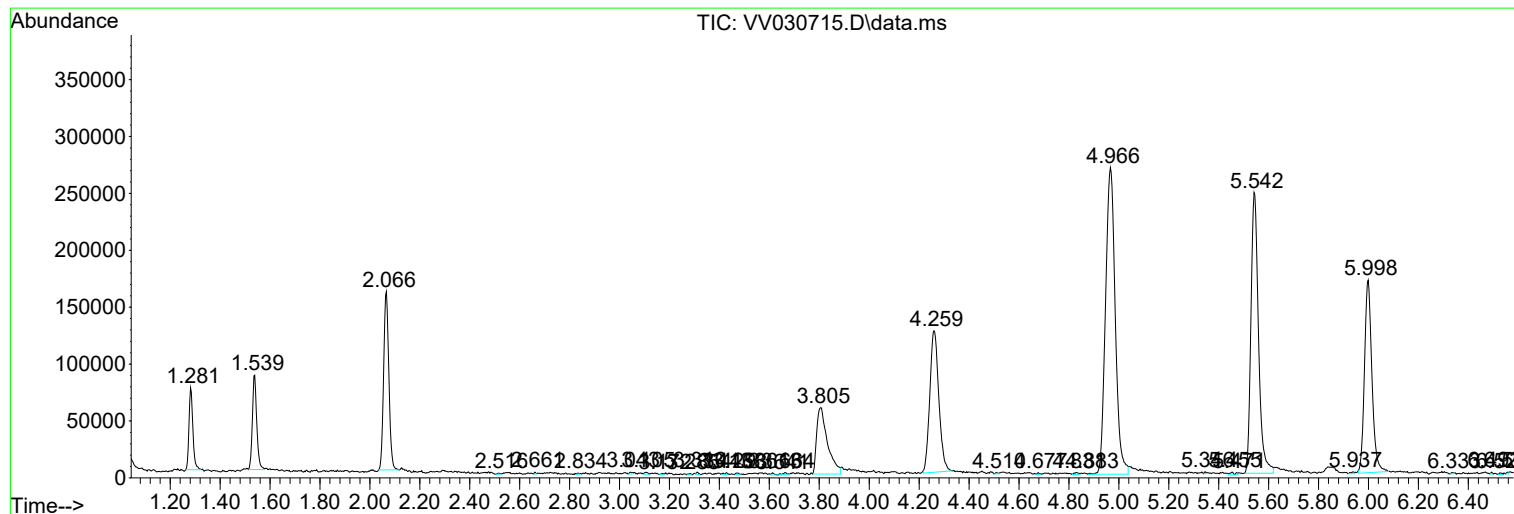

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030715.D
Acq On : 20 Apr 2023 14:36
Operator : SY/MD
Sample : 02411-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030715.D
Acq On : 20 Apr 2023 14:36
Operator : SY/MD
Sample : 02411-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc