

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030716.D
 Acq On : 20 Apr 2023 14:59
 Operator : SY/MD
 Sample : 02411-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rBV	112395	123141	12.14%	1.623%
2	1.539	148	155	171	rVB	110286	130296	12.85%	1.717%
3	2.066	309	319	333	rBV	219205	332809	32.82%	4.385%
4	2.330	399	401	405	rVB5	1570	874	0.09%	0.012%
5	2.500	452	454	455	rBV2	1816	706	0.07%	0.009%
6	2.584	476	480	482	rBV5	1191	925	0.09%	0.012%
7	2.825	551	555	557	rBV4	1096	943	0.09%	0.012%
8	3.105	639	642	643	rBV3	1386	900	0.09%	0.012%
9	3.240	681	684	686	rBV2	1758	758	0.07%	0.010%
10	3.317	705	708	714	rVB6	2258	1901	0.19%	0.025%
11	3.355	714	720	721	rBV5	1063	1031	0.10%	0.014%
12	3.439	744	746	750	rVB6	1092	690	0.07%	0.009%
13	3.542	775	778	781	rVB5	1470	1080	0.11%	0.014%
14	3.590	790	793	798	rVB7	2065	1520	0.15%	0.020%
15	3.693	821	825	828	rVV6	1384	1074	0.11%	0.014%
16	3.761	842	846	847	rBV3	1405	764	0.08%	0.010%
17	3.809	851	861	887	rVV3	58364	199330	19.66%	2.627%
18	4.133	956	962	963	rBV6	2036	1409	0.14%	0.019%
19	4.259	989	1001	1022	rVB	127647	319625	31.52%	4.212%
20	4.670	1127	1129	1133	rVB4	1885	843	0.08%	0.011%
21	4.712	1138	1142	1147	rVB8	2078	1855	0.18%	0.024%
22	4.892	1196	1198	1202	rBV5	1457	1170	0.12%	0.015%
23	4.966	1203	1221	1250	rBV2	302591	808879	79.77%	10.658%
24	5.262	1310	1313	1314	rBV3	2314	982	0.10%	0.013%
25	5.288	1318	1321	1327	rVV9	1348	1502	0.15%	0.020%
26	5.394	1351	1354	1355	rBV2	1129	692	0.07%	0.009%
27	5.410	1357	1359	1365	rVV6	2040	1948	0.19%	0.026%
28	5.542	1388	1400	1425	rBV	293684	606939	59.86%	7.998%
29	5.841	1481	1493	1512	rBV	514911	1013968	100.00%	13.361%
30	5.998	1532	1542	1562	rVB	177598	359835	35.49%	4.741%
31	6.278	1626	1629	1631	rVB4	1902	997	0.10%	0.013%
32	6.291	1631	1633	1635	rBV3	1540	838	0.08%	0.011%
33	6.413	1669	1671	1674	rVB4	1872	828	0.08%	0.011%
34	6.455	1679	1684	1686	rBV6	1365	1255	0.12%	0.017%
35	6.606	1728	1731	1734	rBV4	1833	1172	0.12%	0.015%
36	6.703	1759	1761	1764	rBV4	1259	742	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030716.D
 Acq On : 20 Apr 2023 14:59
 Operator : SY/MD
 Sample : 02411-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1815	1829	1847	rBV2	91911	177732	17.53%	2.342%
38	7.059	1868	1872	1876	rBV6	1622	1381	0.14%	0.018%
39	7.252	1920	1932	1948	rBV	334502	599664	59.14%	7.902%
40	7.561	2019	2028	2046	rBV	64977	119294	11.77%	1.572%
41	7.828	2109	2111	2114	rBV4	1649	927	0.09%	0.012%
42	7.860	2119	2121	2125	rVB4	1800	1134	0.11%	0.015%
43	7.883	2125	2128	2130	rBV4	1438	981	0.10%	0.013%
44	7.921	2138	2140	2145	rVB5	1967	1803	0.18%	0.024%
45	8.034	2165	2175	2190	rBV	162386	308034	30.38%	4.059%
46	8.677	2373	2375	2377	rBV3	1475	883	0.09%	0.012%
47	8.792	2399	2411	2436	rBV	437084	752658	74.23%	9.918%
48	9.214	2537	2542	2543	rBV4	1479	1160	0.11%	0.015%
49	9.593	2659	2660	2663	rVB3	1522	799	0.08%	0.011%
50	9.673	2683	2685	2689	rBV5	1200	714	0.07%	0.009%
51	9.757	2709	2711	2713	rBV2	1325	856	0.08%	0.011%
52	9.857	2737	2742	2746	rBV7	1684	1528	0.15%	0.020%
53	9.899	2751	2755	2756	rBV3	1393	858	0.08%	0.011%
54	9.995	2783	2785	2790	rBV5	984	772	0.08%	0.010%
55	10.159	2819	2836	2858	rBV	237652	392602	38.72%	5.173%
56	10.307	2879	2882	2886	rBV5	1551	1293	0.13%	0.017%
57	10.413	2911	2915	2919	rBV6	1439	1344	0.13%	0.018%
58	10.513	2942	2946	2949	rBV6	1122	820	0.08%	0.011%
59	10.641	2981	2986	2987	rBV4	913	756	0.07%	0.010%
60	10.689	2999	3001	3004	rBV4	1030	769	0.08%	0.010%
61	10.738	3013	3016	3019	rBV4	1362	830	0.08%	0.011%
62	10.776	3026	3028	3033	rBV6	1464	1537	0.15%	0.020%
63	10.831	3042	3045	3046	rBV3	1811	736	0.07%	0.010%
64	10.841	3046	3048	3054	rVB7	1188	949	0.09%	0.013%
65	10.866	3054	3056	3058	rBV3	1415	763	0.08%	0.010%
66	11.040	3107	3110	3112	rBV3	1821	1142	0.11%	0.015%
67	11.194	3147	3158	3178	rVV	438133	690988	68.15%	9.105%
68	11.567	3264	3274	3295	rBV	351373	560351	55.26%	7.384%
69	11.886	3369	3373	3375	rBV5	1819	1071	0.11%	0.014%
70	11.950	3389	3393	3394	rBV4	1705	1021	0.10%	0.013%
71	12.162	3457	3459	3462	rBV4	1714	1120	0.11%	0.015%
72	12.233	3478	3481	3483	rVB4	1557	887	0.09%	0.012%
73	12.262	3487	3490	3495	rVB7	1618	1341	0.13%	0.018%
74	12.313	3502	3506	3508	rBV5	1166	767	0.08%	0.010%
75	12.384	3521	3528	3530	rBV7	1055	1237	0.12%	0.016%
76	12.448	3546	3548	3551	rVB3	2470	1384	0.14%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030716.D
 Acq On : 20 Apr 2023 14:59
 Operator : SY/MD
 Sample : 02411-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.477	3551	3557	3559	rBV6	1327	1480	0.15%	0.020%
78	12.558	3580	3582	3587	rVB6	1185	697	0.07%	0.009%
79	12.725	3632	3634	3636	rBV3	1640	858	0.08%	0.011%
80	12.744	3636	3640	3645	rVB8	1880	1763	0.17%	0.023%
81	12.808	3659	3660	3663	rVB3	1335	716	0.07%	0.009%
82	12.834	3663	3668	3670	rBV5	1327	1089	0.11%	0.014%
83	12.889	3681	3685	3691	rVB8	2475	2577	0.25%	0.034%
84	12.918	3691	3694	3697	rBV5	1503	1279	0.13%	0.017%
85	13.133	3759	3761	3763	rBV3	1233	742	0.07%	0.010%
86	13.172	3771	3773	3778	rBV5	1783	927	0.09%	0.012%
87	13.313	3812	3817	3821	rBV7	2077	2108	0.21%	0.028%
88	13.455	3857	3861	3862	rBV4	1903	1449	0.14%	0.019%
89	13.496	3871	3874	3878	rBV5	1559	1259	0.12%	0.017%
90	13.551	3887	3891	3893	rBV4	1595	1345	0.13%	0.018%
91	13.609	3907	3909	3914	rVB5	1682	1294	0.13%	0.017%
92	13.654	3922	3923	3929	rVB6	2086	1315	0.13%	0.017%
93	13.680	3929	3931	3934	rBV4	1852	1234	0.12%	0.016%
94	13.747	3948	3952	3957	rVB8	1293	1312	0.13%	0.017%
95	13.869	3989	3990	3994	rBV4	1376	968	0.10%	0.013%
96	13.963	4016	4019	4021	rBV4	2076	1558	0.15%	0.021%
97	14.094	4057	4060	4063	rBV5	848	717	0.07%	0.009%
98	14.149	4074	4077	4081	rBV6	1529	1186	0.12%	0.016%
99	15.082	4365	4367	4370	rBV4	1558	1063	0.10%	0.014%
100	15.413	4468	4470	4473	rBV3	1693	1042	0.10%	0.014%




Sum of corrected areas: 7589085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030716.D
Acq On : 20 Apr 2023 14:59
Operator : SY/MD
Sample : 02411-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

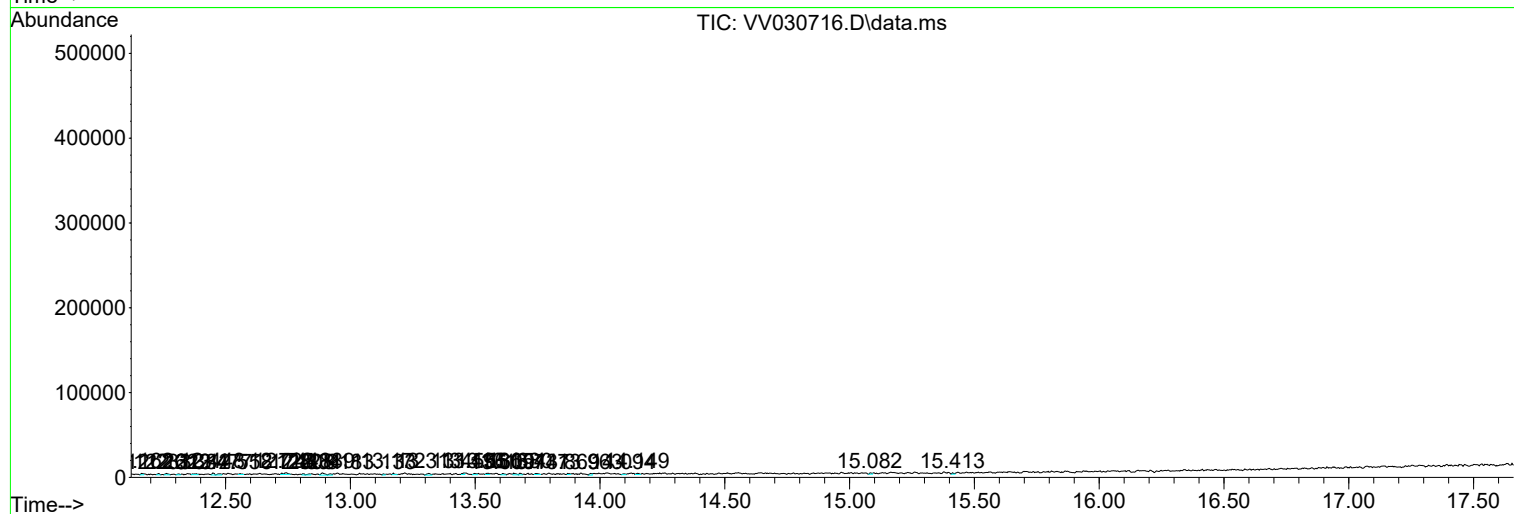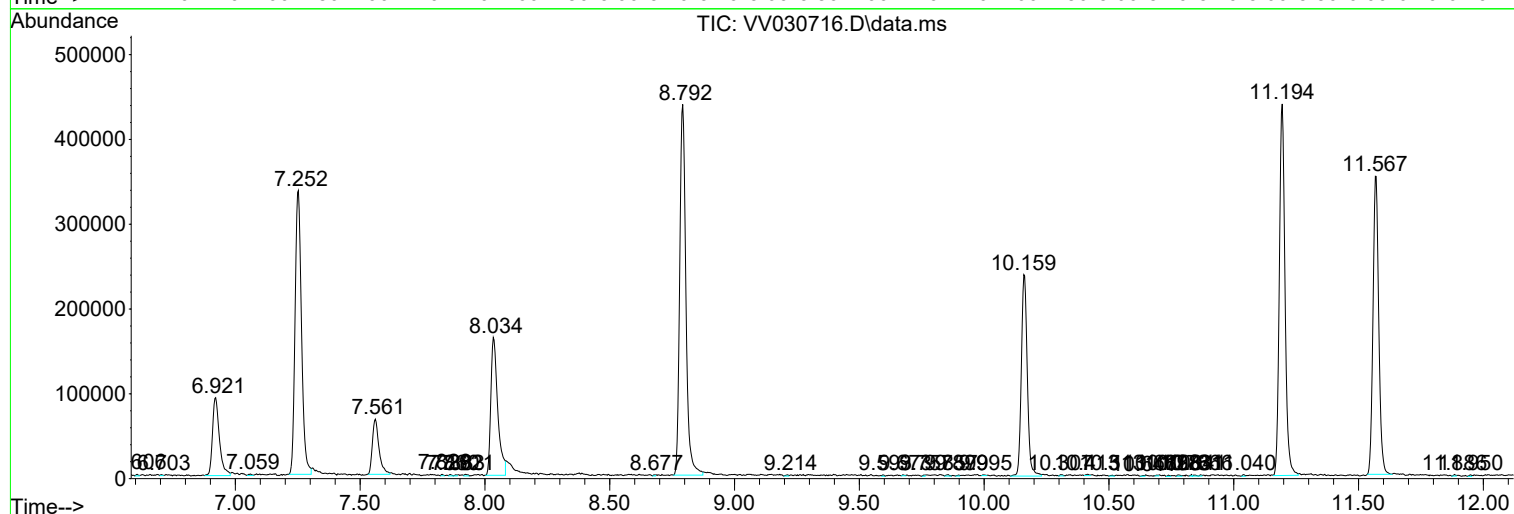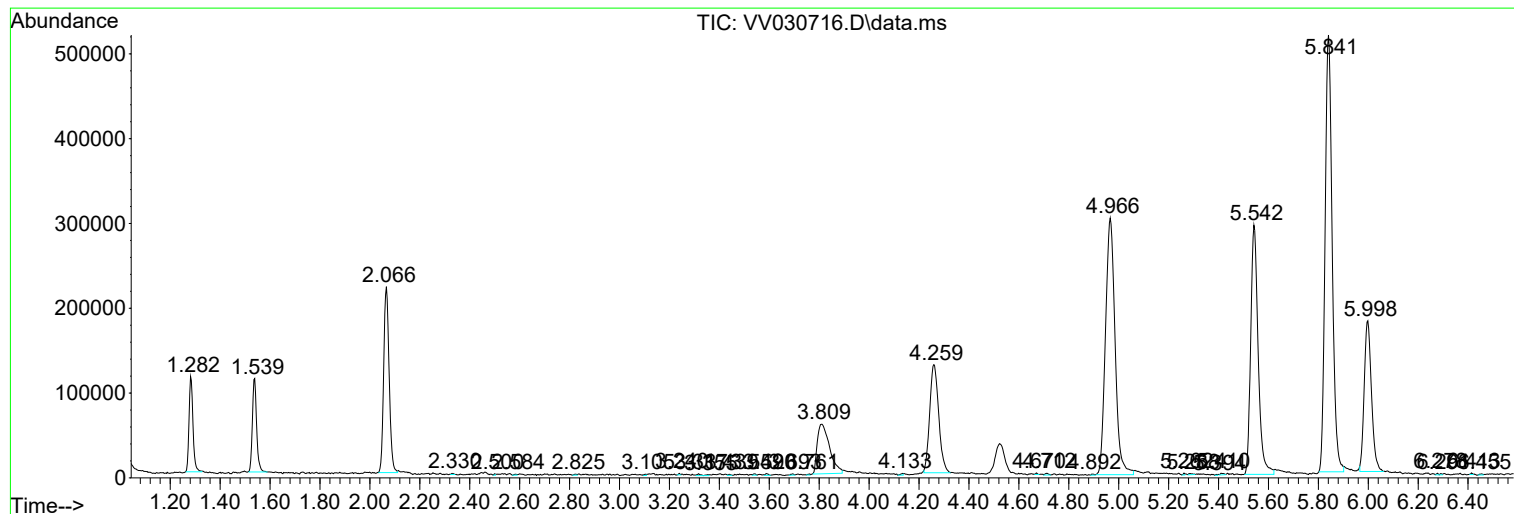

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030716.D
Acq On : 20 Apr 2023 14:59
Operator : SY/MD
Sample : 02411-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030716.D
Acq On : 20 Apr 2023 14:59
Operator : SY/MD
Sample : 02411-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc