

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030717.D
 Acq On : 20 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02411-09 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	51	57	59	rBV4	3041	3317	0.25%	0.042%
2	1.282	69	75	88	rVB	112033	120683	9.18%	1.525%
3	1.536	148	154	168	rVB	108089	128956	9.81%	1.629%
4	2.066	309	319	332	rBV	209979	315200	23.97%	3.983%
5	2.455	432	440	442	rBV7	3828	4949	0.38%	0.063%
6	2.616	487	490	494	rBV5	978	833	0.06%	0.011%
7	2.767	535	537	540	rBV3	1504	749	0.06%	0.009%
8	2.802	545	548	552	rBV6	1375	1156	0.09%	0.015%
9	2.860	564	566	569	rVB4	1092	624	0.05%	0.008%
10	2.876	569	571	573	rBV3	1568	690	0.05%	0.009%
11	3.063	627	629	631	rBV3	1306	725	0.06%	0.009%
12	3.195	668	670	673	rVB4	1061	615	0.05%	0.008%
13	3.343	712	716	717	rBV4	1120	749	0.06%	0.009%
14	3.384	726	729	730	rBV3	972	563	0.04%	0.007%
15	3.404	733	735	738	rBV3	1114	683	0.05%	0.009%
16	3.584	789	791	793	rBV3	1102	702	0.05%	0.009%
17	3.700	825	827	829	rBV3	1389	861	0.07%	0.011%
18	3.757	844	845	848	rBV3	1258	619	0.05%	0.008%
19	3.802	848	859	887	rVV	49081	149687	11.38%	1.891%
20	4.169	969	973	976	rBV6	1474	1480	0.11%	0.019%
21	4.185	976	978	980	rBV3	1238	595	0.05%	0.008%
22	4.262	986	1002	1021	rBV	136876	343513	26.13%	4.340%
23	4.732	1146	1148	1151	rBV3	2111	1302	0.10%	0.016%
24	4.777	1160	1162	1164	rVB2	1799	602	0.05%	0.008%
25	4.905	1200	1202	1203	rBV3	1273	620	0.05%	0.008%
26	4.966	1205	1221	1245	rVV2	300223	793924	60.38%	10.032%
27	5.140	1273	1275	1278	rBV3	2125	1441	0.11%	0.018%
28	5.294	1320	1323	1326	rBV5	992	861	0.07%	0.011%
29	5.362	1340	1344	1345	rBV4	982	613	0.05%	0.008%
30	5.542	1383	1400	1421	rBV2	304988	630714	47.97%	7.969%
31	5.780	1472	1474	1477	rBV4	1604	850	0.06%	0.011%
32	5.841	1479	1493	1520	rBV	656287	1314780	100.00%	16.613%
33	5.998	1532	1542	1563	rVB	174682	357256	27.17%	4.514%
34	6.346	1648	1650	1652	rBV3	1354	804	0.06%	0.010%
35	6.442	1676	1680	1683	rBV6	1595	1358	0.10%	0.017%
36	6.751	1772	1776	1779	rBV6	1185	1141	0.09%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030717.D
 Acq On : 20 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02411-09 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1819	1829	1848	rBV2	91290	170037	12.93%	2.148%
38	7.162	1901	1904	1908	rBV6	2100	1903	0.14%	0.024%
39	7.252	1919	1932	1947	rBV	337331	604817	46.00%	7.642%
40	7.561	2018	2028	2045	rVV	65565	122233	9.30%	1.544%
41	8.034	2165	2175	2208	rBV	164635	344617	26.21%	4.354%
42	8.407	2288	2291	2293	rBV3	1686	848	0.06%	0.011%
43	8.793	2400	2411	2433	rBV	468911	778442	59.21%	9.836%
44	9.031	2480	2485	2486	rBV4	1301	943	0.07%	0.012%
45	9.130	2513	2516	2521	rVB5	1628	1197	0.09%	0.015%
46	9.220	2542	2544	2547	rVB3	1306	610	0.05%	0.008%
47	9.339	2579	2581	2585	rVB4	1653	1154	0.09%	0.015%
48	9.358	2585	2587	2589	rBV3	1369	757	0.06%	0.010%
49	9.503	2630	2632	2635	rBV4	1435	1046	0.08%	0.013%
50	9.609	2663	2665	2671	rVB6	1162	1046	0.08%	0.013%
51	9.664	2677	2682	2683	rBV4	1747	1250	0.10%	0.016%
52	9.870	2743	2746	2747	rBV2	1427	716	0.05%	0.009%
53	9.957	2771	2773	2776	rBV4	974	732	0.06%	0.009%
54	10.159	2826	2836	2855	rVB	238620	376968	28.67%	4.763%
55	10.387	2905	2907	2910	rVV3	1405	706	0.05%	0.009%
56	10.548	2955	2957	2959	rBV3	1395	884	0.07%	0.011%
57	10.577	2964	2966	2967	rBV3	1276	600	0.05%	0.008%
58	10.757	3020	3022	3027	rVB5	1586	907	0.07%	0.011%
59	10.783	3027	3030	3031	rBV4	1498	755	0.06%	0.010%
60	10.973	3087	3089	3096	rVB7	2150	2190	0.17%	0.028%
61	11.024	3101	3105	3107	rBV4	1430	891	0.07%	0.011%
62	11.053	3112	3114	3120	rVB7	1606	1188	0.09%	0.015%
63	11.092	3123	3126	3127	rBV3	1157	634	0.05%	0.008%
64	11.194	3146	3158	3178	rBV	446809	719929	54.76%	9.097%
65	11.503	3251	3254	3257	rBV5	1038	653	0.05%	0.008%
66	11.571	3264	3275	3292	rBV	344398	560350	42.62%	7.080%
67	11.754	3328	3332	3335	rVB5	1836	1343	0.10%	0.017%
68	11.773	3335	3338	3342	rBV5	1301	1043	0.08%	0.013%
69	11.911	3377	3381	3382	rBV3	1899	1310	0.10%	0.017%
70	11.969	3396	3399	3402	rVV4	1763	1529	0.12%	0.019%
71	11.998	3406	3408	3412	rVV5	1247	592	0.05%	0.007%
72	12.230	3477	3480	3483	rBV5	1290	999	0.08%	0.013%
73	12.471	3552	3555	3558	rBV4	1118	833	0.06%	0.011%
74	12.503	3562	3565	3567	rBV4	1437	720	0.05%	0.009%
75	12.657	3611	3613	3616	rBV4	1993	1284	0.10%	0.016%
76	12.731	3633	3636	3639	rVV5	1449	1097	0.08%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030717.D
 Acq On : 20 Apr 2023 15:23
 Operator : SY/MD
 Sample : 02411-09 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.802	3654	3658	3660	rBV5	719	568	0.04%	0.007%
78	12.818	3660	3663	3665	rVB3	1545	711	0.05%	0.009%
79	12.834	3665	3668	3671	rBV5	845	592	0.05%	0.007%
80	12.866	3675	3678	3680	rBV4	1345	857	0.07%	0.011%
81	13.014	3722	3724	3728	rBV5	1357	980	0.07%	0.012%
82	13.066	3737	3740	3742	rBV4	1373	579	0.04%	0.007%
83	13.111	3750	3754	3756	rBV4	1239	913	0.07%	0.012%
84	13.136	3760	3762	3766	rVB5	1123	651	0.05%	0.008%
85	13.204	3780	3783	3785	rBV5	1473	719	0.05%	0.009%
86	13.365	3831	3833	3836	rVB4	1359	742	0.06%	0.009%
87	13.419	3848	3850	3854	rBV4	1177	978	0.07%	0.012%
88	13.493	3871	3873	3876	rVB4	1236	678	0.05%	0.009%
89	13.513	3876	3879	3880	rBV3	1472	929	0.07%	0.012%
90	13.545	3887	3889	3890	rBV2	1404	612	0.05%	0.008%
91	13.593	3903	3904	3908	rBV4	1362	878	0.07%	0.011%
92	13.654	3919	3923	3925	rVB5	1588	985	0.07%	0.012%
93	13.805	3968	3970	3972	rBV3	1252	698	0.05%	0.009%
94	13.924	4002	4007	4012	rVB8	1620	1454	0.11%	0.018%
95	13.953	4012	4016	4018	rBV4	1759	1414	0.11%	0.018%
96	13.985	4023	4026	4027	rBV3	1494	631	0.05%	0.008%
97	14.053	4045	4047	4049	rBV3	959	569	0.04%	0.007%
98	14.378	4143	4148	4151	rBV7	1568	1737	0.13%	0.022%
99	14.490	4179	4183	4184	rBV4	1123	737	0.06%	0.009%
100	14.953	4324	4327	4329	rBV4	1126	679	0.05%	0.009%




Sum of corrected areas: 7914259

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030717.D
Acq On : 20 Apr 2023 15:23
Operator : SY/MD
Sample : 02411-09 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

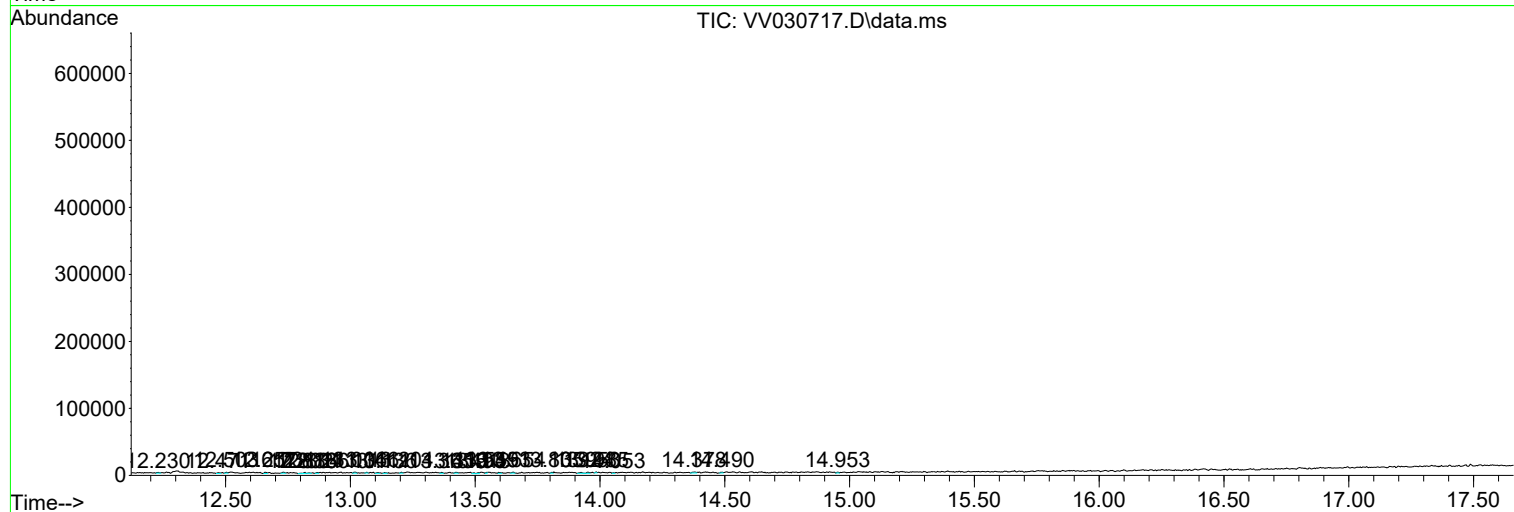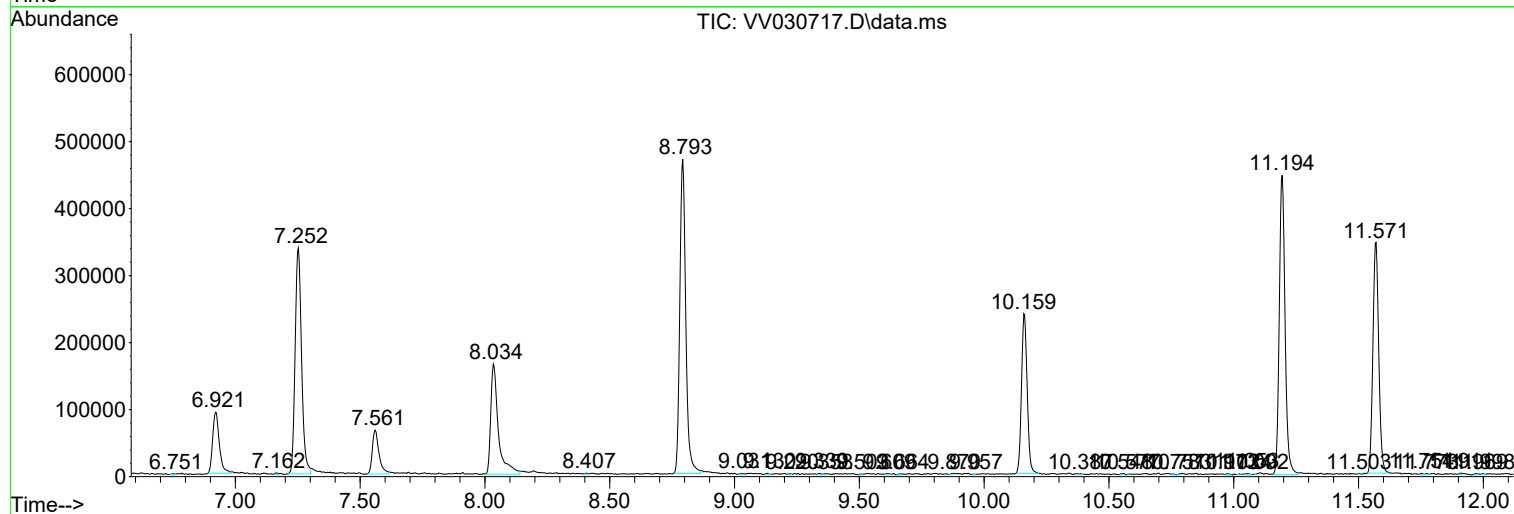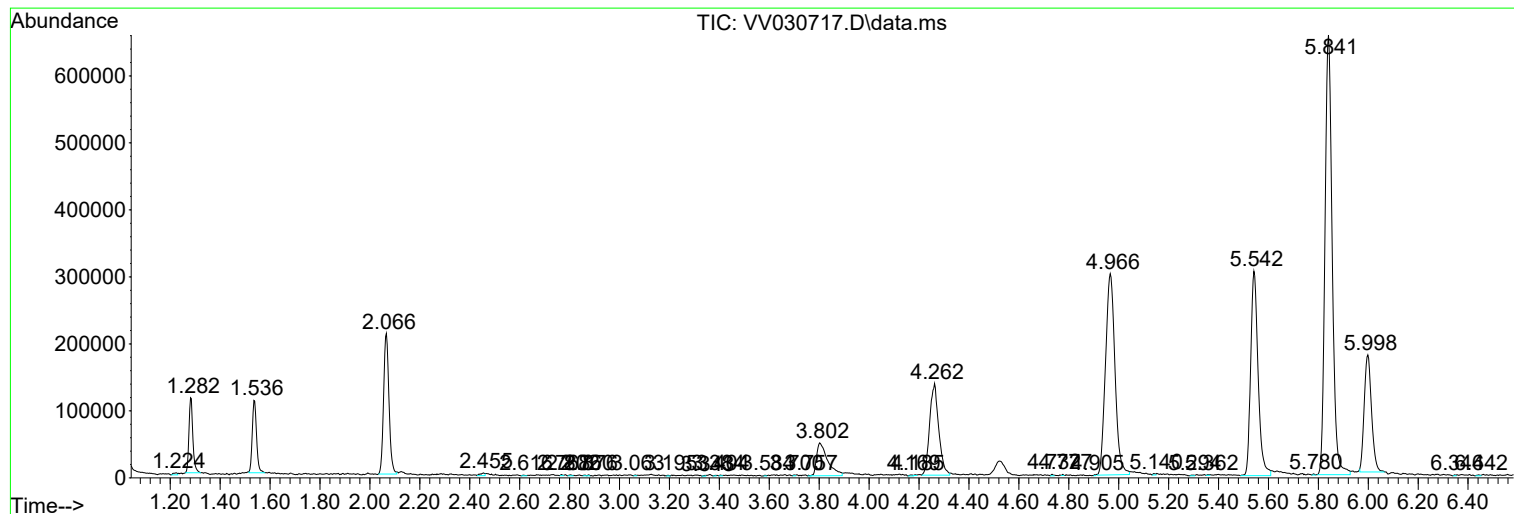

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030717.D
Acq On : 20 Apr 2023 15:23
Operator : SY/MD
Sample : 02411-09 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030717.D
Acq On : 20 Apr 2023 15:23
Operator : SY/MD
Sample : 02411-09 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc