

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030718.D
 Acq On : 20 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02411-19 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	92	rVB	109890	121196	11.03%	1.616%
2	1.539	148	155	170	rVB	103254	120252	10.94%	1.603%
3	1.925	273	275	277	rBV3	1877	774	0.07%	0.010%
4	2.066	309	319	336	rBV	207258	308297	28.06%	4.110%
5	2.269	380	382	383	rBV2	1407	572	0.05%	0.008%
6	2.574	475	477	480	rBV3	1530	905	0.08%	0.012%
7	2.629	491	494	496	rBV3	977	747	0.07%	0.010%
8	2.667	503	506	510	rBV6	1101	870	0.08%	0.012%
9	2.706	516	518	521	rVB3	1633	981	0.09%	0.013%
10	2.928	585	587	590	rBV4	1373	651	0.06%	0.009%
11	2.944	590	592	594	rVV3	1617	761	0.07%	0.010%
12	2.963	594	598	601	rBV6	1533	989	0.09%	0.013%
13	3.073	629	632	638	rVB8	1205	1150	0.10%	0.015%
14	3.098	638	640	643	rBV4	1290	808	0.07%	0.011%
15	3.262	688	691	694	rVV4	1009	971	0.09%	0.013%
16	3.352	714	719	721	rBV6	1006	950	0.09%	0.013%
17	3.491	757	762	765	rBV6	1544	1499	0.14%	0.020%
18	3.510	765	768	773	rBV7	1111	806	0.07%	0.011%
19	3.558	781	783	787	rBV5	1620	1343	0.12%	0.018%
20	3.619	798	802	806	rBV7	1718	1831	0.17%	0.024%
21	3.658	812	814	818	rVB5	1329	933	0.08%	0.012%
22	3.677	818	820	824	rVB5	1031	703	0.06%	0.009%
23	3.709	828	830	834	rVB6	1208	700	0.06%	0.009%
24	3.809	850	861	882	rBV2	49626	153931	14.01%	2.052%
25	4.095	949	950	953	rBV3	1085	769	0.07%	0.010%
26	4.259	988	1001	1019	rBV	124524	305301	27.78%	4.070%
27	4.526	1070	1084	1106	rVB2	25134	69247	6.30%	0.923%
28	4.966	1203	1221	1245	rBV3	293332	778325	70.83%	10.377%
29	5.233	1302	1304	1305	rBV2	1775	737	0.07%	0.010%
30	5.542	1387	1400	1421	rBV	283817	591796	53.86%	7.890%
31	5.841	1480	1493	1510	rBV	557878	1098860	100.00%	14.650%
32	5.998	1532	1542	1567	rVB	169573	349288	31.79%	4.657%
33	6.355	1650	1653	1655	rBV4	1843	1035	0.09%	0.014%
34	6.436	1676	1678	1680	rVB3	1332	592	0.05%	0.008%
35	6.455	1680	1684	1686	rBV4	1295	862	0.08%	0.011%
36	6.545	1708	1712	1713	rBV4	1685	1025	0.09%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030718.D
 Acq On : 20 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02411-19 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.609	1729	1732	1735	rBV4	1824	1225	0.11%	0.016%
38	6.793	1784	1789	1792	rBV6	1473	1266	0.12%	0.017%
39	6.921	1819	1829	1845	rBV	85828	163745	14.90%	2.183%
40	7.056	1867	1871	1874	rVB4	1883	1476	0.13%	0.020%
41	7.252	1917	1932	1954	rBV	323697	586386	53.36%	7.818%
42	7.503	2008	2010	2013	rBV4	1282	613	0.06%	0.008%
43	7.561	2019	2028	2044	rBV2	62194	113035	10.29%	1.507%
44	7.809	2101	2105	2107	rBV4	2595	2296	0.21%	0.031%
45	7.876	2124	2126	2129	rBV4	1023	690	0.06%	0.009%
46	7.895	2130	2132	2135	rVB3	1392	715	0.07%	0.010%
47	8.034	2166	2175	2204	rVV	158503	337309	30.70%	4.497%
48	8.481	2310	2314	2315	rBV4	2071	1321	0.12%	0.018%
49	8.645	2362	2365	2367	rBV4	1552	921	0.08%	0.012%
50	8.731	2390	2392	2395	rVB4	1419	710	0.06%	0.009%
51	8.751	2395	2398	2399	rBV3	1933	1063	0.10%	0.014%
52	8.793	2400	2411	2437	rVV	438047	735281	66.91%	9.803%
53	9.407	2600	2602	2605	rBV3	1320	643	0.06%	0.009%
54	9.493	2627	2629	2630	rBV2	1432	622	0.06%	0.008%
55	9.522	2636	2638	2640	rBV3	1158	581	0.05%	0.008%
56	9.645	2673	2676	2678	rBV3	992	687	0.06%	0.009%
57	9.799	2722	2724	2726	rBV3	1461	715	0.07%	0.010%
58	9.863	2742	2744	2749	rVB6	1453	1057	0.10%	0.014%
59	9.953	2770	2772	2775	rVB3	1429	576	0.05%	0.008%
60	9.995	2783	2785	2790	rBV5	1670	1118	0.10%	0.015%
61	10.024	2790	2794	2797	rVB5	1672	1360	0.12%	0.018%
62	10.043	2797	2800	2801	rBV3	1170	593	0.05%	0.008%
63	10.159	2826	2836	2855	rBV	229942	367410	33.44%	4.898%
64	10.413	2913	2915	2918	rBV4	1342	614	0.06%	0.008%
65	10.455	2926	2928	2930	rBV3	1585	896	0.08%	0.012%
66	10.902	3066	3067	3071	rVB4	2079	911	0.08%	0.012%
67	10.963	3083	3086	3087	rBV3	1372	817	0.07%	0.011%
68	11.079	3119	3122	3124	rBV4	1285	860	0.08%	0.011%
69	11.194	3145	3158	3179	rBV	426157	685578	62.39%	9.140%
70	11.391	3218	3219	3222	rVB3	1814	716	0.07%	0.010%
71	11.571	3264	3275	3292	rVV	331119	537408	48.91%	7.165%
72	11.673	3305	3307	3310	rBV3	1965	1302	0.12%	0.017%
73	11.757	3331	3333	3337	rBV4	1432	1190	0.11%	0.016%
74	11.841	3357	3359	3364	rBV5	1098	613	0.06%	0.008%
75	11.882	3367	3372	3374	rBV6	1754	1725	0.16%	0.023%
76	12.169	3457	3461	3463	rBV5	1295	1101	0.10%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030718.D
 Acq On : 20 Apr 2023 15:47
 Operator : SY/MD
 Sample : 02411-19 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.265	3488	3491	3492	rVV2	1446	757	0.07%	0.010%
78	12.304	3501	3503	3508	rBV6	856	770	0.07%	0.010%
79	12.419	3537	3539	3542	rVB4	1406	806	0.07%	0.011%
80	12.455	3548	3550	3555	rVB6	1659	1445	0.13%	0.019%
81	12.558	3579	3582	3584	rBV3	1008	621	0.06%	0.008%
82	12.574	3584	3587	3591	rBV5	1685	1423	0.13%	0.019%
83	12.667	3613	3616	3620	rBV5	968	712	0.06%	0.009%
84	12.754	3638	3643	3645	rBV5	1674	1187	0.11%	0.016%
85	12.770	3645	3648	3653	rVV6	1935	1225	0.11%	0.016%
86	12.818	3660	3663	3664	rBV3	1255	715	0.07%	0.010%
87	12.956	3704	3706	3710	rBV5	1172	766	0.07%	0.010%
88	13.043	3729	3733	3735	rBV5	1663	966	0.09%	0.013%
89	13.152	3765	3767	3770	rBV4	1880	1263	0.11%	0.017%
90	13.178	3773	3775	3777	rBV3	1180	566	0.05%	0.008%
91	13.246	3794	3796	3800	rBV5	1267	1174	0.11%	0.016%
92	13.365	3830	3833	3835	rBV4	2071	1427	0.13%	0.019%
93	13.435	3851	3855	3856	rBV3	1139	865	0.08%	0.012%
94	13.487	3869	3871	3874	rVB4	1267	670	0.06%	0.009%
95	13.503	3874	3876	3879	rBV3	976	607	0.06%	0.008%
96	13.873	3988	3991	3992	rBV4	1312	707	0.06%	0.009%
97	14.008	4031	4033	4034	rBV2	1849	809	0.07%	0.011%
98	14.107	4062	4064	4066	rBV3	1742	882	0.08%	0.012%
99	14.834	4288	4290	4295	rBV6	1610	1077	0.10%	0.014%
100	14.966	4327	4331	4334	rBV6	1774	1774	0.16%	0.024%




Sum of corrected areas: 7500816

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030718.D
Acq On : 20 Apr 2023 15:47
Operator : SY/MD
Sample : 02411-19 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

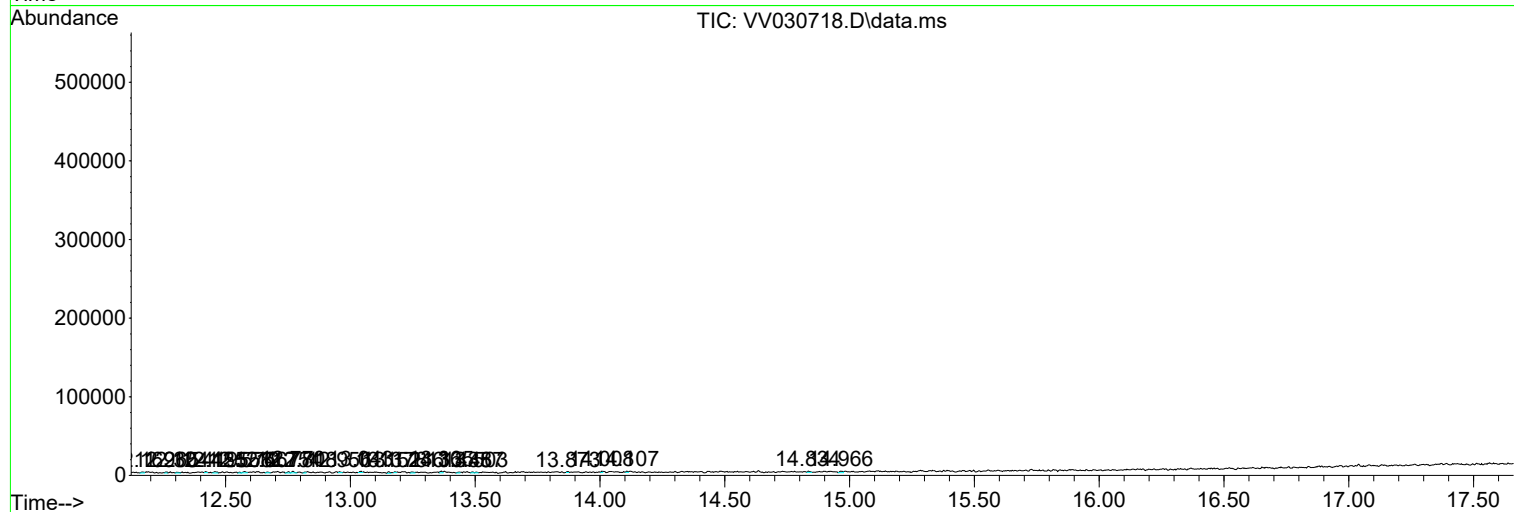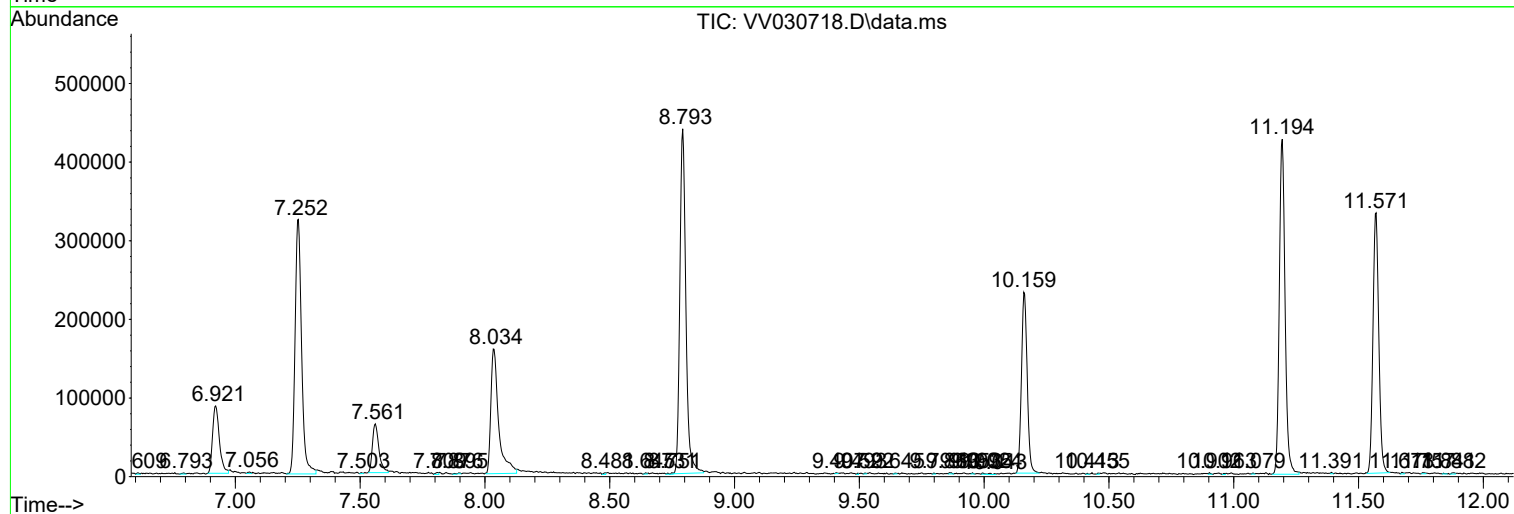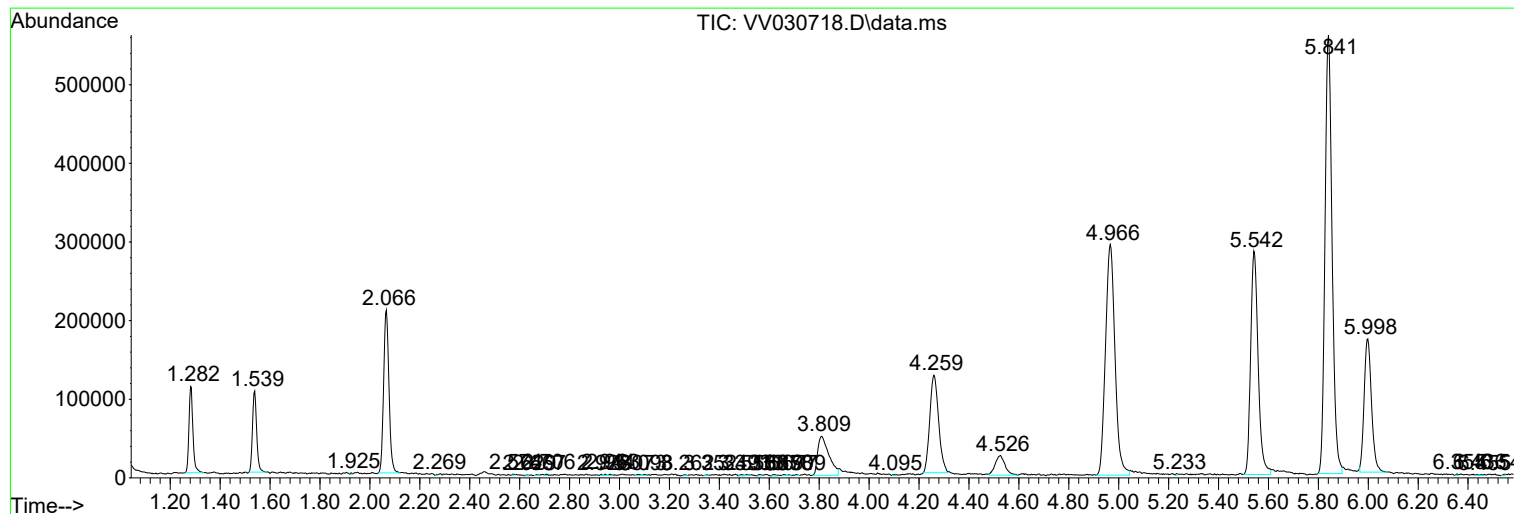

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030718.D
Acq On : 20 Apr 2023 15:47
Operator : SY/MD
Sample : 02411-19 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030718.D
Acq On : 20 Apr 2023 15:47
Operator : SY/MD
Sample : 02411-19 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------