

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030720.D
 Acq On : 20 Apr 2023 16:33
 Operator : SY/MD
 Sample : 02334-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	87	rBV	111624	122030	15.14%	1.857%
2	1.535	148	154	171	rVB	111881	134089	16.64%	2.041%
3	2.066	310	319	334	rBV	211002	306784	38.07%	4.669%
4	2.439	431	435	436	rBV4	1933	1123	0.14%	0.017%
5	2.629	492	494	498	rBV4	1154	805	0.10%	0.012%
6	2.648	498	500	505	rVB5	1008	698	0.09%	0.011%
7	2.760	532	535	537	rBV3	975	699	0.09%	0.011%
8	2.825	553	555	560	rVB5	1522	1339	0.17%	0.020%
9	2.863	560	567	569	rBV7	1293	1450	0.18%	0.022%
10	2.941	589	591	597	rVB7	1462	858	0.11%	0.013%
11	2.976	597	602	607	rBV8	2510	2863	0.36%	0.044%
12	3.101	639	641	644	rBV3	1858	1333	0.17%	0.020%
13	3.166	657	661	667	rVB8	1900	2092	0.26%	0.032%
14	3.201	667	672	674	rBV6	1261	1023	0.13%	0.016%
15	3.297	697	702	704	rBV6	1321	1022	0.13%	0.016%
16	3.391	729	731	733	rBV2	1262	762	0.09%	0.012%
17	3.461	750	753	757	rVB5	1699	1348	0.17%	0.021%
18	3.487	757	761	765	rBV6	973	1236	0.15%	0.019%
19	3.625	802	804	809	rVV6	1302	904	0.11%	0.014%
20	3.731	832	837	840	rBV6	1257	1042	0.13%	0.016%
21	3.802	850	859	878	rBV	50386	140601	17.45%	2.140%
22	4.262	989	1002	1027	rVB	132064	328295	40.74%	4.996%
23	4.510	1075	1079	1082	rBV5	1734	1443	0.18%	0.022%
24	4.603	1105	1108	1110	rBV4	1011	691	0.09%	0.011%
25	4.632	1114	1117	1121	rBV4	1218	1035	0.13%	0.016%
26	4.741	1149	1151	1154	rVB3	1495	767	0.10%	0.012%
27	4.966	1202	1221	1244	rBV2	302152	805835	100.00%	12.264%
28	5.542	1386	1400	1423	rVV	293712	619852	76.92%	9.433%
29	5.738	1457	1461	1462	rBV4	2032	1444	0.18%	0.022%
30	5.998	1530	1542	1564	rBV2	175319	360141	44.69%	5.481%
31	6.529	1704	1707	1708	rBV2	1777	830	0.10%	0.013%
32	6.661	1743	1748	1751	rBV6	1386	1620	0.20%	0.025%
33	6.786	1783	1787	1791	rBV5	990	1139	0.14%	0.017%
34	6.921	1814	1829	1846	rBV	94282	178666	22.17%	2.719%
35	7.252	1919	1932	1950	rBV	342400	604132	74.97%	9.194%
36	7.561	2019	2028	2045	rBV2	66292	122405	15.19%	1.863%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030720.D
 Acq On : 20 Apr 2023 16:33
 Operator : SY/MD
 Sample : 02334-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.860	2118	2121	2122	rBV3	1134	681	0.08%	0.010%
38	7.934	2142	2144	2147	rBV4	1432	699	0.09%	0.011%
39	7.956	2150	2151	2158	rVB6	1473	1163	0.14%	0.018%
40	8.034	2165	2175	2190	rBV	166563	316045	39.22%	4.810%
41	8.455	2304	2306	2310	rBV4	1415	1043	0.13%	0.016%
42	8.529	2325	2329	2330	rBV4	2286	1073	0.13%	0.016%
43	8.561	2336	2339	2340	rBV2	1996	1095	0.14%	0.017%
44	8.673	2370	2374	2375	rBV4	1415	907	0.11%	0.014%
45	8.747	2393	2397	2400	rBV5	1242	882	0.11%	0.013%
46	8.792	2400	2411	2434	rBV	459321	764787	94.91%	11.639%
47	9.027	2482	2484	2487	rVB5	1665	798	0.10%	0.012%
48	9.046	2487	2490	2491	rBV3	1133	687	0.09%	0.010%
49	9.162	2523	2526	2527	rBV3	1546	769	0.10%	0.012%
50	9.194	2533	2536	2537	rBV3	1075	716	0.09%	0.011%
51	9.320	2573	2575	2578	rVB4	1298	668	0.08%	0.010%
52	9.490	2626	2628	2630	rBV3	1354	827	0.10%	0.013%
53	9.538	2640	2643	2645	rBV4	1309	761	0.09%	0.012%
54	9.587	2655	2658	2660	rBV3	1303	720	0.09%	0.011%
55	9.635	2670	2673	2680	rVB7	1567	1510	0.19%	0.023%
56	9.667	2680	2683	2685	rBV5	1285	788	0.10%	0.012%
57	9.725	2699	2701	2705	rVB4	1251	760	0.09%	0.012%
58	10.021	2787	2793	2794	rBV5	1618	1399	0.17%	0.021%
59	10.059	2801	2805	2807	rBV4	1157	1054	0.13%	0.016%
60	10.095	2812	2816	2821	rBV9	1856	2044	0.25%	0.031%
61	10.159	2825	2836	2855	rBV	242743	386098	47.91%	5.876%
62	10.323	2883	2887	2889	rBV3	1591	1285	0.16%	0.020%
63	10.403	2910	2912	2917	rVV6	1264	948	0.12%	0.014%
64	10.442	2922	2924	2927	rVB4	1441	853	0.11%	0.013%
65	10.513	2942	2946	2947	rBV4	1426	897	0.11%	0.014%
66	10.558	2957	2960	2964	rBV4	1250	1245	0.15%	0.019%
67	10.632	2981	2983	2984	rBV	1375	682	0.08%	0.010%
68	10.699	2998	3004	3007	rBV7	1576	1611	0.20%	0.025%
69	10.805	3033	3037	3039	rVB5	1307	955	0.12%	0.015%
70	10.953	3078	3083	3089	rBV5	1421	1599	0.20%	0.024%
71	11.194	3147	3158	3176	rBV	441631	703158	87.26%	10.701%
72	11.451	3235	3238	3241	rBV5	1439	1100	0.14%	0.017%
73	11.570	3264	3275	3300	rVB	350102	576019	71.48%	8.766%
74	12.046	3421	3423	3427	rBV5	1091	748	0.09%	0.011%
75	12.133	3448	3450	3452	rBV2	1022	720	0.09%	0.011%
76	12.191	3464	3468	3470	rBV5	1306	837	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030720.D
 Acq On : 20 Apr 2023 16:33
 Operator : SY/MD
 Sample : 02334-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMH8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.265	3485	3491	3492	rBV4	1034	1064	0.13%	0.016%
78	12.448	3544	3548	3552	rBV5	1223	980	0.12%	0.015%
79	12.493	3558	3562	3563	rBV4	1519	1055	0.13%	0.016%
80	12.538	3571	3576	3579	rBV5	1298	1285	0.16%	0.020%
81	12.612	3595	3599	3600	rBV4	1158	709	0.09%	0.011%
82	12.683	3618	3621	3623	rBV3	1661	978	0.12%	0.015%
83	12.927	3694	3697	3699	rBV4	1317	775	0.10%	0.012%
84	13.065	3737	3740	3742	rBV3	1057	654	0.08%	0.010%
85	13.146	3762	3765	3767	rBV3	1853	1131	0.14%	0.017%
86	13.210	3777	3785	3794	rBV9	8849	15016	1.86%	0.229%
87	13.458	3860	3862	3866	rBV4	1107	755	0.09%	0.011%
88	13.532	3882	3885	3887	rVB4	1588	982	0.12%	0.015%
89	13.548	3887	3890	3892	rBV4	1532	1178	0.15%	0.018%
90	13.741	3948	3950	3953	rBV4	944	694	0.09%	0.011%
91	13.799	3965	3968	3970	rBV4	1421	753	0.09%	0.011%
92	14.088	4054	4058	4061	rBV6	1263	870	0.11%	0.013%
93	14.184	4083	4088	4090	rBV6	1503	1474	0.18%	0.022%
94	14.210	4093	4096	4097	rBV2	1322	754	0.09%	0.011%
95	14.239	4103	4105	4109	rVB4	1580	1101	0.14%	0.017%
96	14.278	4114	4117	4120	rBV5	1637	1307	0.16%	0.020%
97	14.303	4122	4125	4129	rBV5	1203	887	0.11%	0.013%
98	14.487	4180	4182	4187	rBV6	1360	1025	0.13%	0.016%
99	14.538	4194	4198	4199	rBV3	2156	1352	0.17%	0.021%
100	15.036	4351	4353	4356	rVB4	1819	989	0.12%	0.015%




Sum of corrected areas: 6570795

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030720.D
Acq On : 20 Apr 2023 16:33
Operator : SY/MD
Sample : 02334-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

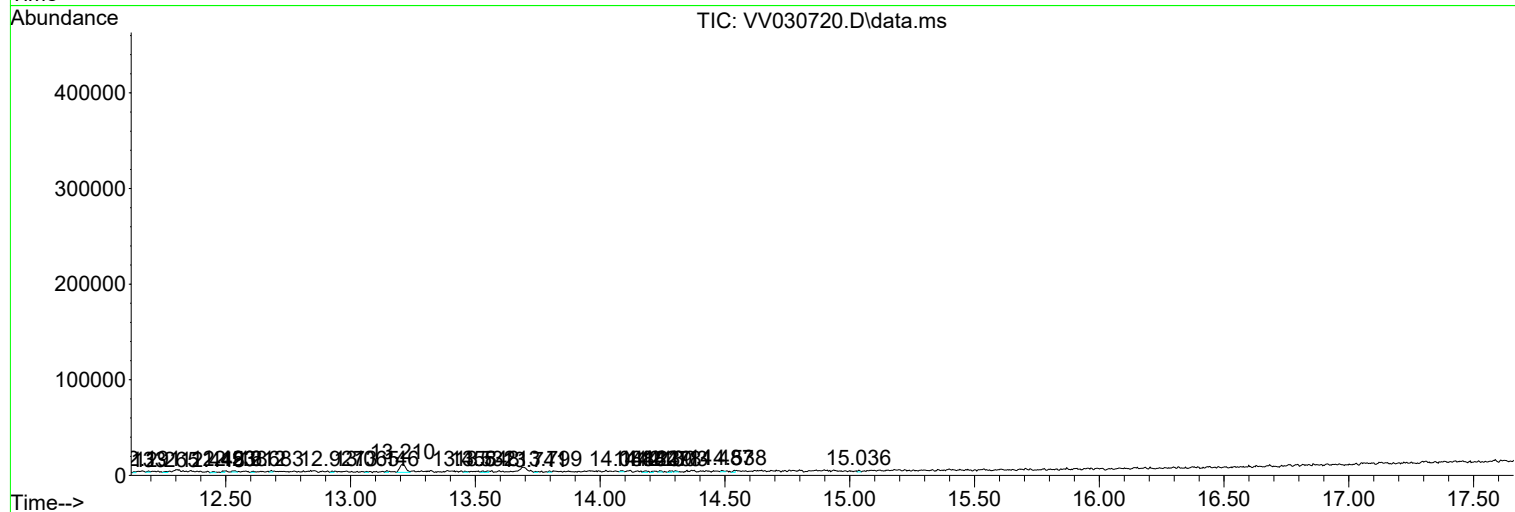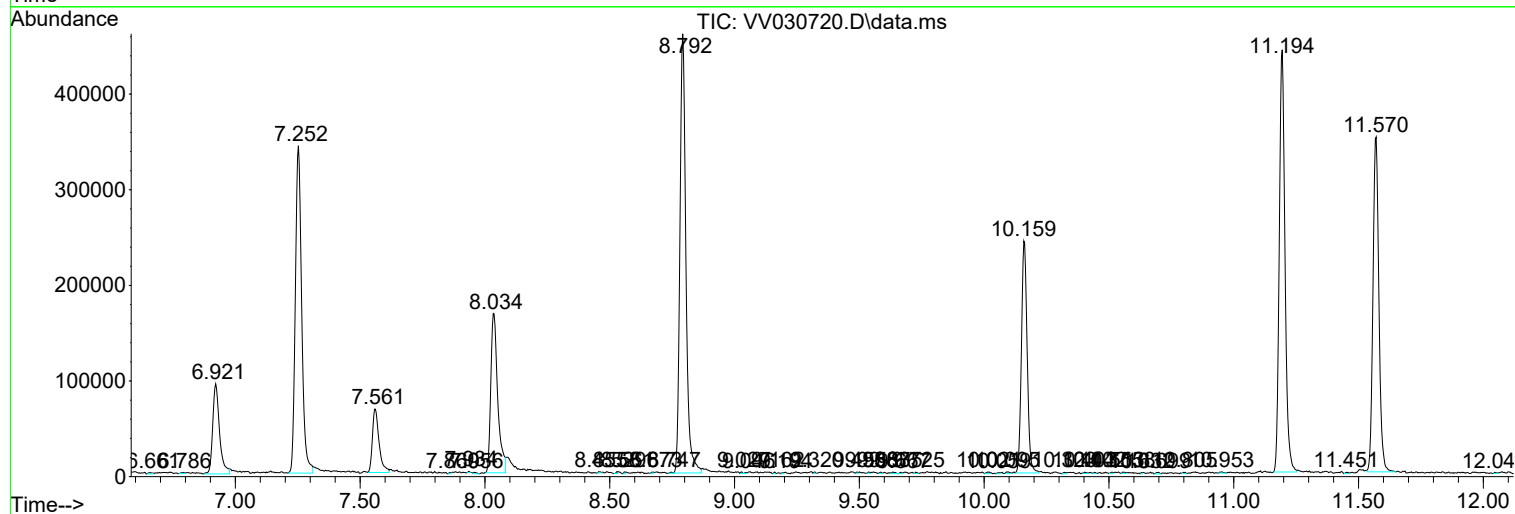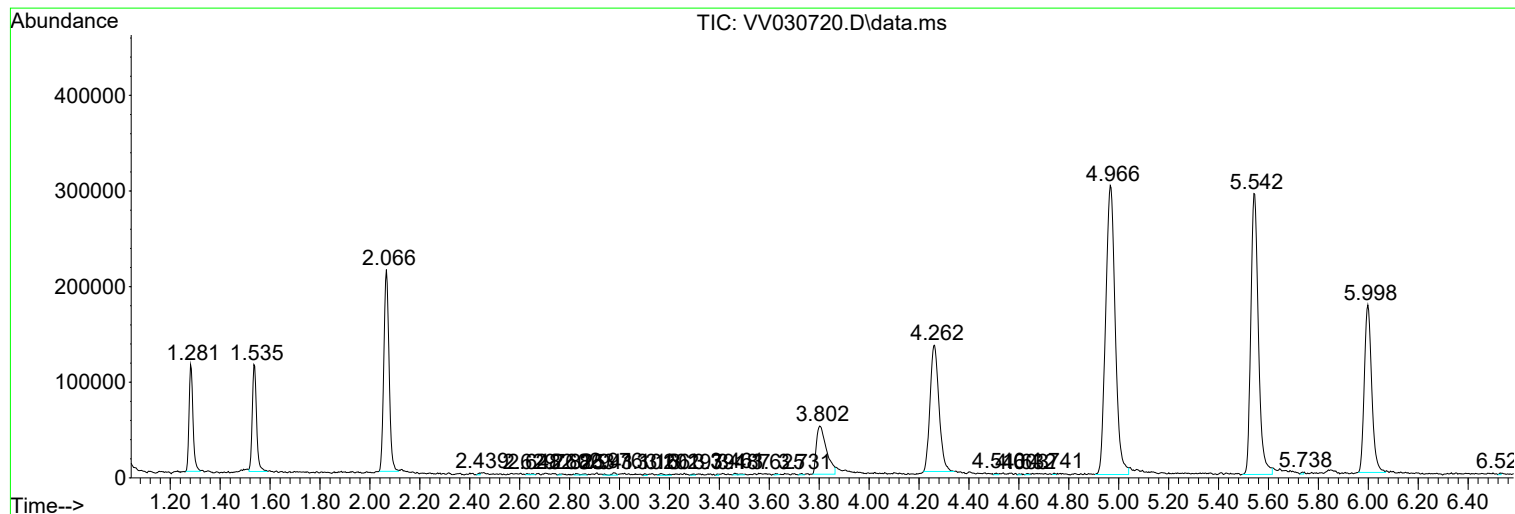

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030720.D
Acq On : 20 Apr 2023 16:33
Operator : SY/MD
Sample : 02334-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030720.D
Acq On : 20 Apr 2023 16:33
Operator : SY/MD
Sample : 02334-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMH8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------