

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030722.D
 Acq On : 20 Apr 2023 17:21
 Operator : SY/MD
 Sample : 02411-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	88	rVB	115485	124879	14.83%	1.951%
2	1.539	148	155	168	rVB	111059	131826	15.65%	2.059%
3	2.066	310	319	331	rVB	216898	312038	37.06%	4.874%
4	2.462	439	442	446	rBV6	1497	1268	0.15%	0.020%
5	2.561	471	473	475	rBV3	1712	816	0.10%	0.013%
6	2.609	484	488	490	rBV5	1129	778	0.09%	0.012%
7	2.642	496	498	501	rBV4	992	699	0.08%	0.011%
8	3.005	606	611	614	rBV5	1748	1369	0.16%	0.021%
9	3.101	638	641	642	rBV3	1492	768	0.09%	0.012%
10	3.182	664	666	670	rVB5	2052	1373	0.16%	0.021%
11	3.204	670	673	678	rBV4	1309	1224	0.15%	0.019%
12	3.294	695	701	704	rBV7	1959	1932	0.23%	0.030%
13	3.445	744	748	753	rVB7	1465	1440	0.17%	0.022%
14	3.474	753	757	758	rBV4	1669	1052	0.12%	0.016%
15	3.552	779	781	785	rBV6	1160	944	0.11%	0.015%
16	3.638	804	808	812	rBV6	1333	1182	0.14%	0.018%
17	3.699	823	827	829	rBV4	1647	1237	0.15%	0.019%
18	3.767	845	848	850	rBV3	1428	1079	0.13%	0.017%
19	3.802	850	859	882	rBV	49962	139326	16.55%	2.176%
20	4.259	986	1001	1022	rBV	136538	350574	41.63%	5.476%
21	4.648	1119	1122	1124	rBV4	1037	720	0.09%	0.011%
22	4.683	1129	1133	1135	rBV4	2040	1367	0.16%	0.021%
23	4.966	1200	1221	1245	rBV2	314210	842089	100.00%	13.154%
24	5.484	1380	1382	1383	rBV2	1296	706	0.08%	0.011%
25	5.542	1389	1400	1425	rBV	244510	508704	60.41%	7.946%
26	5.995	1528	1541	1565	rBV	185194	387611	46.03%	6.055%
27	6.243	1616	1618	1620	rBV3	1263	738	0.09%	0.012%
28	6.336	1644	1647	1650	rBV5	2212	1396	0.17%	0.022%
29	6.362	1653	1655	1659	rVB4	2081	1353	0.16%	0.021%
30	6.384	1659	1662	1665	rBV6	1561	1328	0.16%	0.021%
31	6.458	1682	1685	1687	rBV4	1738	966	0.11%	0.015%
32	6.658	1745	1747	1751	rBV5	1058	775	0.09%	0.012%
33	6.715	1761	1765	1767	rBV5	1380	1141	0.14%	0.018%
34	6.921	1817	1829	1849	rBV	95622	183477	21.79%	2.866%
35	7.252	1918	1932	1953	rBV	355953	638889	75.87%	9.980%
36	7.558	2018	2027	2041	rBV	70846	127279	15.11%	1.988%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030722.D
 Acq On : 20 Apr 2023 17:21
 Operator : SY/MD
 Sample : 02411-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.931	2141	2143	2146	rBV4	1215	937	0.11%	0.015%
38	8.034	2166	2175	2191	rBV	167088	319224	37.91%	4.986%
39	8.445	2301	2303	2308	rVB6	1985	1140	0.14%	0.018%
40	8.490	2313	2317	2319	rVV4	1421	752	0.09%	0.012%
41	8.564	2337	2340	2341	rBV2	1585	759	0.09%	0.012%
42	8.651	2364	2367	2370	rBV5	1300	1025	0.12%	0.016%
43	8.693	2374	2380	2382	rBV7	2697	2182	0.26%	0.034%
44	8.792	2400	2411	2438	rVV	381139	642362	76.28%	10.034%
45	9.063	2493	2495	2498	rBV4	1012	695	0.08%	0.011%
46	9.188	2531	2534	2537	rBV4	1173	727	0.09%	0.011%
47	9.207	2537	2540	2542	rBV4	1190	749	0.09%	0.012%
48	9.503	2628	2632	2634	rBV5	1385	910	0.11%	0.014%
49	9.561	2648	2650	2655	rVV6	952	724	0.09%	0.011%
50	9.754	2706	2710	2711	rBV4	1606	1127	0.13%	0.018%
51	9.799	2722	2724	2727	rVV4	1322	706	0.08%	0.011%
52	9.831	2730	2734	2737	rBV5	1011	828	0.10%	0.013%
53	9.944	2766	2769	2773	rVB6	1089	731	0.09%	0.011%
54	9.982	2778	2781	2783	rVV3	1733	853	0.10%	0.013%
55	10.046	2799	2801	2806	rVB7	1671	1125	0.13%	0.018%
56	10.072	2806	2809	2811	rBV3	1537	899	0.11%	0.014%
57	10.114	2820	2822	2825	rVB4	1784	1058	0.13%	0.017%
58	10.162	2825	2837	2852	rBV	249921	404995	48.09%	6.326%
59	10.484	2935	2937	2939	rBV3	1104	724	0.09%	0.011%
60	10.522	2946	2949	2955	rVB6	1613	1375	0.16%	0.021%
61	10.612	2975	2977	2980	rBV4	1486	920	0.11%	0.014%
62	10.741	3015	3017	3021	rVB5	1693	899	0.11%	0.014%
63	10.850	3049	3051	3053	rBV2	1385	704	0.08%	0.011%
64	10.924	3072	3074	3078	rBV3	1454	1010	0.12%	0.016%
65	10.982	3089	3092	3095	rBV5	1675	1100	0.13%	0.017%
66	11.098	3123	3128	3129	rBV4	1877	1440	0.17%	0.022%
67	11.194	3145	3158	3178	rBV	368621	596057	70.78%	9.310%
68	11.365	3208	3211	3214	rBV5	1908	1343	0.16%	0.021%
69	11.381	3214	3216	3218	rBV3	1245	710	0.08%	0.011%
70	11.452	3235	3238	3241	rVB5	1436	716	0.09%	0.011%
71	11.570	3264	3275	3293	rVB	357205	582128	69.13%	9.093%
72	11.921	3379	3384	3388	rBV7	1659	1657	0.20%	0.026%
73	12.062	3424	3428	3431	rVB4	1667	1192	0.14%	0.019%
74	12.130	3446	3449	3451	rVB5	1532	905	0.11%	0.014%
75	12.146	3451	3454	3457	rBV5	1430	1021	0.12%	0.016%
76	12.297	3492	3501	3513	rBV8	12841	23346	2.77%	0.365%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030722.D
 Acq On : 20 Apr 2023 17:21
 Operator : SY/MD
 Sample : 02411-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.439	3540	3545	3547	rBV6	1129	967	0.11%	0.015%
78	12.496	3559	3563	3567	rVB6	1186	952	0.11%	0.015%
79	12.599	3590	3595	3597	rVB3	1467	1158	0.14%	0.018%
80	12.860	3674	3676	3679	rVB4	1501	721	0.09%	0.011%
81	12.924	3693	3696	3698	rBV4	1691	1208	0.14%	0.019%
82	13.021	3722	3726	3727	rVB4	1181	744	0.09%	0.012%
83	13.066	3736	3740	3743	rVB5	1527	1128	0.13%	0.018%
84	13.136	3759	3762	3764	rBV4	1417	874	0.10%	0.014%
85	13.197	3779	3781	3782	rBV2	1767	963	0.11%	0.015%
86	13.304	3808	3814	3820	rBV8	1905	2323	0.28%	0.036%
87	13.342	3823	3826	3830	rBV5	2098	1326	0.16%	0.021%
88	13.451	3856	3860	3866	rBV9	2035	2014	0.24%	0.031%
89	13.590	3899	3903	3907	rBV6	1180	1141	0.14%	0.018%
90	13.882	3990	3994	3995	rBV4	1381	895	0.11%	0.014%
91	14.062	4048	4050	4056	rBV6	1557	1215	0.14%	0.019%
92	14.095	4056	4060	4061	rBV3	1106	835	0.10%	0.013%
93	14.320	4128	4130	4133	rVB5	2103	902	0.11%	0.014%
94	14.336	4133	4135	4138	rBV4	1512	851	0.10%	0.013%
95	14.455	4170	4172	4174	rBV2	1522	717	0.09%	0.011%
96	14.648	4230	4232	4237	rBV5	1105	732	0.09%	0.011%
97	14.802	4277	4280	4283	rBV5	1826	1097	0.13%	0.017%
98	14.821	4284	4286	4289	rBV4	1426	842	0.10%	0.013%
99	14.940	4319	4323	4325	rBV5	2001	1318	0.16%	0.021%
100	14.956	4325	4328	4330	rBV3	1690	985	0.12%	0.015%




Sum of corrected areas: 6402006

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030722.D
Acq On : 20 Apr 2023 17:21
Operator : SY/MD
Sample : 02411-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

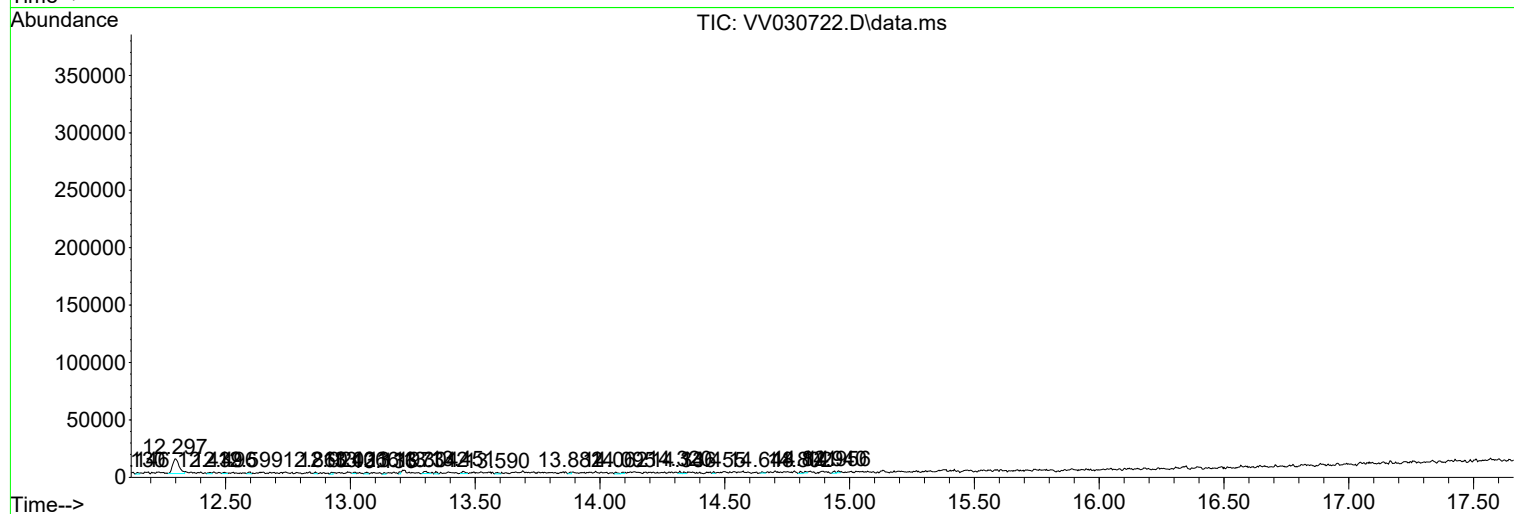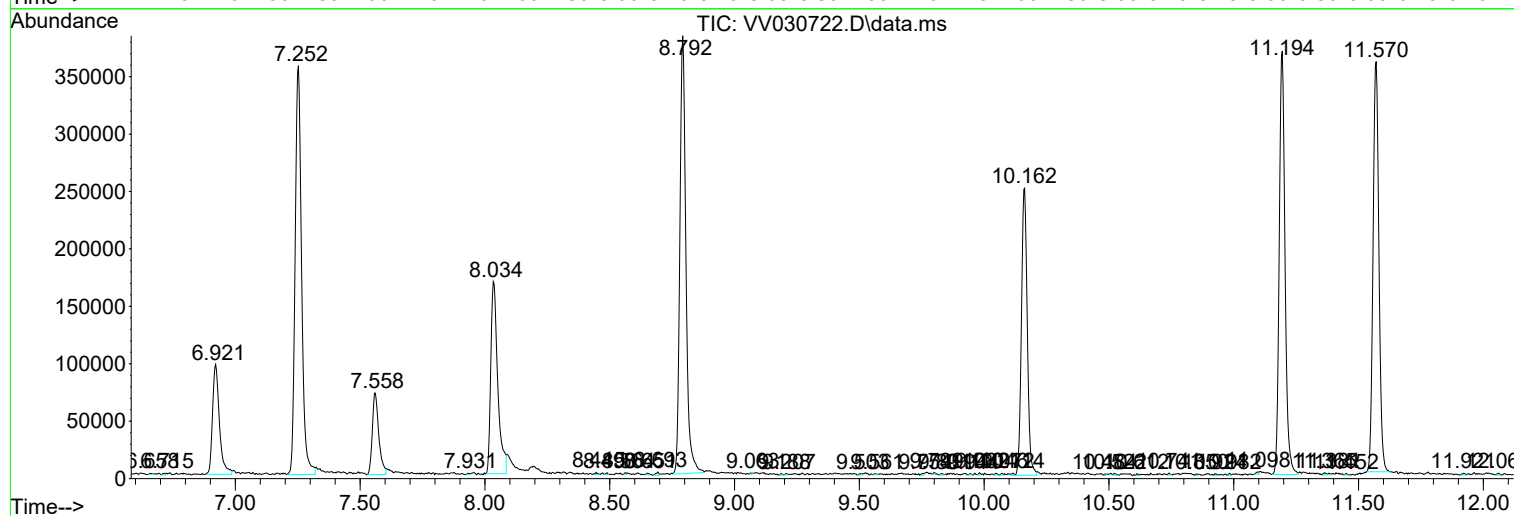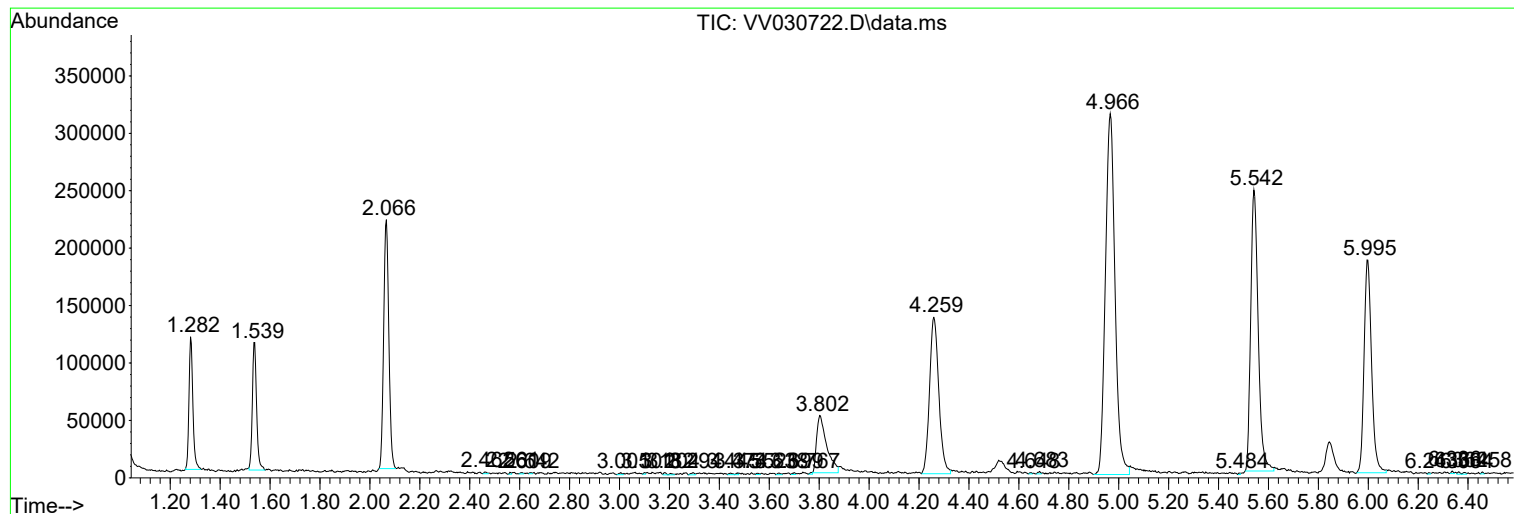

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030722.D
Acq On : 20 Apr 2023 17:21
Operator : SY/MD
Sample : 02411-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030722.D
Acq On : 20 Apr 2023 17:21
Operator : SY/MD
Sample : 02411-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------