

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030723.D
 Acq On : 20 Apr 2023 17:45
 Operator : SY/MD
 Sample : 02411-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rVB	112404	123721	15.90%	1.899%
2	1.539	148	155	170	rVB	100198	123384	15.85%	1.894%
3	2.066	310	319	333	rVB	207041	302650	38.88%	4.646%
4	2.458	437	441	446	rBV8	1987	2482	0.32%	0.038%
5	2.641	494	498	500	rBV5	1448	1039	0.13%	0.016%
6	2.886	571	574	577	rBV4	1071	734	0.09%	0.011%
7	2.934	585	589	590	rBV3	1602	1093	0.14%	0.017%
8	3.021	609	616	620	rBV10	1555	2378	0.31%	0.037%
9	3.297	699	702	705	rVB5	1976	1052	0.14%	0.016%
10	3.391	729	731	736	rVV7	1420	1138	0.15%	0.017%
11	3.429	741	743	747	rVV5	1146	914	0.12%	0.014%
12	3.449	747	749	755	rVV5	1804	1231	0.16%	0.019%
13	3.555	778	782	786	rBV7	1533	1662	0.21%	0.026%
14	3.590	789	793	797	rBV7	843	826	0.11%	0.013%
15	3.738	834	839	842	rBV8	1447	1265	0.16%	0.019%
16	3.757	842	845	846	rBV2	1551	895	0.11%	0.014%
17	3.805	851	860	883	rBV	46864	138286	17.77%	2.123%
18	4.050	935	936	941	rBV5	1508	1041	0.13%	0.016%
19	4.259	987	1001	1026	rBV2	128671	331344	42.57%	5.087%
20	4.680	1128	1132	1134	rBV4	1352	924	0.12%	0.014%
21	4.876	1189	1193	1194	rBV4	1238	812	0.10%	0.012%
22	4.966	1205	1221	1244	rBV2	294599	778363	100.00%	11.950%
23	5.320	1330	1331	1333	rBV2	1509	749	0.10%	0.011%
24	5.542	1387	1400	1421	rBV	299469	622627	79.99%	9.559%
25	5.998	1529	1542	1561	rBV	175022	364397	46.82%	5.594%
26	6.400	1662	1667	1669	rBV4	1990	2007	0.26%	0.031%
27	6.484	1686	1693	1695	rBV6	1521	1700	0.22%	0.026%
28	6.780	1781	1785	1787	rBV5	1333	989	0.13%	0.015%
29	6.834	1799	1802	1804	rBV4	1396	1028	0.13%	0.016%
30	6.921	1819	1829	1846	rBV	88046	167163	21.48%	2.566%
31	7.146	1894	1899	1903	rBV8	1721	1788	0.23%	0.027%
32	7.252	1920	1932	1958	rBV	330355	599402	77.01%	9.202%
33	7.516	2011	2014	2017	rBV4	1530	1108	0.14%	0.017%
34	7.561	2018	2028	2044	rBV2	66755	120934	15.54%	1.857%
35	7.866	2121	2123	2129	rVB6	1265	1013	0.13%	0.016%
36	7.927	2137	2142	2143	rBV5	1535	1214	0.16%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030723.D
 Acq On : 20 Apr 2023 17:45
 Operator : SY/MD
 Sample : 02411-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.969	2148	2155	2160	rBV10	1509	1845	0.24%	0.028%
38	8.034	2163	2175	2207	rBV	154739	331391	42.58%	5.088%
39	8.416	2291	2294	2297	rVB5	1943	1098	0.14%	0.017%
40	8.792	2397	2411	2434	rBV	451117	770366	98.97%	11.827%
41	9.226	2543	2546	2550	rBV6	1207	981	0.13%	0.015%
42	9.464	2617	2620	2621	rBV3	1132	788	0.10%	0.012%
43	9.593	2657	2660	2662	rBV4	1480	896	0.12%	0.014%
44	9.722	2698	2700	2706	rVB6	1381	1071	0.14%	0.016%
45	9.744	2706	2707	2711	rBV4	998	765	0.10%	0.012%
46	9.905	2753	2757	2759	rBV4	1347	921	0.12%	0.014%
47	9.956	2770	2773	2775	rBV4	1208	781	0.10%	0.012%
48	10.159	2825	2836	2856	rVV	230518	377014	48.44%	5.788%
49	10.278	2869	2873	2877	rVB6	1977	1526	0.20%	0.023%
50	10.297	2877	2879	2885	rBV8	1726	1558	0.20%	0.024%
51	10.484	2934	2937	2940	rVV3	1640	987	0.13%	0.015%
52	10.667	2990	2994	2996	rBV5	1357	775	0.10%	0.012%
53	10.976	3087	3090	3092	rVB4	1588	1047	0.13%	0.016%
54	11.066	3114	3118	3120	rBV5	1223	852	0.11%	0.013%
55	11.130	3137	3138	3142	rVB3	1766	764	0.10%	0.012%
56	11.194	3147	3158	3176	rVV	442455	700703	90.02%	10.757%
57	11.397	3219	3221	3226	rBV6	2244	1699	0.22%	0.026%
58	11.513	3255	3257	3261	rVB4	1234	762	0.10%	0.012%
59	11.567	3261	3274	3291	rBV	346571	564406	72.51%	8.665%
60	11.744	3325	3329	3331	rBV5	1388	1195	0.15%	0.018%
61	11.882	3370	3372	3375	rVB4	1680	908	0.12%	0.014%
62	11.934	3384	3388	3393	rBV7	2250	2221	0.29%	0.034%
63	12.066	3426	3429	3432	rVV4	1623	1299	0.17%	0.020%
64	12.088	3434	3436	3440	rBV6	899	771	0.10%	0.012%
65	12.162	3455	3459	3460	rBV3	1525	1231	0.16%	0.019%
66	12.194	3467	3469	3472	rBV5	1139	746	0.10%	0.011%
67	12.262	3484	3490	3491	rBV6	1403	1282	0.16%	0.020%
68	12.303	3497	3503	3506	rBV6	1618	1921	0.25%	0.029%
69	12.442	3543	3546	3550	rVV4	1480	1312	0.17%	0.020%
70	12.461	3550	3552	3559	rVB7	1480	1173	0.15%	0.018%
71	12.493	3559	3562	3566	rBV6	1744	1504	0.19%	0.023%
72	12.603	3592	3596	3597	rBV3	1436	926	0.12%	0.014%
73	12.635	3605	3606	3609	rBV3	1121	750	0.10%	0.012%
74	12.683	3617	3621	3624	rBV6	1045	976	0.13%	0.015%
75	12.760	3640	3645	3651	rBV8	1180	1506	0.19%	0.023%
76	12.863	3672	3677	3678	rBV4	1367	1170	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030723.D
 Acq On : 20 Apr 2023 17:45
 Operator : SY/MD
 Sample : 02411-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.924	3694	3696	3702	rVB5	1590	1239	0.16%	0.019%
78	12.979	3709	3713	3716	rBV6	1737	1241	0.16%	0.019%
79	13.088	3745	3747	3750	rBV4	1552	1054	0.14%	0.016%
80	13.152	3763	3767	3768	rVV4	1534	1042	0.13%	0.016%
81	13.252	3795	3798	3799	rBV3	1225	799	0.10%	0.012%
82	13.329	3818	3822	3826	rBV6	1630	1286	0.17%	0.020%
83	13.348	3826	3828	3832	rVB5	1494	982	0.13%	0.015%
84	13.438	3852	3856	3858	rVV4	1234	948	0.12%	0.015%
85	13.574	3894	3898	3899	rBV4	1585	1047	0.13%	0.016%
86	13.612	3906	3910	3914	rVB6	2145	1586	0.20%	0.024%
87	13.635	3914	3917	3919	rBV4	1305	802	0.10%	0.012%
88	13.673	3927	3929	3931	rBV2	1523	774	0.10%	0.012%
89	13.783	3961	3963	3968	rBV6	1641	861	0.11%	0.013%
90	13.847	3979	3983	3985	rBV4	1501	1190	0.15%	0.018%
91	13.947	4010	4014	4018	rBV6	1544	1493	0.19%	0.023%
92	13.979	4021	4024	4027	rBV5	1267	1060	0.14%	0.016%
93	14.088	4054	4058	4060	rVB3	1127	866	0.11%	0.013%
94	14.120	4064	4068	4072	rBV6	1744	1578	0.20%	0.024%
95	14.139	4072	4074	4078	rVV4	1416	761	0.10%	0.012%
96	14.348	4135	4139	4142	rBV6	2349	1918	0.25%	0.029%
97	14.381	4147	4149	4150	rBV2	1957	807	0.10%	0.012%
98	14.461	4170	4174	4177	rBV6	1115	897	0.12%	0.014%
99	14.680	4240	4242	4245	rBV4	1621	857	0.11%	0.013%
100	14.908	4310	4313	4316	rBV5	2026	1442	0.19%	0.022%




Sum of corrected areas: 6513770

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030723.D
Acq On : 20 Apr 2023 17:45
Operator : SY/MD
Sample : 02411-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

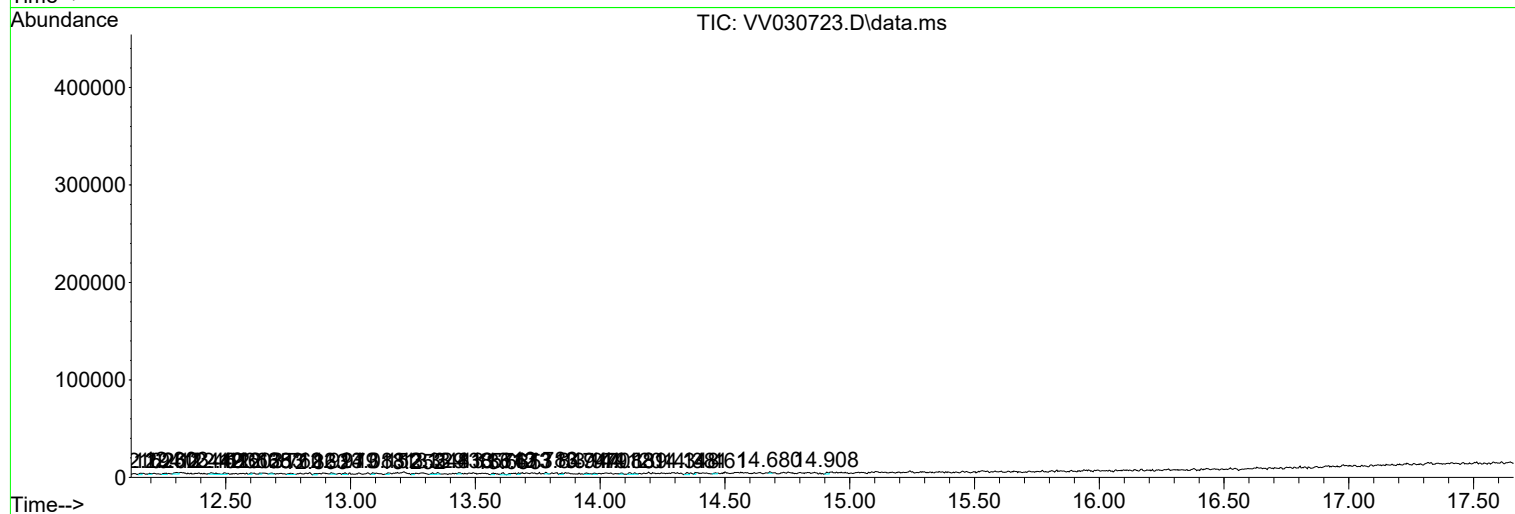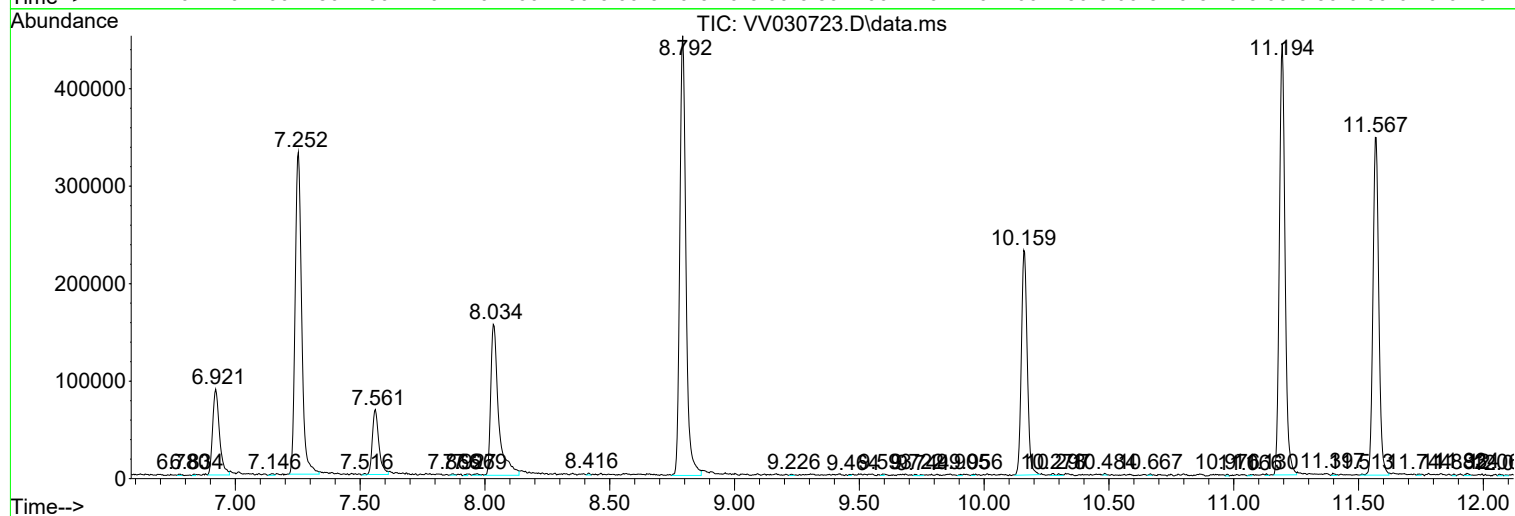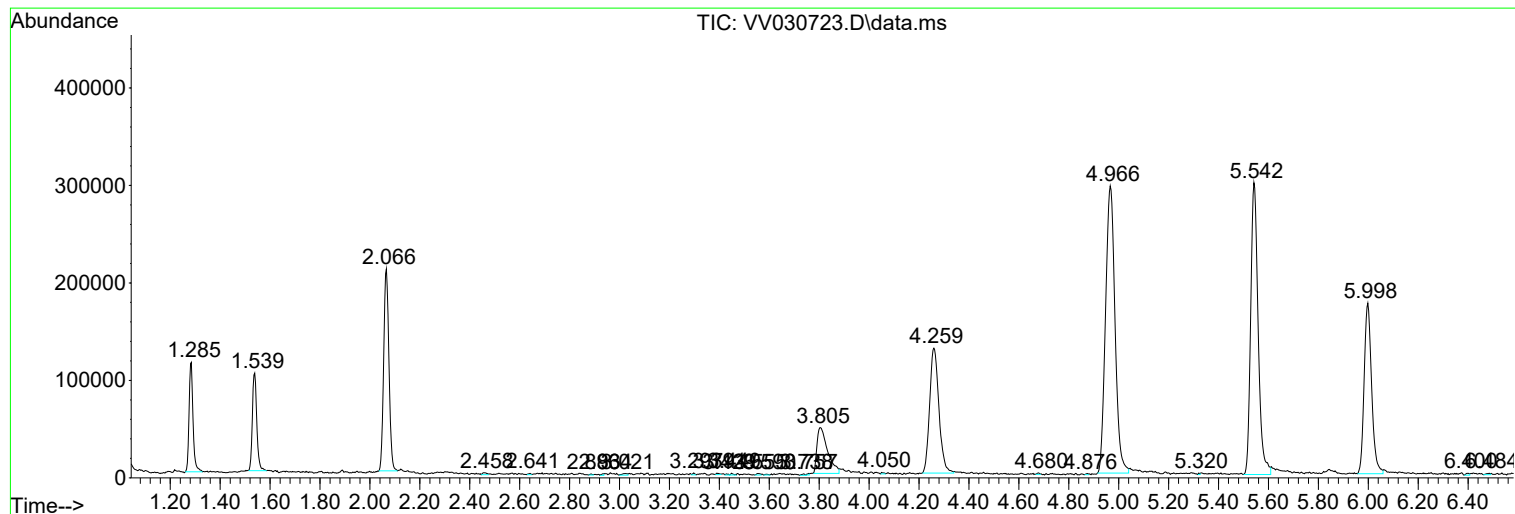

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030723.D
Acq On : 20 Apr 2023 17:45
Operator : SY/MD
Sample : 02411-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030723.D
Acq On : 20 Apr 2023 17:45
Operator : SY/MD
Sample : 02411-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc