

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030724.D
 Acq On : 20 Apr 2023 18:09
 Operator : SY/MD
 Sample : 02411-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	93	rVB	109801	123356	16.19%	1.930%
2	1.452	126	128	133	rBV4	2396	1858	0.24%	0.029%
3	1.539	147	155	169	rBV	103397	121896	16.00%	1.907%
4	2.066	310	319	332	rBV	201120	294851	38.71%	4.614%
5	2.728	520	525	529	rVB8	1514	1364	0.18%	0.021%
6	2.751	529	532	535	rBV5	1571	1353	0.18%	0.021%
7	2.902	574	579	580	rBV4	1356	1201	0.16%	0.019%
8	3.002	606	610	612	rBV4	1348	759	0.10%	0.012%
9	3.240	677	684	685	rBV6	1927	1780	0.23%	0.028%
10	3.355	718	720	723	rVV4	1655	985	0.13%	0.015%
11	3.471	753	756	759	rBV5	1360	1232	0.16%	0.019%
12	3.503	763	766	770	rBV6	872	889	0.12%	0.014%
13	3.551	775	781	784	rBV7	1460	1502	0.20%	0.024%
14	3.651	809	812	813	rVB3	1358	669	0.09%	0.010%
15	3.677	817	820	823	rVB5	984	552	0.07%	0.009%
16	3.696	823	826	829	rBV4	1318	855	0.11%	0.013%
17	3.754	840	844	848	rBV5	1384	1421	0.19%	0.022%
18	3.805	851	860	887	rVV	46160	141575	18.59%	2.215%
19	4.259	984	1001	1025	rBV	124458	329050	43.20%	5.149%
20	4.587	1100	1103	1106	rBV5	1013	644	0.08%	0.010%
21	4.648	1116	1122	1123	rBV6	1386	1133	0.15%	0.018%
22	4.796	1165	1168	1171	rBV5	1046	919	0.12%	0.014%
23	4.892	1194	1198	1202	rBV6	1830	1641	0.22%	0.026%
24	4.966	1205	1221	1246	rVV2	285849	761700	100.00%	11.919%
25	5.375	1346	1348	1349	rBV2	1036	530	0.07%	0.008%
26	5.542	1388	1400	1428	rVV	286889	601427	78.96%	9.411%
27	5.844	1486	1494	1510	rVB2	45899	91428	12.00%	1.431%
28	5.998	1530	1542	1564	rBV	173864	347422	45.61%	5.436%
29	6.645	1737	1743	1746	rBV6	1734	1617	0.21%	0.025%
30	6.754	1775	1777	1780	rBV3	1119	692	0.09%	0.011%
31	6.770	1780	1782	1786	rVB4	1633	918	0.12%	0.014%
32	6.799	1786	1791	1793	rBV6	942	851	0.11%	0.013%
33	6.825	1793	1799	1802	rBV8	1453	1706	0.22%	0.027%
34	6.921	1819	1829	1844	rBV2	87209	160384	21.06%	2.510%
35	7.082	1876	1879	1880	rBV3	1681	944	0.12%	0.015%
36	7.130	1891	1894	1898	rBV4	2468	2456	0.32%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030724.D
 Acq On : 20 Apr 2023 18:09
 Operator : SY/MD
 Sample : 02411-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1921	1932	1953	rBV	316749	568698	74.66%	8.899%
38	7.561	2019	2028	2044	rBV	62328	112147	14.72%	1.755%
39	8.034	2166	2175	2211	rBV	159749	334621	43.93%	5.236%
40	8.448	2301	2304	2305	rBV2	1600	1021	0.13%	0.016%
41	8.635	2359	2362	2365	rVB5	1647	813	0.11%	0.013%
42	8.654	2365	2368	2371	rVB5	1352	942	0.12%	0.015%
43	8.673	2371	2374	2375	rBV3	1850	1022	0.13%	0.016%
44	8.683	2375	2377	2381	rVB5	2006	1211	0.16%	0.019%
45	8.792	2399	2411	2436	rBV	428453	736605	96.71%	11.526%
46	9.136	2515	2518	2519	rBV2	1182	663	0.09%	0.010%
47	9.210	2537	2541	2542	rBV3	1977	1285	0.17%	0.020%
48	9.236	2548	2549	2554	rBV5	902	655	0.09%	0.010%
49	9.281	2561	2563	2567	rVB5	1035	514	0.07%	0.008%
50	9.397	2594	2599	2600	rVV5	1459	1133	0.15%	0.018%
51	9.442	2611	2613	2615	rVB4	1260	586	0.08%	0.009%
52	9.461	2615	2619	2620	rBV3	1145	671	0.09%	0.010%
53	9.783	2716	2719	2721	rBV4	1800	1062	0.14%	0.017%
54	9.927	2762	2764	2767	rVB3	1298	553	0.07%	0.009%
55	10.001	2784	2787	2791	rVB5	1489	1052	0.14%	0.016%
56	10.034	2791	2797	2798	rBV5	1334	1132	0.15%	0.018%
57	10.114	2817	2822	2826	rBV8	1859	2550	0.33%	0.040%
58	10.162	2826	2837	2857	rVV	235675	377804	49.60%	5.912%
59	10.278	2870	2873	2879	rBV7	1395	1328	0.17%	0.021%
60	10.471	2929	2933	2936	rBV5	1178	951	0.12%	0.015%
61	10.513	2943	2946	2947	rBV3	1381	607	0.08%	0.009%
62	10.619	2976	2979	2981	rBV3	1727	1095	0.14%	0.017%
63	10.689	2998	3001	3003	rBV4	1267	958	0.13%	0.015%
64	10.844	3046	3049	3052	rVB6	1194	561	0.07%	0.009%
65	10.915	3070	3071	3073	rBV2	1528	743	0.10%	0.012%
66	11.030	3105	3107	3111	rVV3	1136	608	0.08%	0.010%
67	11.066	3115	3118	3122	rBV6	1199	1103	0.14%	0.017%
68	11.111	3127	3132	3134	rBV6	1843	1314	0.17%	0.021%
69	11.194	3148	3158	3179	rVB	417600	665434	87.36%	10.412%
70	11.313	3192	3195	3200	rVB6	2424	2380	0.31%	0.037%
71	11.371	3211	3213	3218	rBV6	1749	1067	0.14%	0.017%
72	11.567	3264	3274	3293	rVB	333829	537421	70.56%	8.409%
73	11.699	3312	3315	3317	rBV4	1367	827	0.11%	0.013%
74	11.972	3397	3400	3403	rBV4	983	584	0.08%	0.009%
75	11.995	3403	3407	3412	rBV8	1328	1640	0.22%	0.026%
76	12.021	3412	3415	3417	rBV4	976	730	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030724.D
 Acq On : 20 Apr 2023 18:09
 Operator : SY/MD
 Sample : 02411-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.107	3439	3442	3444	rBV3	1032	525	0.07%	0.008%
78	12.185	3463	3466	3468	rBV3	1091	781	0.10%	0.012%
79	12.201	3468	3471	3473	rBV3	1369	926	0.12%	0.014%
80	12.242	3482	3484	3486	rBV3	1053	733	0.10%	0.011%
81	12.365	3520	3522	3524	rBV3	962	581	0.08%	0.009%
82	12.403	3531	3534	3537	rBV5	1540	1266	0.17%	0.020%
83	12.509	3564	3567	3569	rBV3	1050	581	0.08%	0.009%
84	12.648	3609	3610	3612	rBV2	1153	551	0.07%	0.009%
85	12.680	3618	3620	3622	rBV3	1510	751	0.10%	0.012%
86	12.738	3636	3638	3641	rBV4	1289	724	0.10%	0.011%
87	12.763	3644	3646	3648	rBV3	1092	511	0.07%	0.008%
88	12.799	3653	3657	3658	rBV3	1070	639	0.08%	0.010%
89	12.892	3680	3686	3690	rBV9	2101	2613	0.34%	0.041%
90	12.972	3708	3711	3713	rBV4	1346	830	0.11%	0.013%
91	13.082	3743	3745	3748	rVB3	1134	617	0.08%	0.010%
92	13.101	3749	3751	3754	rBV4	1329	877	0.12%	0.014%
93	13.258	3797	3800	3801	rBV3	1829	972	0.13%	0.015%
94	13.310	3813	3816	3818	rBV3	1387	784	0.10%	0.012%
95	13.574	3897	3898	3902	rBV4	1486	1153	0.15%	0.018%
96	13.767	3956	3958	3962	rVB4	1850	697	0.09%	0.011%
97	13.783	3962	3963	3967	rVV3	1213	743	0.10%	0.012%
98	13.808	3969	3971	3975	rVB4	1210	898	0.12%	0.014%
99	13.914	4000	4004	4006	rBV5	1665	1058	0.14%	0.017%
100	15.371	4455	4457	4461	rBV5	1593	1288	0.17%	0.020%




Sum of corrected areas: 6390750

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030724.D
Acq On : 20 Apr 2023 18:09
Operator : SY/MD
Sample : 02411-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

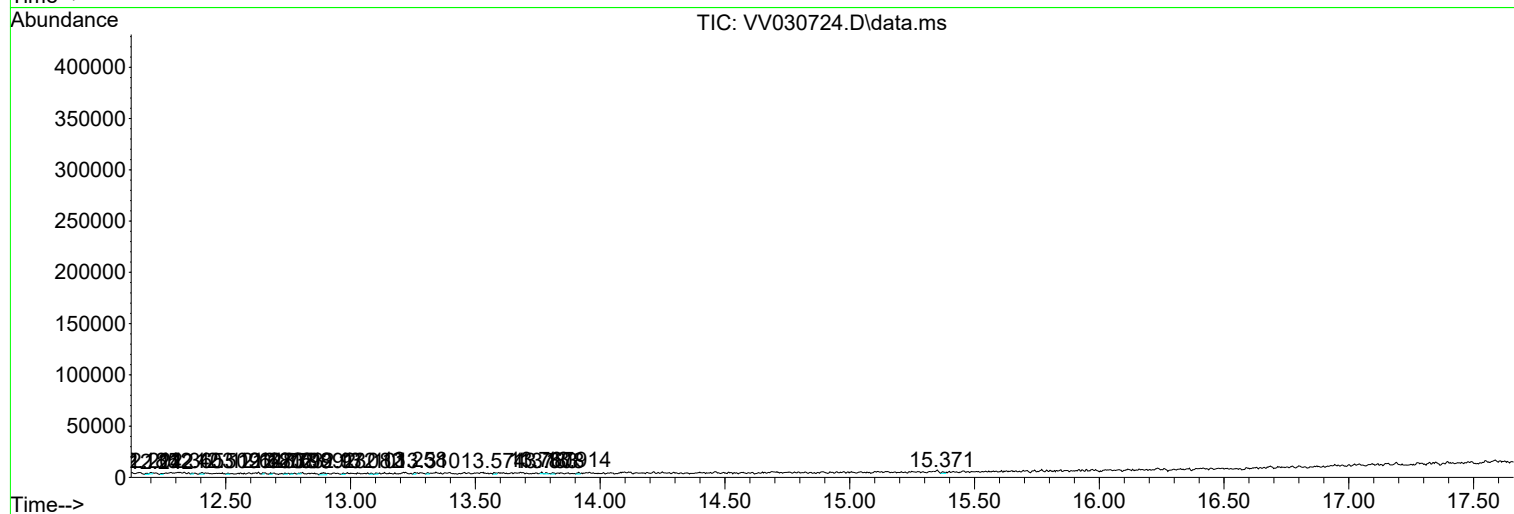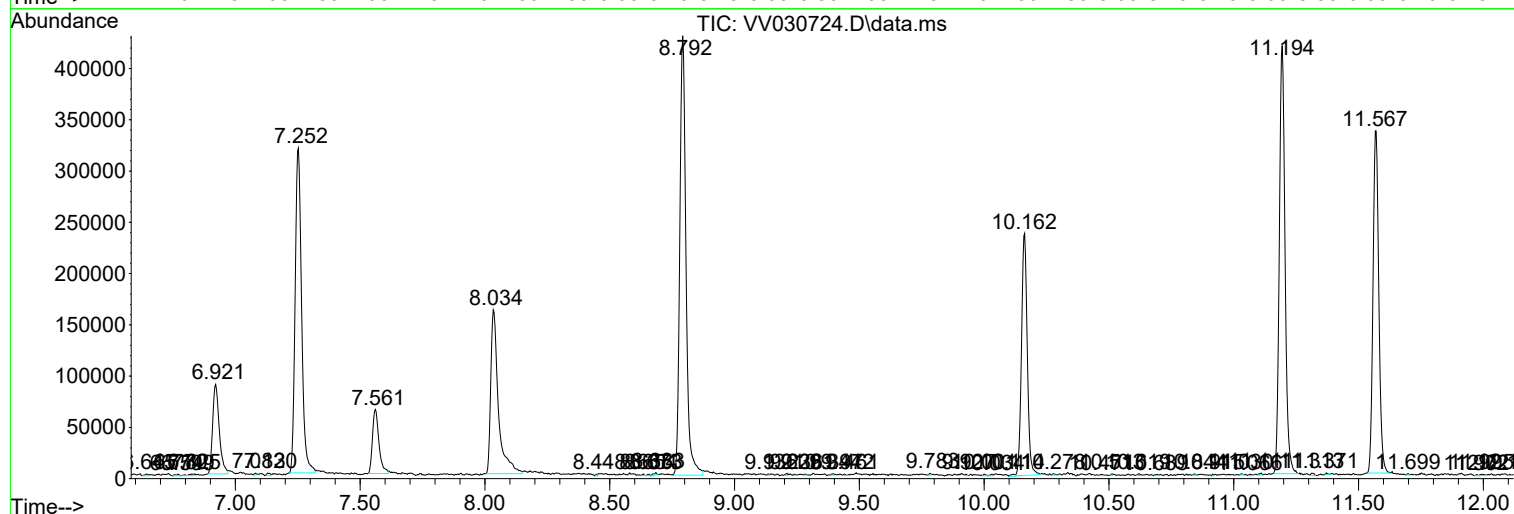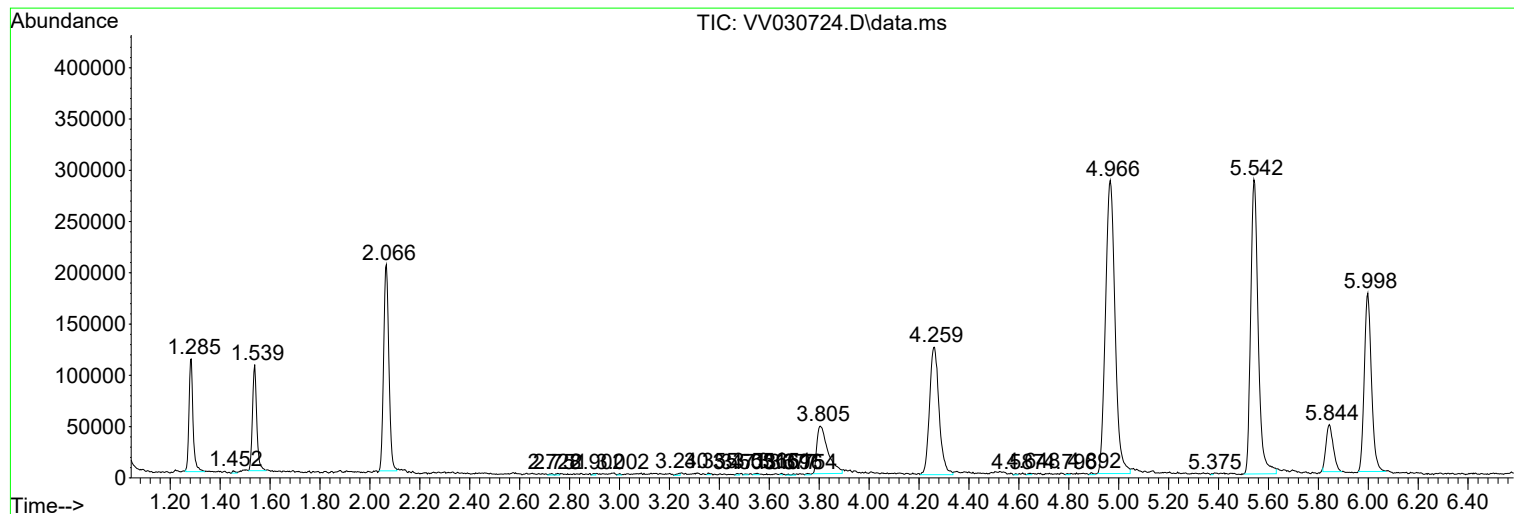

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030724.D
Acq On : 20 Apr 2023 18:09
Operator : SY/MD
Sample : 02411-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030724.D
Acq On : 20 Apr 2023 18:09
Operator : SY/MD
Sample : 02411-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------