

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030725.D
 Acq On : 20 Apr 2023 18:33
 Operator : SY/MD
 Sample : 02411-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	89	rBV	107348	118448	15.40%	1.884%
2	1.539	148	155	168	rVB	103175	118901	15.46%	1.892%
3	2.066	310	319	334	rBV	201936	288920	37.56%	4.596%
4	2.236	368	372	375	rBV6	2020	2114	0.27%	0.034%
5	2.381	415	417	420	rVB4	1828	791	0.10%	0.013%
6	2.400	420	423	427	rBV4	1261	937	0.12%	0.015%
7	2.423	427	430	432	rBV3	1967	1094	0.14%	0.017%
8	2.613	486	489	491	rBV3	1061	563	0.07%	0.009%
9	2.661	502	504	508	rVV4	1247	960	0.12%	0.015%
10	2.921	582	585	589	rVB6	1784	1274	0.17%	0.020%
11	2.941	589	591	593	rVB3	1125	583	0.08%	0.009%
12	2.973	595	601	604	rBV6	1620	1648	0.21%	0.026%
13	3.076	631	633	635	rVB3	1564	673	0.09%	0.011%
14	3.092	635	638	641	rBV4	1682	1031	0.13%	0.016%
15	3.140	650	653	654	rBV3	1191	727	0.09%	0.012%
16	3.172	659	663	665	rVB7	1484	1073	0.14%	0.017%
17	3.288	695	699	700	rBV5	1288	849	0.11%	0.014%
18	3.323	707	710	712	rBV4	1118	676	0.09%	0.011%
19	3.432	741	744	745	rBV3	1726	1130	0.15%	0.018%
20	3.442	745	747	750	rVV3	1617	885	0.12%	0.014%
21	3.455	750	751	755	rVB4	1126	553	0.07%	0.009%
22	3.490	760	762	766	rVV4	1535	1091	0.14%	0.017%
23	3.574	785	788	789	rBV2	1187	660	0.09%	0.010%
24	3.686	821	823	825	rBV3	1479	730	0.09%	0.012%
25	3.809	848	861	883	rBV2	46055	139365	18.12%	2.217%
26	4.259	988	1001	1025	rVB	123636	305154	39.67%	4.855%
27	4.677	1129	1131	1133	rBV3	923	547	0.07%	0.009%
28	4.767	1156	1159	1160	rBV3	1721	1051	0.14%	0.017%
29	4.902	1198	1201	1202	rBV4	1391	647	0.08%	0.010%
30	4.966	1205	1221	1250	rVV2	290405	769302	100.00%	12.238%
31	5.288	1315	1321	1324	rBV8	1773	2100	0.27%	0.033%
32	5.423	1359	1363	1365	rBV4	1041	665	0.09%	0.011%
33	5.542	1387	1400	1426	rBV	285412	603467	78.44%	9.600%
34	5.895	1509	1510	1512	rBV2	1163	571	0.07%	0.009%
35	5.998	1530	1542	1563	rBV	167138	343186	44.61%	5.460%
36	6.419	1671	1673	1675	rBV3	1836	781	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030725.D
 Acq On : 20 Apr 2023 18:33
 Operator : SY/MD
 Sample : 02411-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.490	1690	1695	1697	rBV6	1792	1139	0.15%	0.018%
38	6.561	1716	1717	1720	rBV3	1342	685	0.09%	0.011%
39	6.815	1793	1796	1798	rBV3	1158	708	0.09%	0.011%
40	6.921	1818	1829	1847	rVV	86602	164270	21.35%	2.613%
41	7.127	1887	1893	1895	rBV6	1595	1924	0.25%	0.031%
42	7.252	1920	1932	1955	rBV	319278	579421	75.32%	9.218%
43	7.561	2019	2028	2045	rBV	60334	113461	14.75%	1.805%
44	7.841	2113	2115	2119	rBV4	1206	689	0.09%	0.011%
45	8.034	2159	2175	2205	rBV	157870	338612	44.02%	5.387%
46	8.632	2358	2361	2362	rBV2	1687	884	0.11%	0.014%
47	8.792	2398	2411	2437	rBV	437761	747777	97.20%	11.896%
48	9.066	2493	2496	2499	rBV5	909	845	0.11%	0.013%
49	9.281	2560	2563	2564	rBV3	1267	560	0.07%	0.009%
50	9.326	2573	2577	2580	rBV5	1480	1595	0.21%	0.025%
51	9.384	2592	2595	2596	rBV2	2151	892	0.12%	0.014%
52	9.435	2608	2611	2614	rBV5	1729	1291	0.17%	0.021%
53	9.452	2614	2616	2617	rBV2	1143	572	0.07%	0.009%
54	9.619	2664	2668	2670	rBV5	1445	1334	0.17%	0.021%
55	9.760	2709	2712	2715	rBV3	1826	1262	0.16%	0.020%
56	9.866	2743	2745	2748	rBV3	1203	920	0.12%	0.015%
57	9.943	2765	2769	2771	rBV5	1224	691	0.09%	0.011%
58	9.960	2771	2774	2776	rVV3	1422	705	0.09%	0.011%
59	10.088	2813	2814	2817	rBV3	982	595	0.08%	0.009%
60	10.159	2823	2836	2856	rVV	229710	372215	48.38%	5.921%
61	10.333	2888	2890	2893	rVB3	1329	805	0.10%	0.013%
62	10.432	2917	2921	2926	rVB7	1646	1409	0.18%	0.022%
63	10.519	2945	2948	2949	rBV3	1333	736	0.10%	0.012%
64	10.558	2958	2960	2963	rBV5	1267	830	0.11%	0.013%
65	10.632	2978	2983	2986	rBV6	2058	2211	0.29%	0.035%
66	10.664	2991	2993	2997	rVV5	1084	794	0.10%	0.013%
67	10.683	2997	2999	3004	rVB5	1604	860	0.11%	0.014%
68	10.728	3009	3013	3015	rVB3	1320	819	0.11%	0.013%
69	10.744	3015	3018	3019	rBV3	1514	754	0.10%	0.012%
70	10.889	3060	3063	3065	rBV4	1143	818	0.11%	0.013%
71	10.927	3073	3075	3079	rBV5	1271	578	0.08%	0.009%
72	10.959	3083	3085	3088	rBV3	1060	633	0.08%	0.010%
73	10.988	3092	3094	3098	rVB5	1255	656	0.09%	0.010%
74	11.046	3109	3112	3114	rBV4	853	701	0.09%	0.011%
75	11.194	3146	3158	3180	rBV	409331	665442	86.50%	10.586%
76	11.487	3246	3249	3251	rBV3	1127	754	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030725.D
 Acq On : 20 Apr 2023 18:33
 Operator : SY/MD
 Sample : 02411-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.567	3263	3274	3293	rBV	327401	530463	68.95%	8.439%
78	11.725	3320	3323	3329	rVB6	1513	1142	0.15%	0.018%
79	11.963	3394	3397	3399	rBV4	1041	622	0.08%	0.010%
80	12.297	3491	3501	3510	rBV4	5968	11804	1.53%	0.188%
81	12.580	3587	3589	3590	rBV2	1176	543	0.07%	0.009%
82	12.664	3612	3615	3618	rBV4	1761	903	0.12%	0.014%
83	12.766	3643	3647	3650	rBV5	1172	989	0.13%	0.016%
84	12.802	3657	3658	3664	rVB5	1646	1034	0.13%	0.016%
85	12.857	3672	3675	3677	rBV3	1204	811	0.11%	0.013%
86	13.056	3735	3737	3741	rVB5	1380	778	0.10%	0.012%
87	13.085	3744	3746	3747	rVV2	1584	550	0.07%	0.009%
88	13.104	3750	3752	3754	rBV3	1356	644	0.08%	0.010%
89	13.127	3758	3759	3762	rBV3	1201	681	0.09%	0.011%
90	13.156	3765	3768	3774	rVB6	1232	990	0.13%	0.016%
91	13.307	3812	3815	3819	rVB6	1126	735	0.10%	0.012%
92	13.390	3839	3841	3846	rBV6	905	948	0.12%	0.015%
93	13.426	3850	3852	3853	rBV2	1335	553	0.07%	0.009%
94	13.509	3876	3878	3880	rBV3	1247	769	0.10%	0.012%
95	13.574	3895	3898	3902	rBV6	1342	1227	0.16%	0.020%
96	13.602	3905	3907	3909	rVB3	1654	718	0.09%	0.011%
97	13.676	3927	3930	3935	rVB7	1088	855	0.11%	0.014%
98	13.869	3988	3990	3993	rBV4	958	661	0.09%	0.011%
99	13.963	4017	4019	4022	rBV4	1248	884	0.11%	0.014%
100	14.059	4045	4049	4054	rVB8	1786	1686	0.22%	0.027%




Sum of corrected areas: 6285984

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030725.D
Acq On : 20 Apr 2023 18:33
Operator : SY/MD
Sample : 02411-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

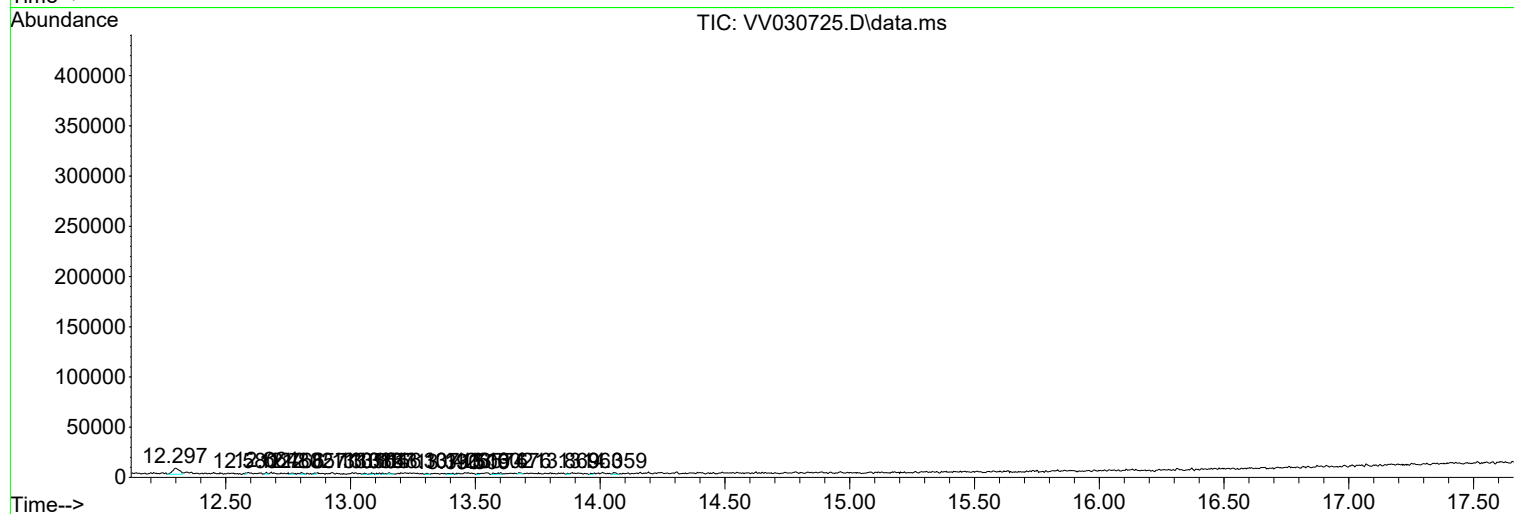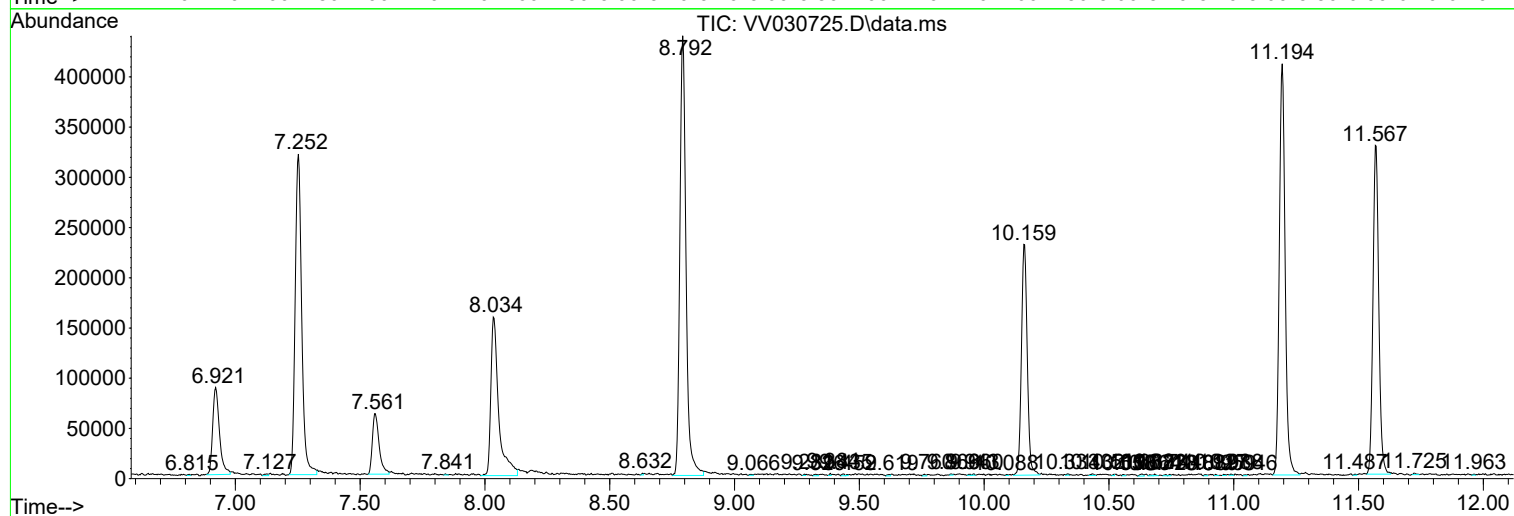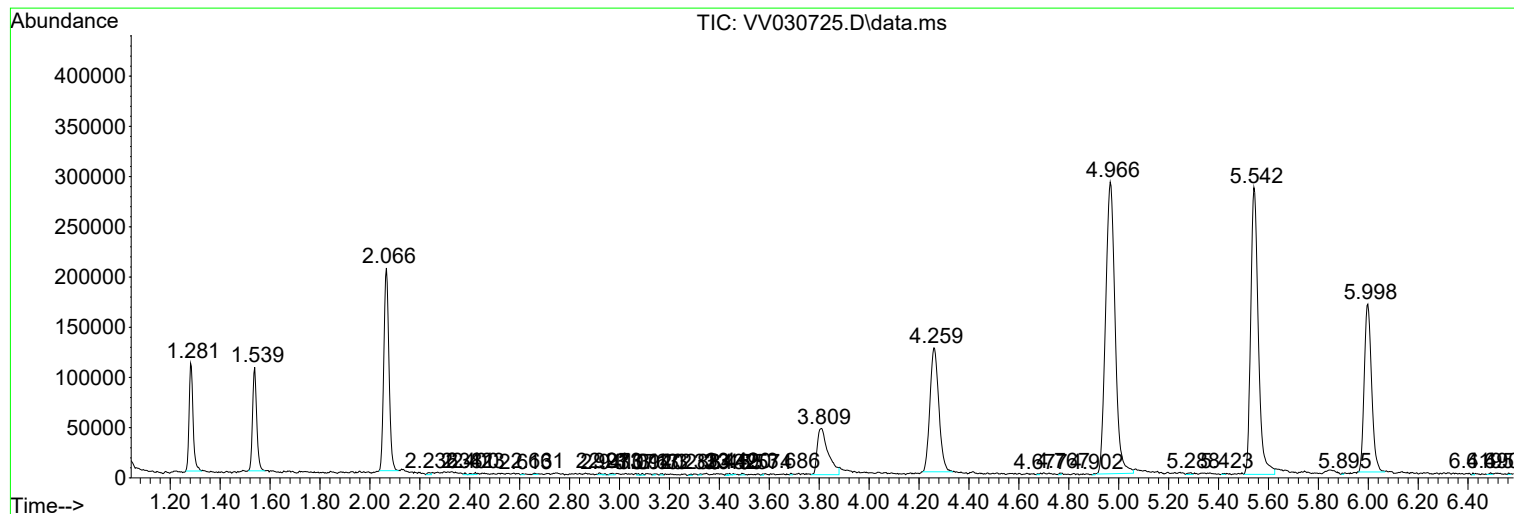

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030725.D
Acq On : 20 Apr 2023 18:33
Operator : SY/MD
Sample : 02411-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030725.D
Acq On : 20 Apr 2023 18:33
Operator : SY/MD
Sample : 02411-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------