

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030726.D
 Acq On : 20 Apr 2023 18:55
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rBV	104512	110254	14.53%	1.724%
2	1.539	148	155	167	rBV	101816	116305	15.32%	1.819%
3	2.066	309	319	335	rBV	197859	294425	38.79%	4.605%
4	2.520	457	460	462	rBV4	921	688	0.09%	0.011%
5	2.783	540	542	545	rBV4	1547	809	0.11%	0.013%
6	2.799	545	547	550	rVV3	1101	665	0.09%	0.010%
7	2.844	558	561	563	rBV4	1137	757	0.10%	0.012%
8	2.883	571	573	579	rVB7	1562	1389	0.18%	0.022%
9	2.909	579	581	582	rBV2	1128	533	0.07%	0.008%
10	2.986	603	605	608	rBV2	1593	1120	0.15%	0.018%
11	3.089	634	637	638	rBV3	1280	684	0.09%	0.011%
12	3.150	652	656	659	rBV5	1421	899	0.12%	0.014%
13	3.336	710	714	717	rVB6	1337	1007	0.13%	0.016%
14	3.413	733	738	741	rBV6	1482	1199	0.16%	0.019%
15	3.439	744	746	749	rVB4	1949	884	0.12%	0.014%
16	3.455	749	751	754	rBV4	1059	635	0.08%	0.010%
17	3.529	771	774	776	rBV3	1418	743	0.10%	0.012%
18	3.545	776	779	786	rVV8	1786	2061	0.27%	0.032%
19	3.754	842	844	848	rVB4	1572	923	0.12%	0.014%
20	3.809	851	861	889	rVV2	46642	145096	19.12%	2.269%
21	4.262	989	1002	1026	rVB	120269	305011	40.19%	4.770%
22	4.481	1065	1070	1071	rBV4	2902	2197	0.29%	0.034%
23	4.687	1131	1134	1138	rVB6	1461	1226	0.16%	0.019%
24	4.815	1172	1174	1176	rBV3	999	536	0.07%	0.008%
25	4.863	1188	1189	1192	rVB2	1714	649	0.09%	0.010%
26	4.966	1203	1221	1248	rBV3	281567	758960	100.00%	11.870%
27	5.404	1354	1357	1359	rBV4	1247	706	0.09%	0.011%
28	5.439	1365	1368	1369	rBV3	1284	760	0.10%	0.012%
29	5.542	1387	1400	1422	rBV	277534	579961	76.42%	9.070%
30	5.789	1475	1477	1478	rBV2	1806	706	0.09%	0.011%
31	5.844	1483	1494	1516	rVB2	122671	248373	32.73%	3.884%
32	5.998	1531	1542	1559	rVB2	163964	331359	43.66%	5.182%
33	6.667	1744	1750	1754	rBV8	1739	1934	0.25%	0.030%
34	6.802	1789	1792	1794	rBV4	1944	1095	0.14%	0.017%
35	6.921	1820	1829	1846	rVB2	83771	151012	19.90%	2.362%
36	7.252	1921	1932	1954	rBV	318134	566922	74.70%	8.866%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042023\
 Data File : VW030726.D
 Acq On : 20 Apr 2023 18:55
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.442	1989	1991	1995	rBV4	1327	741	0.10%	0.012%
38	7.513	2011	2013	2015	rBV3	1220	562	0.07%	0.009%
39	7.561	2019	2028	2046	rVV2	61951	115046	15.16%	1.799%
40	7.728	2078	2080	2081	rBV3	1743	780	0.10%	0.012%
41	8.037	2166	2176	2205	rBV	147313	314360	41.42%	4.916%
42	8.429	2296	2298	2303	rVB6	1765	1360	0.18%	0.021%
43	8.465	2303	2309	2312	rBV6	1583	1903	0.25%	0.030%
44	8.513	2322	2324	2331	rBV8	1056	1012	0.13%	0.016%
45	8.728	2389	2391	2394	rBV5	1582	883	0.12%	0.014%
46	8.793	2400	2411	2432	rBV	428857	715072	94.22%	11.183%
47	9.194	2533	2536	2539	rBV5	1914	1649	0.22%	0.026%
48	9.313	2571	2573	2577	rBV4	1565	883	0.12%	0.014%
49	9.349	2582	2584	2587	rVB4	1507	657	0.09%	0.010%
50	9.436	2609	2611	2614	rBV4	1073	652	0.09%	0.010%
51	9.535	2640	2642	2648	rBV7	1753	2175	0.29%	0.034%
52	9.683	2686	2688	2692	rBV4	1456	789	0.10%	0.012%
53	9.828	2731	2733	2737	rBV4	1482	1015	0.13%	0.016%
54	9.976	2777	2779	2781	rBV2	1022	562	0.07%	0.009%
55	10.162	2825	2837	2853	rBV	228073	363705	47.92%	5.688%
56	10.307	2879	2882	2884	rBV4	1325	937	0.12%	0.015%
57	10.432	2918	2921	2924	rBV5	1995	1593	0.21%	0.025%
58	10.558	2957	2960	2965	rBV7	1363	1001	0.13%	0.016%
59	10.580	2965	2967	2969	rBV2	919	537	0.07%	0.008%
60	10.667	2992	2994	2996	rBV3	1078	541	0.07%	0.008%
61	10.834	3043	3046	3048	rBV4	1403	991	0.13%	0.015%
62	10.876	3054	3059	3060	rBV4	1282	1045	0.14%	0.016%
63	10.953	3078	3083	3084	rBV5	724	550	0.07%	0.009%
64	10.992	3089	3095	3097	rVV5	1380	1109	0.15%	0.017%
65	11.001	3097	3098	3102	rVB4	1573	839	0.11%	0.013%
66	11.034	3104	3108	3112	rBV7	746	736	0.10%	0.012%
67	11.072	3117	3120	3122	rBV4	1245	881	0.12%	0.014%
68	11.108	3125	3131	3133	rBV6	1937	2030	0.27%	0.032%
69	11.194	3144	3158	3179	rBV	419434	668038	88.02%	10.448%
70	11.452	3236	3238	3241	rVV3	1382	642	0.08%	0.010%
71	11.474	3243	3245	3247	rBV3	1094	598	0.08%	0.009%
72	11.571	3264	3275	3292	rBV	321587	527795	69.54%	8.254%
73	11.683	3307	3310	3311	rBV3	1953	1101	0.15%	0.017%
74	11.731	3322	3325	3329	rBV6	1492	1085	0.14%	0.017%
75	11.992	3404	3406	3409	rBV4	1702	956	0.13%	0.015%
76	12.108	3439	3442	3444	rBV5	1865	918	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030726.D
 Acq On : 20 Apr 2023 18:55
 Operator : SY/MD
 Sample : 02411-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.416	3535	3538	3543	rBV7	1900	1676	0.22%	0.026%
78	12.464	3551	3553	3556	rVB3	1822	904	0.12%	0.014%
79	12.497	3561	3563	3567	rBV4	808	635	0.08%	0.010%
80	12.522	3570	3571	3574	rVB3	1518	738	0.10%	0.012%
81	12.542	3574	3577	3583	rBV7	2338	2049	0.27%	0.032%
82	12.571	3583	3586	3588	rBV3	1203	711	0.09%	0.011%
83	12.792	3653	3655	3656	rBV2	1629	564	0.07%	0.009%
84	12.972	3705	3711	3714	rBV7	1442	1424	0.19%	0.022%
85	13.014	3720	3724	3725	rBV4	1451	1007	0.13%	0.016%
86	13.056	3731	3737	3738	rBV6	1424	1115	0.15%	0.017%
87	13.191	3776	3779	3783	rBV6	1811	1869	0.25%	0.029%
88	13.236	3789	3793	3797	rBV6	1244	1020	0.13%	0.016%
89	13.262	3799	3801	3804	rVB4	1554	672	0.09%	0.011%
90	13.291	3804	3810	3811	rBV4	925	916	0.12%	0.014%
91	13.355	3826	3830	3831	rBV2	992	730	0.10%	0.011%
92	13.683	3930	3932	3935	rVV4	1387	754	0.10%	0.012%
93	13.754	3952	3954	3956	rBV2	1302	663	0.09%	0.010%
94	13.825	3974	3976	3980	rVB5	1176	582	0.08%	0.009%
95	13.844	3980	3982	3984	rBV2	1291	723	0.10%	0.011%
96	13.989	4025	4027	4029	rBV3	1248	690	0.09%	0.011%
97	14.136	4071	4073	4075	rBV3	1332	643	0.08%	0.010%
98	14.268	4112	4114	4117	rBV4	1314	663	0.09%	0.010%
99	14.397	4152	4154	4156	rBV3	2256	1459	0.19%	0.023%
100	14.754	4260	4265	4266	rBV5	2163	1739	0.23%	0.027%




Sum of corrected areas: 6394158

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030726.D
Acq On : 20 Apr 2023 18:55
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

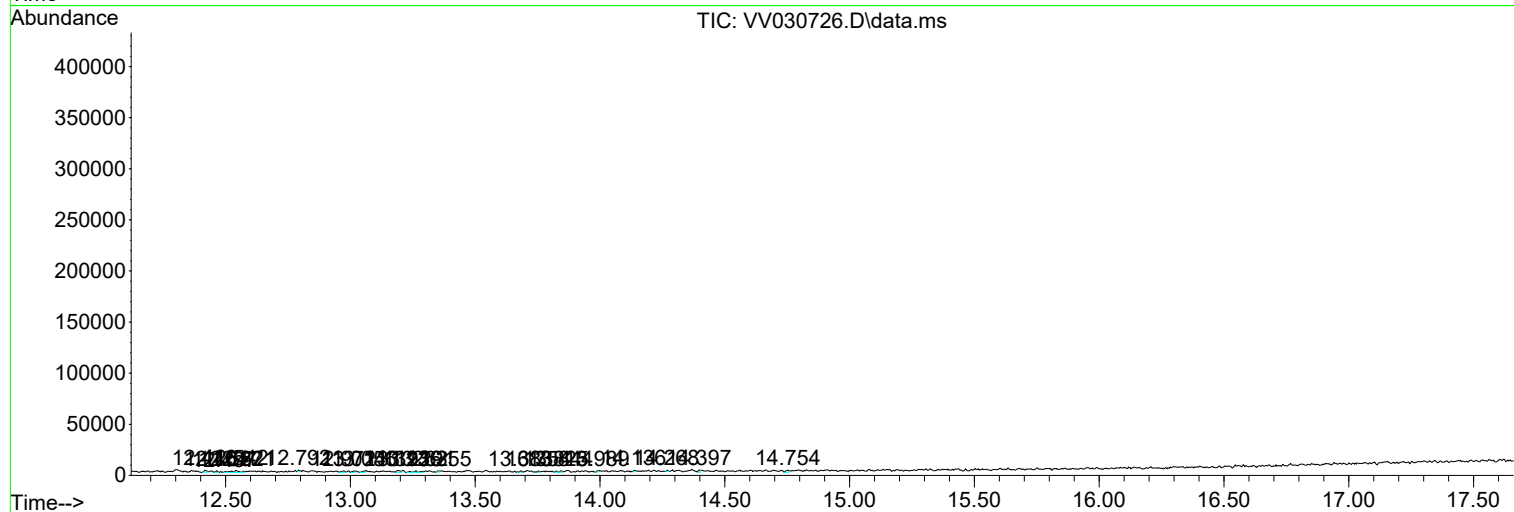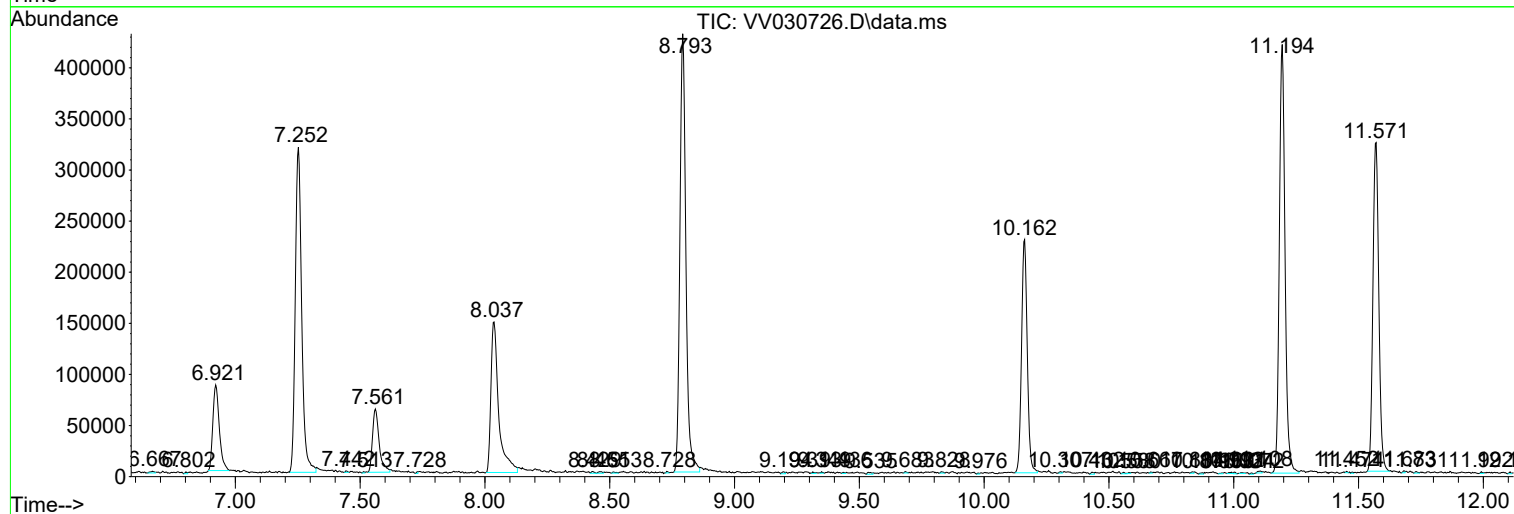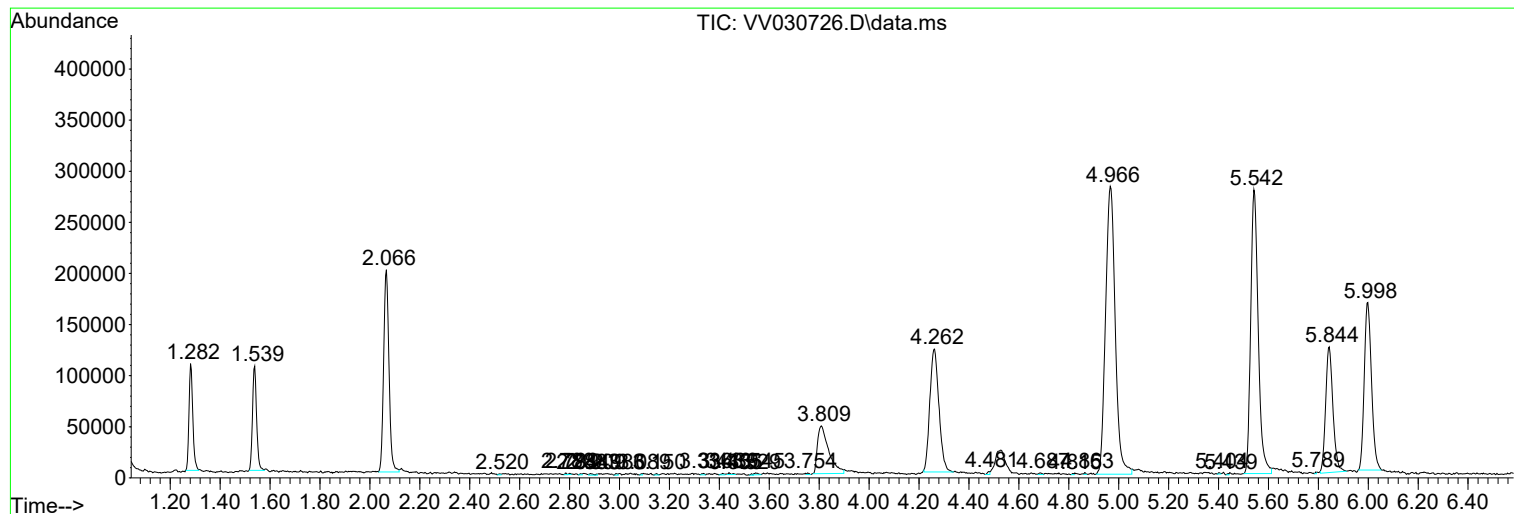

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030726.D
Acq On : 20 Apr 2023 18:55
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030726.D
Acq On : 20 Apr 2023 18:55
Operator : SY/MD
Sample : 02411-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc