

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030727.D
 Acq On : 20 Apr 2023 19:19
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rBV	103412	112304	15.07%	1.635%
2	1.539	148	155	170	rVB	99700	118305	15.88%	1.722%
3	2.066	310	319	333	rBV	197230	286343	38.44%	4.169%
4	2.413	425	427	431	rBV6	985	578	0.08%	0.008%
5	2.516	455	459	462	rBV5	1451	1206	0.16%	0.018%
6	2.597	482	484	487	rVB3	1207	444	0.06%	0.006%
7	2.899	576	578	581	rBV4	1138	552	0.07%	0.008%
8	2.954	593	595	597	rBV3	1149	737	0.10%	0.011%
9	3.015	611	614	618	rVB5	1457	984	0.13%	0.014%
10	3.047	620	624	627	rVB7	1277	926	0.12%	0.013%
11	3.069	627	631	632	rBV3	850	484	0.06%	0.007%
12	3.082	633	635	637	rBV2	1159	488	0.07%	0.007%
13	3.114	640	645	648	rBV7	1758	2057	0.28%	0.030%
14	3.182	665	666	669	rBV3	774	479	0.06%	0.007%
15	3.310	704	706	707	rBV2	1262	682	0.09%	0.010%
16	3.346	714	717	718	rBV3	819	492	0.07%	0.007%
17	3.355	718	720	722	rVB3	1323	587	0.08%	0.009%
18	3.404	734	735	738	rVB3	1139	600	0.08%	0.009%
19	3.423	738	741	742	rBV2	1056	649	0.09%	0.009%
20	3.433	742	744	747	rVV4	1364	824	0.11%	0.012%
21	3.462	751	753	754	rBV2	984	482	0.06%	0.007%
22	3.513	767	769	773	rVB5	1034	761	0.10%	0.011%
23	3.654	811	813	817	rBV5	1007	646	0.09%	0.009%
24	3.683	819	822	827	rVB6	1209	1104	0.15%	0.016%
25	3.719	830	833	836	rBV4	1947	1229	0.16%	0.018%
26	3.815	850	863	888	rBV4	54641	186777	25.07%	2.719%
27	4.163	969	971	974	rVB4	1175	661	0.09%	0.010%
28	4.262	982	1002	1029	rBV4	130005	403448	54.15%	5.874%
29	4.693	1133	1136	1140	rBV6	1177	785	0.11%	0.011%
30	4.799	1167	1169	1171	rBV3	1028	500	0.07%	0.007%
31	4.835	1179	1180	1184	rBV4	891	495	0.07%	0.007%
32	4.902	1196	1201	1202	rBV4	712	597	0.08%	0.009%
33	4.966	1202	1221	1245	rBV2	280575	745000	100.00%	10.846%
34	5.304	1322	1326	1329	rVB6	1292	937	0.13%	0.014%
35	5.471	1374	1378	1381	rBV6	1444	1380	0.19%	0.020%
36	5.542	1384	1400	1425	rBV	270864	572717	76.87%	8.338%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030727.D
 Acq On : 20 Apr 2023 19:19
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.841	1481	1493	1517	rBV	352298	701805	94.20%	10.217%
38	5.998	1531	1542	1559	rVB	162445	325785	43.73%	4.743%
39	6.301	1633	1636	1637	rBV3	1323	810	0.11%	0.012%
40	6.394	1663	1665	1666	rBV2	1837	821	0.11%	0.012%
41	6.423	1672	1674	1675	rBV2	1534	811	0.11%	0.012%
42	6.580	1720	1723	1725	rBV4	1681	1070	0.14%	0.016%
43	6.921	1818	1829	1849	rBV	84981	162851	21.86%	2.371%
44	7.111	1886	1888	1890	rBV3	1346	786	0.11%	0.011%
45	7.156	1900	1902	1903	rBV2	1094	520	0.07%	0.008%
46	7.182	1908	1910	1912	rVV3	1588	746	0.10%	0.011%
47	7.252	1921	1932	1951	rBV	305749	547813	73.53%	7.976%
48	7.561	2019	2028	2047	rBV	60712	108695	14.59%	1.582%
49	7.889	2127	2130	2132	rBV3	1662	846	0.11%	0.012%
50	7.950	2144	2149	2151	rBV6	2461	2118	0.28%	0.031%
51	7.989	2159	2161	2163	rBV2	1493	757	0.10%	0.011%
52	8.034	2166	2175	2209	rBV	138089	301049	40.41%	4.383%
53	8.490	2314	2317	2322	rVB7	1563	1181	0.16%	0.017%
54	8.510	2322	2323	2327	rBV4	1435	738	0.10%	0.011%
55	8.564	2337	2340	2343	rBV5	1598	1139	0.15%	0.017%
56	8.793	2400	2411	2434	rBV	409839	695653	93.38%	10.128%
57	9.188	2532	2534	2536	rVB3	1178	504	0.07%	0.007%
58	9.387	2593	2596	2597	rBV3	1032	531	0.07%	0.008%
59	9.558	2647	2649	2653	rVB6	895	564	0.08%	0.008%
60	9.580	2653	2656	2657	rBV3	1516	764	0.10%	0.011%
61	9.590	2657	2659	2663	rBV4	1250	785	0.11%	0.011%
62	9.902	2754	2756	2759	rVB3	1577	832	0.11%	0.012%
63	9.918	2759	2761	2762	rBV2	1772	755	0.10%	0.011%
64	9.960	2770	2774	2776	rVB6	952	753	0.10%	0.011%
65	9.979	2777	2780	2783	rBV4	1380	967	0.13%	0.014%
66	10.162	2826	2837	2852	rBV	216146	352958	47.38%	5.139%
67	10.317	2883	2885	2887	rVV2	1540	789	0.11%	0.011%
68	10.381	2902	2905	2906	rBV3	2177	903	0.12%	0.013%
69	10.603	2973	2974	2978	rBV3	840	551	0.07%	0.008%
70	10.670	2989	2995	2997	rBV6	2440	2561	0.34%	0.037%
71	10.725	3011	3012	3015	rVB2	1205	472	0.06%	0.007%
72	10.738	3015	3016	3021	rVB5	1529	961	0.13%	0.014%
73	10.786	3027	3031	3033	rBV4	1301	933	0.13%	0.014%
74	10.825	3041	3043	3046	rVB3	1663	643	0.09%	0.009%
75	10.841	3046	3048	3051	rBV4	1510	908	0.12%	0.013%
76	11.066	3116	3118	3120	rBV3	1053	583	0.08%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030727.D
 Acq On : 20 Apr 2023 19:19
 Operator : SY/MD
 Sample : 02411-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.194	3146	3158	3177	rBV	399590	641057	86.05%	9.333%
78	11.571	3264	3275	3291	rVB	329481	532566	71.49%	7.754%
79	12.063	3425	3428	3429	rBV3	1663	980	0.13%	0.014%
80	12.574	3585	3587	3591	rBV5	1426	1029	0.14%	0.015%
81	12.744	3636	3640	3646	rBV7	2096	1832	0.25%	0.027%
82	12.940	3698	3701	3704	rBV4	2295	1888	0.25%	0.027%
83	13.059	3736	3738	3740	rBV3	1074	639	0.09%	0.009%
84	13.146	3763	3765	3766	rBV2	1003	464	0.06%	0.007%
85	13.349	3826	3828	3831	rBV4	998	565	0.08%	0.008%
86	13.464	3862	3864	3866	rVB3	1539	643	0.09%	0.009%
87	13.567	3894	3896	3899	rBV4	1184	872	0.12%	0.013%
88	13.612	3908	3910	3913	rBV4	1061	533	0.07%	0.008%
89	13.844	3980	3982	3983	rBV2	1115	532	0.07%	0.008%
90	13.873	3988	3991	3994	rBV5	1138	675	0.09%	0.010%
91	13.889	3994	3996	3998	rBV2	1698	1012	0.14%	0.015%
92	13.940	4010	4012	4015	rBV4	1940	1358	0.18%	0.020%
93	13.998	4026	4030	4038	rVB9	1651	2028	0.27%	0.030%
94	14.033	4038	4041	4043	rBV4	1508	811	0.11%	0.012%
95	14.095	4058	4060	4062	rBV3	1216	587	0.08%	0.009%
96	14.516	4187	4191	4193	rBV4	1803	1444	0.19%	0.021%
97	14.879	4297	4304	4307	rBV8	1891	2268	0.30%	0.033%
98	14.902	4307	4311	4317	rVB7	1688	1191	0.16%	0.017%
99	14.927	4317	4319	4321	rBV4	1468	900	0.12%	0.013%
100	15.291	4430	4432	4434	rBV3	1766	867	0.12%	0.013%




Sum of corrected areas: 6868692

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030727.D
Acq On : 20 Apr 2023 19:19
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

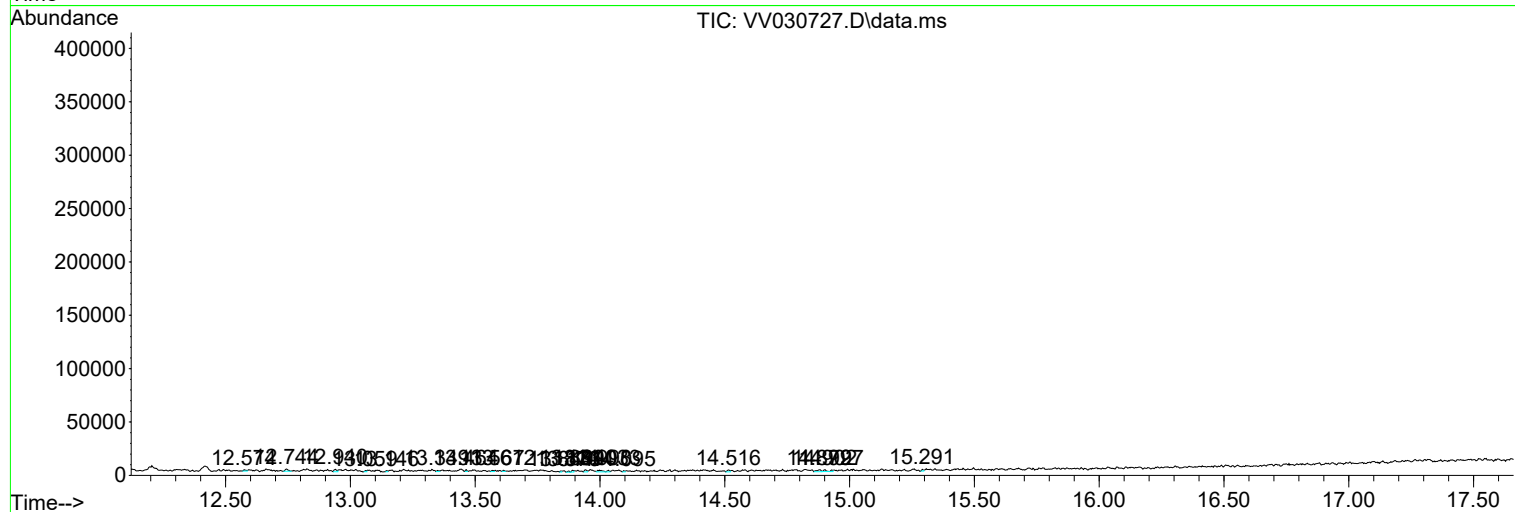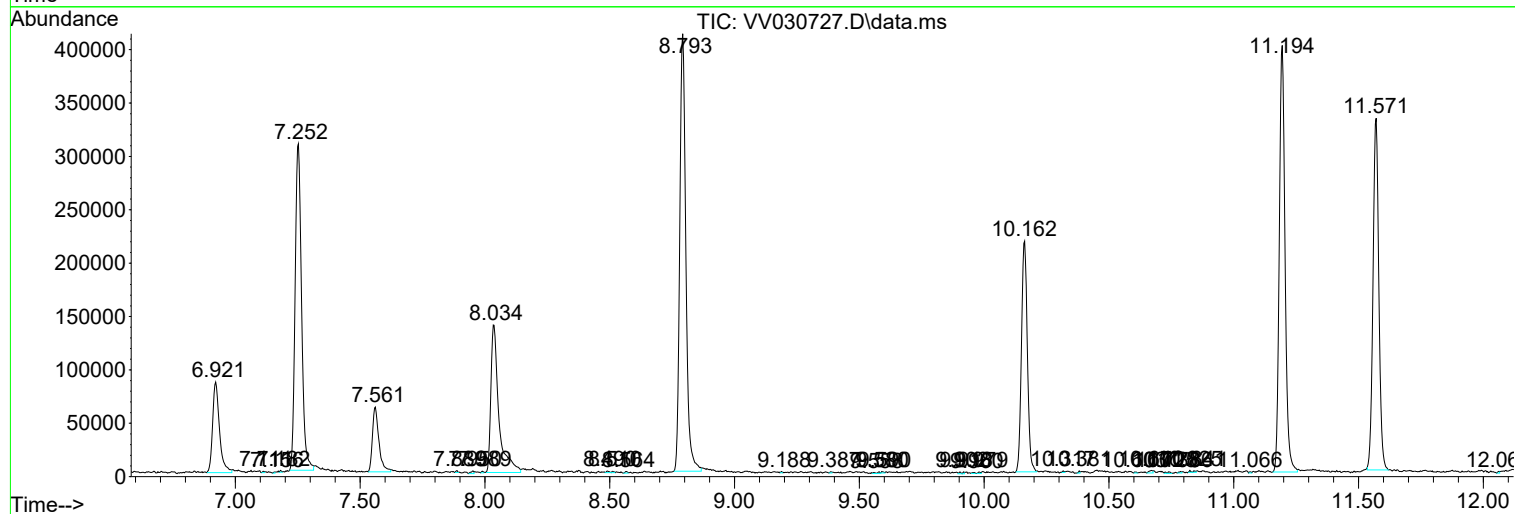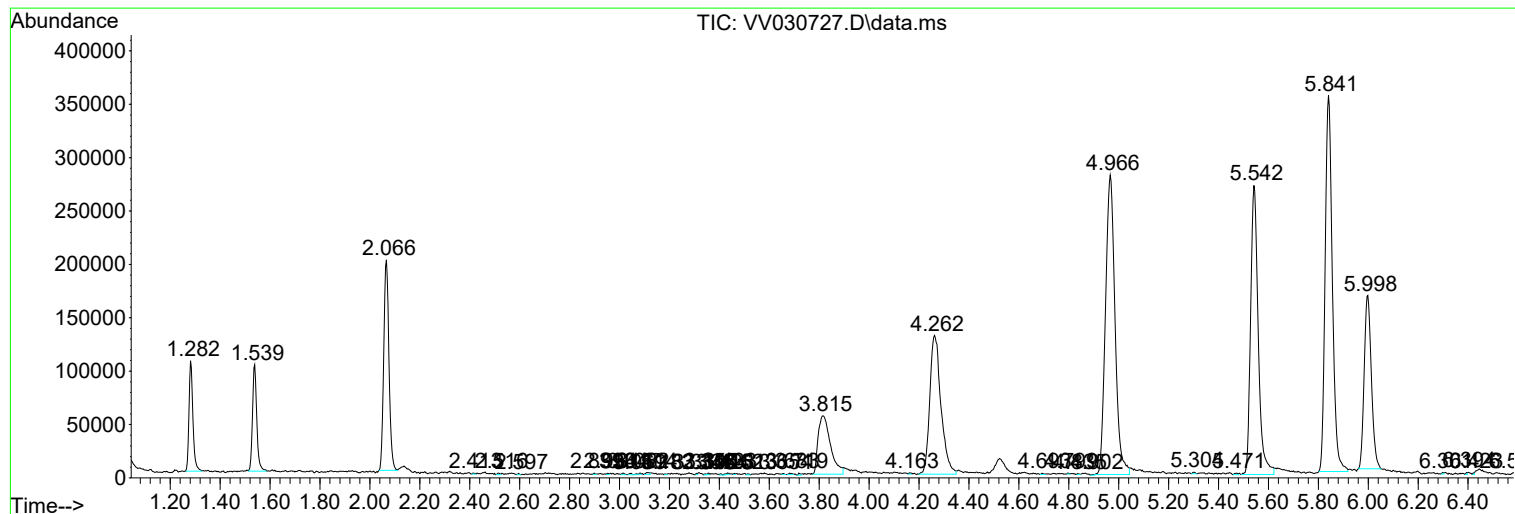

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030727.D
Acq On : 20 Apr 2023 19:19
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030727.D
Acq On : 20 Apr 2023 19:19
Operator : SY/MD
Sample : 02411-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc