

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030729.D
 Acq On : 20 Apr 2023 20:06
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rBV	112567	122182	15.31%	2.014%
2	1.539	148	155	167	rVB	107908	126364	15.84%	2.083%
3	2.066	310	319	332	rBV	207547	303487	38.03%	5.004%
4	2.500	450	454	455	rVB3	1340	736	0.09%	0.012%
5	2.625	492	493	496	rVB3	1495	633	0.08%	0.010%
6	2.645	496	499	507	rVB8	1837	1665	0.21%	0.027%
7	2.683	507	511	517	rBV8	2026	2097	0.26%	0.035%
8	2.712	517	520	522	rBV4	2016	1271	0.16%	0.021%
9	2.857	561	565	567	rBV5	1304	1005	0.13%	0.017%
10	3.066	628	630	633	rBV3	1324	861	0.11%	0.014%
11	3.153	654	657	660	rBV5	957	797	0.10%	0.013%
12	3.195	666	670	675	rVB7	2005	1833	0.23%	0.030%
13	3.220	675	678	680	rBV4	1486	953	0.12%	0.016%
14	3.288	695	699	701	rBV4	954	635	0.08%	0.010%
15	3.400	732	734	736	rBV4	1901	723	0.09%	0.012%
16	3.442	744	747	750	rBV5	1512	1102	0.14%	0.018%
17	3.622	800	803	807	rBV6	1405	1395	0.17%	0.023%
18	3.722	830	834	835	rBV3	2052	1361	0.17%	0.022%
19	3.805	851	860	888	rBV2	46827	143665	18.00%	2.369%
20	4.259	984	1001	1024	rBV	128700	333206	41.76%	5.494%
21	4.555	1090	1093	1097	rBV5	1805	1415	0.18%	0.023%
22	4.844	1179	1183	1185	rBV5	1339	1126	0.14%	0.019%
23	4.966	1204	1221	1249	rBV2	296729	797998	100.00%	13.157%
24	5.410	1357	1359	1362	rBV3	1435	828	0.10%	0.014%
25	5.455	1371	1373	1375	rBV3	1109	620	0.08%	0.010%
26	5.542	1388	1400	1423	rBV	231666	480657	60.23%	7.925%
27	5.998	1527	1542	1563	rBV	175013	374814	46.97%	6.180%
28	6.268	1623	1626	1627	rBV3	1904	910	0.11%	0.015%
29	6.278	1627	1629	1632	rVB5	2620	1226	0.15%	0.020%
30	6.339	1646	1648	1650	rBV2	1381	754	0.09%	0.012%
31	6.371	1653	1658	1660	rBV4	1346	1501	0.19%	0.025%
32	6.474	1686	1690	1694	rBV6	2002	1996	0.25%	0.033%
33	6.571	1718	1720	1724	rBV4	1542	826	0.10%	0.014%
34	6.921	1820	1829	1848	rBV	85199	159432	19.98%	2.629%
35	7.207	1913	1918	1919	rBV5	1924	1814	0.23%	0.030%
36	7.252	1921	1932	1950	rVV	333208	590131	73.95%	9.730%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030729.D
 Acq On : 20 Apr 2023 20:06
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.561	2020	2028	2046	rBV	61694	108431	13.59%	1.788%
38	7.853	2116	2119	2121	rBV4	1289	769	0.10%	0.013%
39	7.998	2161	2164	2165	rBV3	1395	849	0.11%	0.014%
40	8.037	2166	2176	2191	rBV	157037	301761	37.81%	4.975%
41	8.349	2271	2273	2275	rBV3	1717	931	0.12%	0.015%
42	8.519	2323	2326	2328	rBV4	1219	836	0.10%	0.014%
43	8.593	2346	2349	2356	rBV8	2253	2697	0.34%	0.044%
44	8.792	2398	2411	2438	rBV	356928	610729	76.53%	10.069%
45	9.011	2478	2479	2483	rVB4	2338	1130	0.14%	0.019%
46	9.152	2522	2523	2525	rBV2	1385	700	0.09%	0.012%
47	9.178	2529	2531	2534	rBV4	1325	841	0.11%	0.014%
48	9.268	2556	2559	2561	rBV4	1155	723	0.09%	0.012%
49	9.333	2576	2579	2581	rBV4	1707	1160	0.15%	0.019%
50	9.458	2616	2618	2620	rBV3	988	636	0.08%	0.010%
51	9.622	2664	2669	2671	rBV6	1384	948	0.12%	0.016%
52	9.648	2674	2677	2679	rBV4	1559	953	0.12%	0.016%
53	9.728	2700	2702	2706	rBV4	1405	668	0.08%	0.011%
54	9.779	2713	2718	2721	rBV7	1744	1513	0.19%	0.025%
55	9.943	2766	2769	2771	rVB3	2064	1061	0.13%	0.017%
56	10.162	2824	2837	2860	rVV	236969	393231	49.28%	6.483%
57	10.406	2911	2913	2916	rVB4	1895	939	0.12%	0.015%
58	10.429	2916	2920	2924	rVB6	2224	1803	0.23%	0.030%
59	10.461	2924	2930	2932	rBV7	1701	1661	0.21%	0.027%
60	10.612	2974	2977	2978	rBV2	1533	628	0.08%	0.010%
61	10.667	2990	2994	2995	rBV4	1114	745	0.09%	0.012%
62	10.734	3012	3015	3018	rVB5	1634	986	0.12%	0.016%
63	10.841	3046	3048	3051	rBV3	1800	913	0.11%	0.015%
64	10.863	3051	3055	3059	rVV6	1902	1852	0.23%	0.031%
65	10.892	3062	3064	3068	rVV5	1205	900	0.11%	0.015%
66	10.972	3087	3089	3092	rBV4	1225	847	0.11%	0.014%
67	11.011	3097	3101	3104	rBV6	1053	1184	0.15%	0.020%
68	11.130	3133	3138	3139	rBV5	2021	1428	0.18%	0.024%
69	11.194	3146	3158	3175	rBV	347127	562436	70.48%	9.273%
70	11.361	3208	3210	3212	rBV3	1309	702	0.09%	0.012%
71	11.397	3218	3221	3224	rBV5	1583	1090	0.14%	0.018%
72	11.461	3239	3241	3243	rBV3	1467	835	0.10%	0.014%
73	11.570	3262	3275	3291	rBV	343836	563208	70.58%	9.286%
74	11.857	3360	3364	3368	rBV7	1433	1311	0.16%	0.022%
75	12.046	3421	3423	3426	rVB4	1366	677	0.08%	0.011%
76	12.091	3434	3437	3438	rBV3	1146	642	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030729.D
 Acq On : 20 Apr 2023 20:06
 Operator : SY/MD
 Sample : 02334-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.278	3491	3495	3498	rVB6	1438	1079	0.14%	0.018%
78	12.567	3581	3585	3587	rBV4	1095	763	0.10%	0.013%
79	12.602	3592	3596	3599	rBV6	2777	1825	0.23%	0.030%
80	12.654	3608	3612	3615	rVB6	1809	1293	0.16%	0.021%
81	12.673	3615	3618	3619	rBV2	1188	734	0.09%	0.012%
82	12.799	3654	3657	3661	rVV5	1673	1261	0.16%	0.021%
83	12.850	3670	3673	3677	rBV6	1642	1418	0.18%	0.023%
84	12.882	3681	3683	3687	rBV5	1288	1188	0.15%	0.020%
85	12.963	3706	3708	3710	rBV3	1224	652	0.08%	0.011%
86	13.020	3723	3726	3728	rBV4	1041	691	0.09%	0.011%
87	13.065	3738	3740	3743	rVB3	2045	1056	0.13%	0.017%
88	13.165	3767	3771	3773	rBV4	1839	1223	0.15%	0.020%
89	13.374	3833	3836	3839	rBV5	1867	1022	0.13%	0.017%
90	13.458	3858	3862	3865	rBV6	1200	1226	0.15%	0.020%
91	13.625	3910	3914	3917	rBV6	2006	2154	0.27%	0.036%
92	13.805	3965	3970	3975	rBV8	2096	2337	0.29%	0.039%
93	13.959	4015	4018	4019	rBV2	1089	634	0.08%	0.010%
94	14.165	4080	4082	4086	rBV5	1227	934	0.12%	0.015%
95	14.268	4110	4114	4115	rBV5	1165	903	0.11%	0.015%
96	14.461	4171	4174	4177	rBV5	1790	1269	0.16%	0.021%
97	14.525	4191	4194	4196	rBV4	1333	824	0.10%	0.014%
98	14.564	4202	4206	4207	rBV4	1884	1305	0.16%	0.022%
99	14.667	4236	4238	4241	rVB3	1566	754	0.09%	0.012%
100	15.535	4506	4508	4511	rBV4	2267	1302	0.16%	0.021%




Sum of corrected areas: 6065220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030729.D
Acq On : 20 Apr 2023 20:06
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

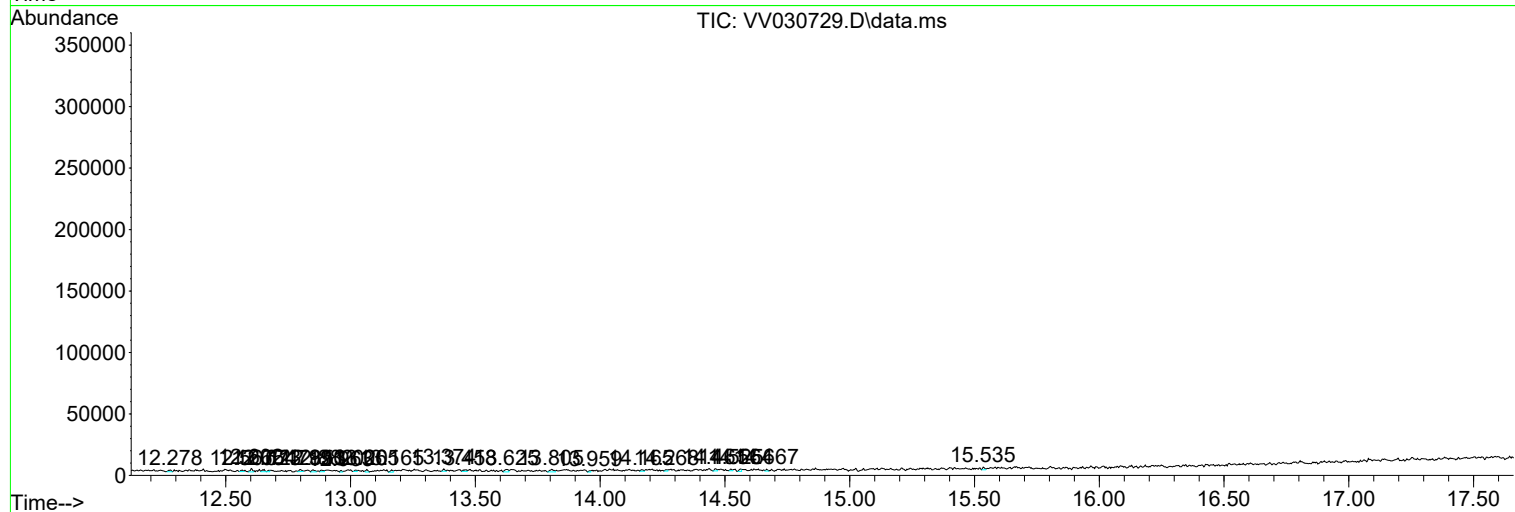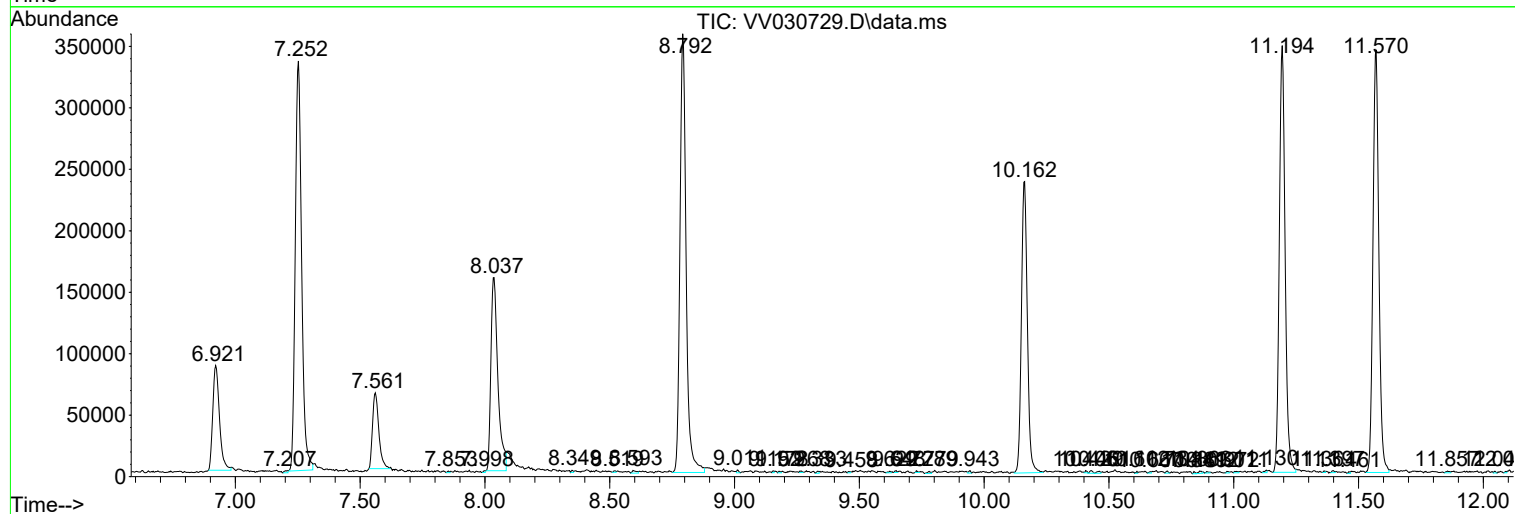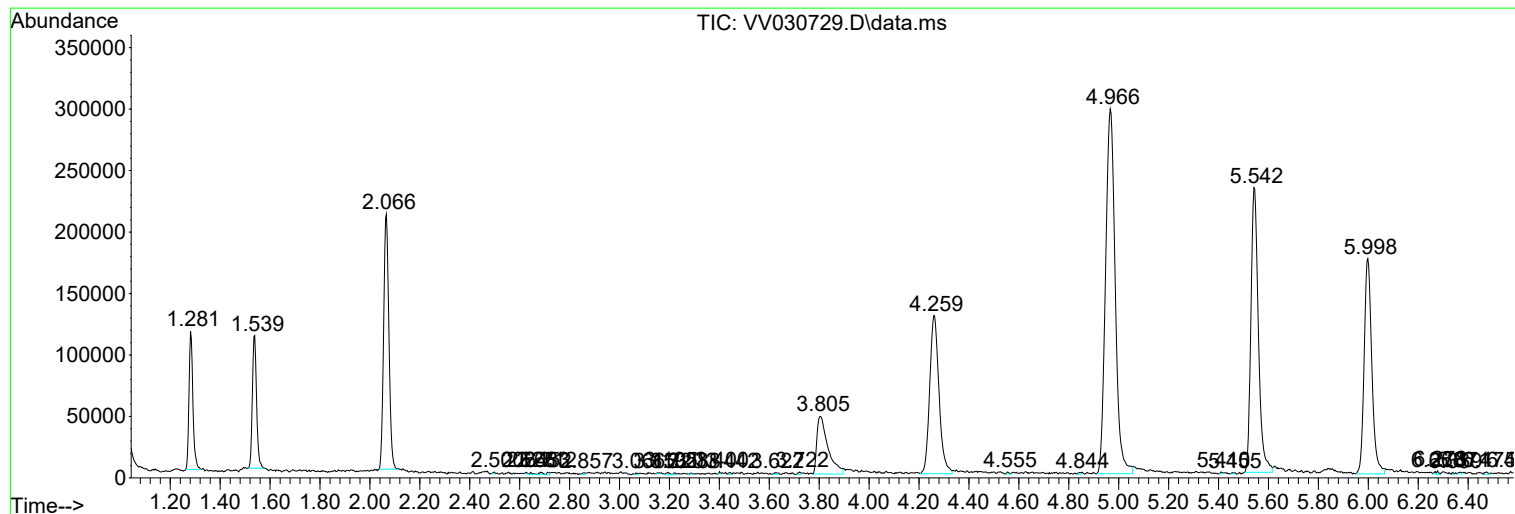

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030729.D
Acq On : 20 Apr 2023 20:06
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030729.D
Acq On : 20 Apr 2023 20:06
Operator : SY/MD
Sample : 02334-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------