

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030734.D
 Acq On : 20 Apr 2023 22:28
 Operator : SY/MD
 Sample : 02440-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	86	rBV	104560	113040	14.84%	1.841%
2	1.535	147	154	167	rVB	93759	112857	14.81%	1.838%
3	2.063	310	318	332	rVB	192986	281896	37.00%	4.591%
4	2.400	419	423	424	rBV2	1294	740	0.10%	0.012%
5	2.449	434	438	440	rBV4	2013	1660	0.22%	0.027%
6	2.754	527	533	535	rBV6	1530	1630	0.21%	0.027%
7	2.879	571	572	575	rVB3	2061	922	0.12%	0.015%
8	2.921	583	585	589	rBV3	1464	972	0.13%	0.016%
9	2.940	589	591	594	rVV4	1177	730	0.10%	0.012%
10	2.992	601	607	611	rVB9	1841	1748	0.23%	0.028%
11	3.024	611	617	622	rBV9	1354	1996	0.26%	0.033%
12	3.092	635	638	641	rVV5	1114	745	0.10%	0.012%
13	3.146	652	655	657	rBV3	1320	739	0.10%	0.012%
14	3.178	662	665	668	rVV5	1452	1106	0.15%	0.018%
15	3.214	672	676	678	rVV5	1488	1050	0.14%	0.017%
16	3.227	678	680	683	rVV3	1192	693	0.09%	0.011%
17	3.371	722	725	726	rBV3	1385	998	0.13%	0.016%
18	3.490	759	762	764	rBV4	1716	1129	0.15%	0.018%
19	3.677	817	820	823	rVB3	1500	923	0.12%	0.015%
20	3.693	823	825	828	rBV4	954	675	0.09%	0.011%
21	3.715	828	832	836	rVB7	1243	1190	0.16%	0.019%
22	3.754	842	844	847	rBV4	1949	1547	0.20%	0.025%
23	3.799	849	858	881	rVV	49490	133581	17.53%	2.176%
24	4.259	988	1001	1024	rVB	123780	308478	40.48%	5.024%
25	4.596	1103	1106	1109	rBV4	1809	1490	0.20%	0.024%
26	4.677	1125	1131	1134	rBV7	1736	1706	0.22%	0.028%
27	4.773	1157	1161	1162	rBV4	1550	821	0.11%	0.013%
28	4.966	1199	1221	1251	rBV2	284018	761962	100.00%	12.409%
29	5.156	1278	1280	1283	rBV4	1945	1119	0.15%	0.018%
30	5.493	1382	1385	1387	rBV5	1431	930	0.12%	0.015%
31	5.542	1387	1400	1422	rBV	274242	571063	74.95%	9.300%
32	5.735	1457	1460	1462	rBV4	1445	854	0.11%	0.014%
33	5.940	1522	1524	1526	rVB3	1968	739	0.10%	0.012%
34	5.998	1527	1542	1560	rBV2	167586	352653	46.28%	5.743%
35	6.339	1646	1648	1651	rVB4	1492	741	0.10%	0.012%
36	6.561	1715	1717	1719	rBV3	1285	720	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030734.D
 Acq On : 20 Apr 2023 22:28
 Operator : SY/MD
 Sample : 02440-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.619	1732	1735	1736	rBV3	1482	776	0.10%	0.013%
38	6.670	1745	1751	1753	rBV7	1408	1208	0.16%	0.020%
39	6.754	1774	1777	1780	rBV4	1370	1159	0.15%	0.019%
40	6.831	1798	1801	1805	rBV6	1001	858	0.11%	0.014%
41	6.921	1818	1829	1849	rBV	84546	160372	21.05%	2.612%
42	7.204	1914	1917	1919	rBV3	1343	740	0.10%	0.012%
43	7.252	1921	1932	1951	rBV	315025	560255	73.53%	9.124%
44	7.561	2019	2028	2043	rBV	61081	108160	14.19%	1.762%
45	7.741	2082	2084	2088	rBV4	1656	1284	0.17%	0.021%
46	7.873	2123	2125	2127	rVB2	1961	783	0.10%	0.013%
47	7.892	2127	2131	2135	rBV6	1977	1441	0.19%	0.023%
48	8.034	2166	2175	2206	rBV	161911	326136	42.80%	5.311%
49	8.509	2321	2323	2326	rBV4	1179	830	0.11%	0.014%
50	8.548	2333	2335	2338	rBV4	1308	731	0.10%	0.012%
51	8.792	2400	2411	2434	rBV	420186	697649	91.56%	11.362%
52	9.001	2473	2476	2478	rBV4	1584	908	0.12%	0.015%
53	9.069	2491	2497	2498	rBV6	1990	1790	0.23%	0.029%
54	9.326	2575	2577	2580	rBV4	1138	797	0.10%	0.013%
55	9.371	2590	2591	2594	rBV3	1137	677	0.09%	0.011%
56	9.429	2606	2609	2611	rBV4	1180	676	0.09%	0.011%
57	9.654	2672	2679	2681	rBV8	2280	2397	0.31%	0.039%
58	9.667	2681	2683	2687	rBV4	864	761	0.10%	0.012%
59	9.767	2711	2714	2717	rVB4	1509	898	0.12%	0.015%
60	9.796	2717	2723	2724	rBV5	1327	1155	0.15%	0.019%
61	10.072	2805	2809	2811	rBV4	1550	1014	0.13%	0.017%
62	10.162	2825	2837	2856	rBV	224643	365927	48.02%	5.960%
63	10.252	2864	2865	2870	rBV5	1217	828	0.11%	0.013%
64	10.345	2888	2894	2897	rBV6	1721	1762	0.23%	0.029%
65	10.374	2901	2903	2910	rVB5	1631	1822	0.24%	0.030%
66	10.432	2917	2921	2922	rBV4	1069	813	0.11%	0.013%
67	10.474	2931	2934	2937	rBV4	1197	985	0.13%	0.016%
68	10.551	2955	2958	2960	rBV4	1619	883	0.12%	0.014%
69	10.631	2979	2983	2984	rBV3	1145	770	0.10%	0.013%
70	10.686	2997	3000	3001	rVV3	1996	1115	0.15%	0.018%
71	10.696	3001	3003	3006	rVB4	1582	932	0.12%	0.015%
72	10.754	3019	3021	3024	rBV4	1239	793	0.10%	0.013%
73	10.918	3070	3072	3075	rBV3	1516	1105	0.15%	0.018%
74	10.976	3088	3090	3096	rVB7	1825	1704	0.22%	0.028%
75	11.117	3128	3134	3135	rBV6	1750	1349	0.18%	0.022%
76	11.194	3145	3158	3178	rBV	404245	658378	86.41%	10.722%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030734.D
 Acq On : 20 Apr 2023 22:28
 Operator : SY/MD
 Sample : 02440-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.429	3228	3231	3233	rBV3	1437	876	0.11%	0.014%
78	11.570	3260	3275	3292	rBV	325331	537131	70.49%	8.748%
79	11.863	3363	3366	3374	rVB8	1470	1313	0.17%	0.021%
80	11.895	3374	3376	3379	rBV4	1070	722	0.09%	0.012%
81	12.049	3421	3424	3430	rVB8	1774	1277	0.17%	0.021%
82	12.429	3539	3542	3545	rBV5	1384	881	0.12%	0.014%
83	12.493	3560	3562	3565	rVV4	1526	967	0.13%	0.016%
84	12.660	3611	3614	3615	rBV3	1771	993	0.13%	0.016%
85	12.689	3621	3623	3626	rBV4	1073	770	0.10%	0.013%
86	12.760	3641	3645	3647	rBV4	1417	1051	0.14%	0.017%
87	12.805	3657	3659	3661	rBV3	1397	923	0.12%	0.015%
88	12.860	3673	3676	3679	rBV4	1085	818	0.11%	0.013%
89	12.927	3695	3697	3698	rBV2	1227	674	0.09%	0.011%
90	13.207	3781	3784	3789	rBV6	1728	2103	0.28%	0.034%
91	13.229	3789	3791	3794	rVV4	1759	962	0.13%	0.016%
92	13.297	3809	3812	3816	rBV6	1171	945	0.12%	0.015%
93	13.400	3841	3844	3846	rBV4	1972	1123	0.15%	0.018%
94	13.590	3899	3903	3907	rBV6	1649	1455	0.19%	0.024%
95	13.959	4015	4018	4021	rBV5	1743	1061	0.14%	0.017%
96	14.046	4042	4045	4048	rBV5	1292	862	0.11%	0.014%
97	14.162	4078	4081	4084	rBV5	1442	1015	0.13%	0.017%
98	14.175	4084	4085	4090	rVB5	1317	830	0.11%	0.014%
99	14.477	4174	4179	4184	rBV7	1510	1743	0.23%	0.028%
100	14.606	4217	4219	4223	rVB5	1817	1257	0.16%	0.020%




Sum of corrected areas: 6140216

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030734.D
Acq On : 20 Apr 2023 22:28
Operator : SY/MD
Sample : 02440-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

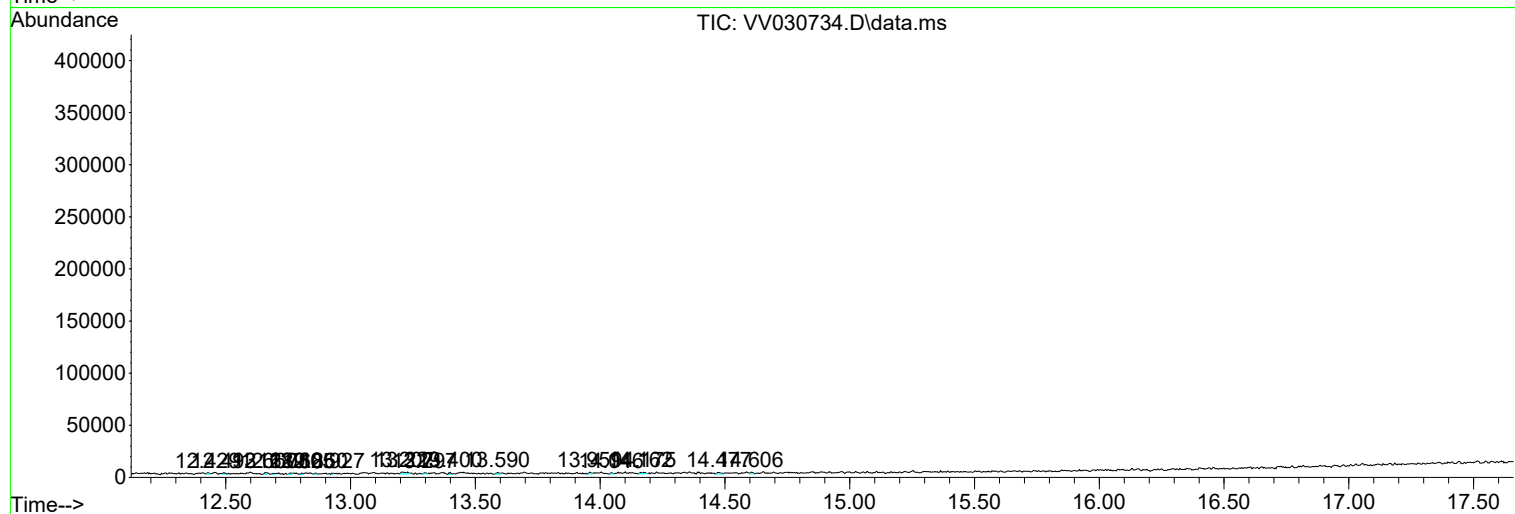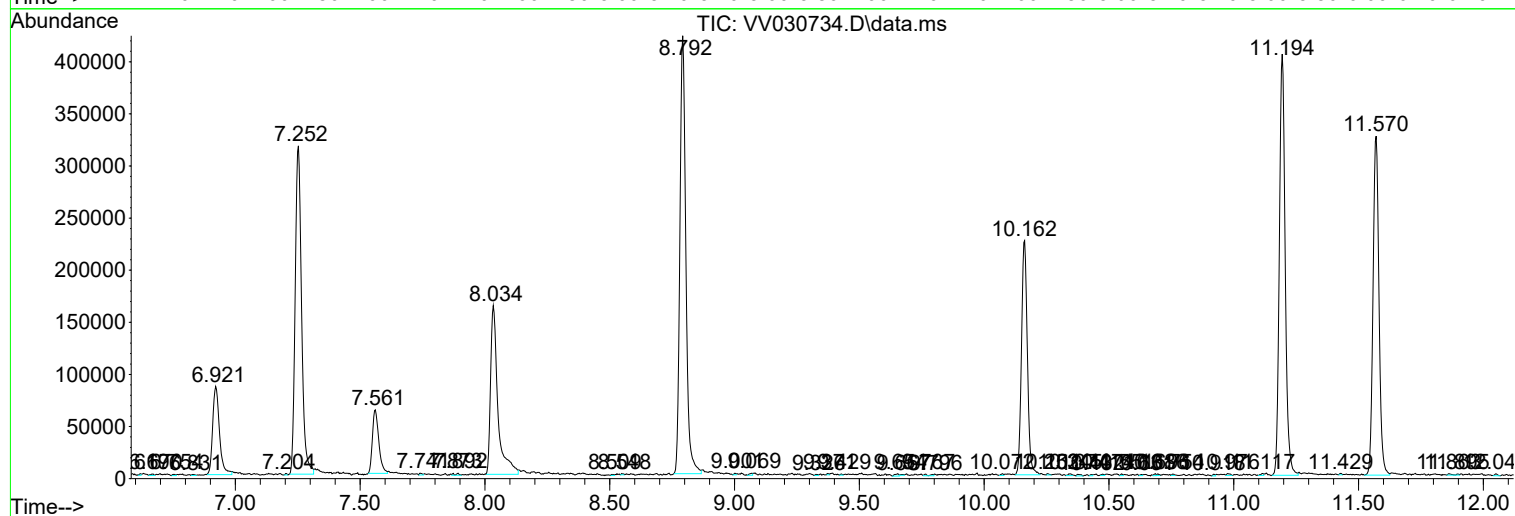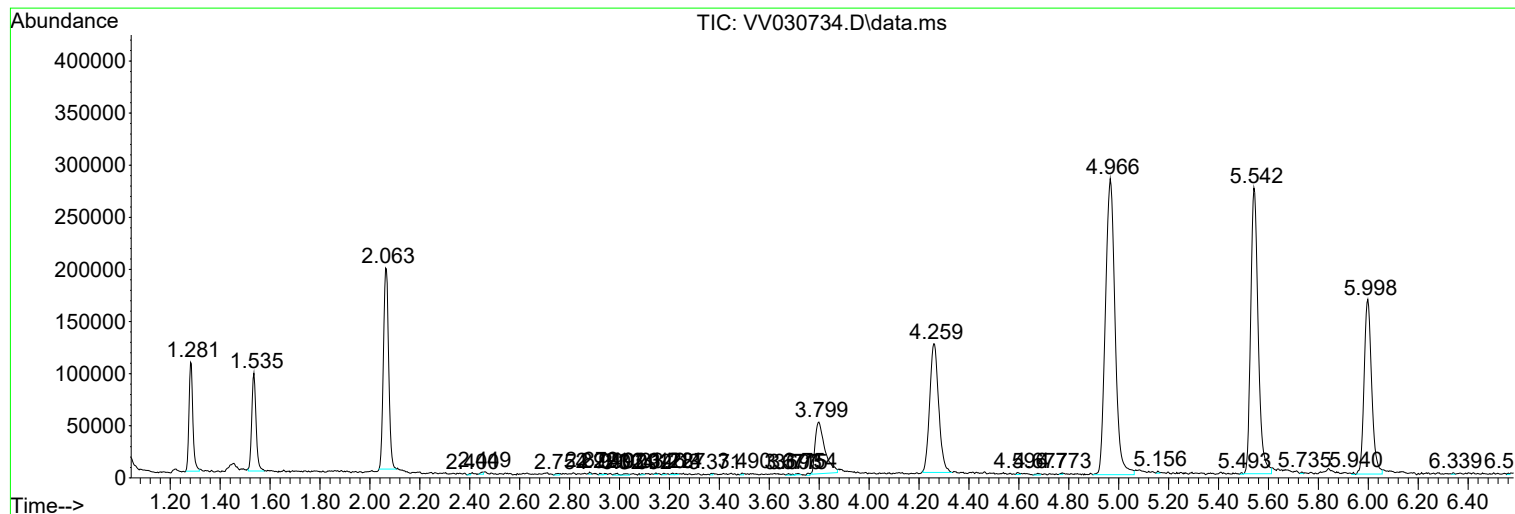

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030734.D
Acq On : 20 Apr 2023 22:28
Operator : SY/MD
Sample : 02440-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030734.D
Acq On : 20 Apr 2023 22:28
Operator : SY/MD
Sample : 02440-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------