

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030735.D
 Acq On : 20 Apr 2023 22:52
 Operator : SY/MD
 Sample : 02440-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	92	rVB	109558	120606	15.00%	1.902%
2	1.535	147	154	166	rVB	101344	119464	14.86%	1.884%
3	2.063	309	318	332	rBV	208082	303672	37.78%	4.788%
4	2.397	418	422	424	rVB3	1012	612	0.08%	0.010%
5	2.410	424	426	429	rBV4	1350	803	0.10%	0.013%
6	2.580	477	479	480	rBV2	1393	543	0.07%	0.009%
7	2.629	492	494	497	rBV3	1165	607	0.08%	0.010%
8	2.786	539	543	544	rBV4	1297	941	0.12%	0.015%
9	2.883	571	573	578	rBV6	1119	1067	0.13%	0.017%
10	3.008	607	612	614	rBV5	1789	1261	0.16%	0.020%
11	3.108	639	643	645	rBV4	1408	1074	0.13%	0.017%
12	3.146	653	655	657	rBV3	1245	840	0.10%	0.013%
13	3.410	732	737	738	rBV5	1260	971	0.12%	0.015%
14	3.471	754	756	757	rBV2	2022	830	0.10%	0.013%
15	3.674	816	819	821	rVB3	1413	668	0.08%	0.011%
16	3.693	821	825	831	rBV7	2654	2252	0.28%	0.036%
17	3.725	831	835	836	rBV3	1140	846	0.11%	0.013%
18	3.796	849	857	883	rVV2	52147	143988	17.91%	2.270%
19	4.259	989	1001	1022	rVB	127229	313840	39.04%	4.949%
20	4.619	1111	1113	1116	rVB4	1296	746	0.09%	0.012%
21	4.635	1116	1118	1121	rBV3	1271	819	0.10%	0.013%
22	4.728	1145	1147	1152	rBV5	1192	1012	0.13%	0.016%
23	4.767	1157	1159	1162	rBV4	946	548	0.07%	0.009%
24	4.905	1199	1202	1203	rBV4	1308	822	0.10%	0.013%
25	4.966	1205	1221	1251	rVV2	298742	803800	100.00%	12.674%
26	5.336	1333	1336	1337	rBV2	1514	708	0.09%	0.011%
27	5.458	1371	1374	1376	rVB4	1444	790	0.10%	0.012%
28	5.542	1388	1400	1422	rBV	278094	573731	71.38%	9.047%
29	5.995	1530	1541	1564	rBV	174870	359670	44.75%	5.671%
30	6.252	1618	1621	1623	rBV3	1676	1207	0.15%	0.019%
31	6.426	1672	1675	1676	rBV3	1302	659	0.08%	0.010%
32	6.561	1714	1717	1720	rBV4	1416	923	0.11%	0.015%
33	6.677	1747	1753	1756	rBV8	2363	2063	0.26%	0.033%
34	6.693	1756	1758	1759	rBV2	1706	715	0.09%	0.011%
35	6.751	1774	1776	1779	rBV2	1231	752	0.09%	0.012%
36	6.921	1815	1829	1846	rBV	89950	175280	21.81%	2.764%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030735.D
 Acq On : 20 Apr 2023 22:52
 Operator : SY/MD
 Sample : 02440-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.108	1884	1887	1889	rBV4	1885	1074	0.13%	0.017%
38	7.252	1921	1932	1956	rBV	336466	593903	73.89%	9.365%
39	7.423	1983	1985	1988	rBV4	1620	780	0.10%	0.012%
40	7.500	2006	2009	2010	rBV3	1407	860	0.11%	0.014%
41	7.561	2019	2028	2044	rBV2	64637	113019	14.06%	1.782%
42	7.712	2071	2075	2077	rBV5	1893	1603	0.20%	0.025%
43	7.982	2155	2159	2161	rBV4	1565	1343	0.17%	0.021%
44	8.034	2165	2175	2193	rBV	168090	320987	39.93%	5.061%
45	8.294	2253	2256	2258	rBV4	1731	1347	0.17%	0.021%
46	8.333	2264	2268	2274	rBV7	2306	2399	0.30%	0.038%
47	8.503	2319	2321	2323	rBV2	1491	875	0.11%	0.014%
48	8.661	2368	2370	2372	rBV3	1414	838	0.10%	0.013%
49	8.792	2399	2411	2434	rBV	427173	710923	88.45%	11.210%
50	9.149	2519	2522	2524	rBV4	1287	720	0.09%	0.011%
51	9.304	2567	2570	2574	rBV6	1704	1644	0.20%	0.026%
52	9.329	2574	2578	2579	rVV4	975	661	0.08%	0.010%
53	9.464	2617	2620	2622	rBV3	1646	1078	0.13%	0.017%
54	9.731	2701	2703	2704	rBV2	1356	595	0.07%	0.009%
55	9.902	2754	2756	2758	rBV3	1062	499	0.06%	0.008%
56	9.927	2762	2764	2766	rBV3	961	508	0.06%	0.008%
57	9.998	2784	2786	2787	rBV3	1095	536	0.07%	0.008%
58	10.050	2800	2802	2805	rBV5	1721	866	0.11%	0.014%
59	10.075	2807	2810	2814	rVB5	1211	1010	0.13%	0.016%
60	10.111	2818	2821	2823	rBV3	1924	1267	0.16%	0.020%
61	10.162	2825	2837	2853	rBV	241971	386262	48.05%	6.091%
62	10.333	2888	2890	2893	rBV4	1406	1036	0.13%	0.016%
63	10.419	2915	2917	2921	rBV6	1046	767	0.10%	0.012%
64	10.564	2959	2962	2965	rBV5	1361	894	0.11%	0.014%
65	10.689	2997	3001	3004	rBV5	1723	1692	0.21%	0.027%
66	10.744	3014	3018	3023	rVB7	1790	1678	0.21%	0.026%
67	10.963	3083	3086	3088	rBV3	1042	664	0.08%	0.010%
68	11.050	3111	3113	3116	rVB4	1231	615	0.08%	0.010%
69	11.072	3116	3120	3122	rBV4	1332	946	0.12%	0.015%
70	11.088	3122	3125	3129	rVB5	1334	876	0.11%	0.014%
71	11.111	3129	3132	3134	rBV4	1333	843	0.10%	0.013%
72	11.194	3147	3158	3175	rBV	410273	653885	81.35%	10.311%
73	11.320	3194	3197	3200	rBV5	2137	1662	0.21%	0.026%
74	11.432	3230	3232	3236	rBV5	1645	1028	0.13%	0.016%
75	11.570	3263	3275	3295	rBV	348678	565985	70.41%	8.924%
76	11.683	3308	3310	3312	rBV3	1235	624	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030735.D
 Acq On : 20 Apr 2023 22:52
 Operator : SY/MD
 Sample : 02440-04 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.744	3327	3329	3333	rBV5	1233	909	0.11%	0.014%
78	11.953	3389	3394	3401	rBV8	1299	1709	0.21%	0.027%
79	12.091	3435	3437	3438	rBV2	1313	576	0.07%	0.009%
80	12.213	3474	3475	3478	rVB3	1368	718	0.09%	0.011%
81	12.236	3478	3482	3486	rBV7	1805	1863	0.23%	0.029%
82	12.635	3603	3606	3607	rBV2	1127	615	0.08%	0.010%
83	12.680	3615	3620	3624	rBV8	1592	1265	0.16%	0.020%
84	12.699	3624	3626	3630	rVV4	1346	818	0.10%	0.013%
85	12.795	3653	3656	3658	rBV4	1892	1282	0.16%	0.020%
86	12.905	3687	3690	3693	rBV5	1400	1123	0.14%	0.018%
87	12.937	3697	3700	3703	rBV4	1637	1097	0.14%	0.017%
88	13.027	3725	3728	3729	rBV3	1072	514	0.06%	0.008%
89	13.120	3753	3757	3760	rBV5	1357	1148	0.14%	0.018%
90	13.207	3779	3784	3787	rBV7	2799	2711	0.34%	0.043%
91	13.303	3811	3814	3815	rBV4	1135	520	0.06%	0.008%
92	13.538	3884	3887	3888	rBV3	1007	561	0.07%	0.009%
93	13.615	3909	3911	3913	rVB3	1736	701	0.09%	0.011%
94	13.651	3920	3922	3924	rVB3	1329	552	0.07%	0.009%
95	13.664	3924	3926	3929	rBV4	1378	869	0.11%	0.014%
96	13.889	3994	3996	3999	rBV3	1316	686	0.09%	0.011%
97	13.959	4014	4018	4021	rBV6	1187	888	0.11%	0.014%
98	14.139	4070	4074	4076	rVB5	1934	1203	0.15%	0.019%
99	14.278	4115	4117	4118	rBV2	1148	517	0.06%	0.008%
100	14.844	4289	4293	4295	rBV5	1797	1161	0.14%	0.018%




Sum of corrected areas: 6341928

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030735.D
Acq On : 20 Apr 2023 22:52
Operator : SY/MD
Sample : 02440-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

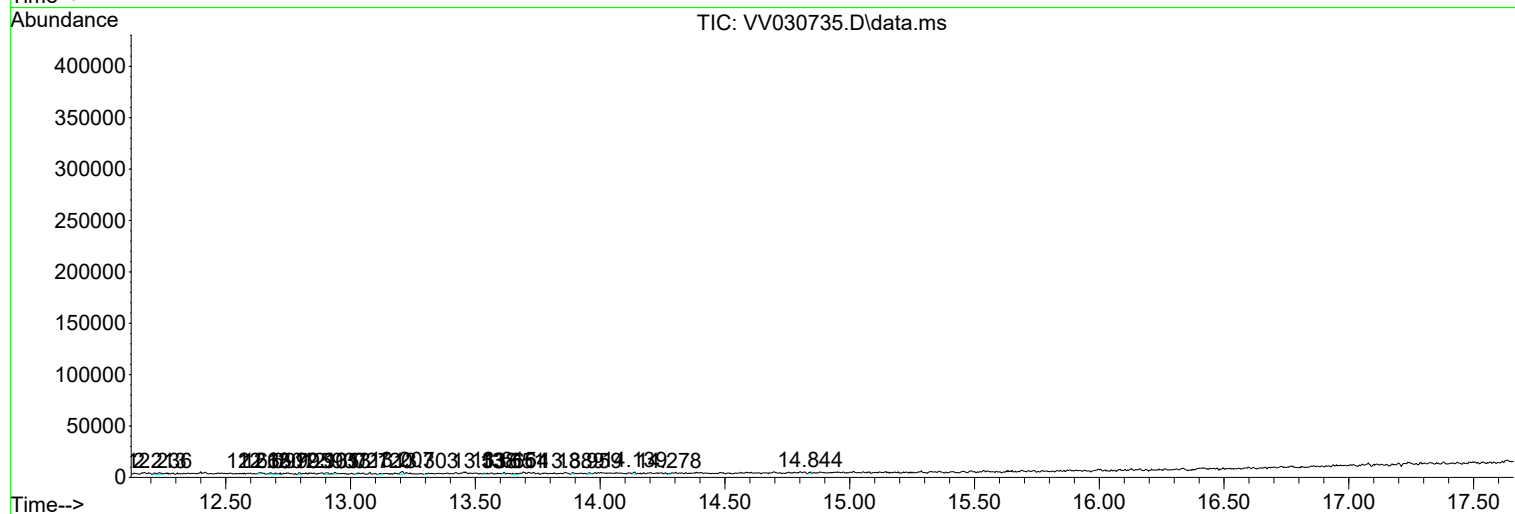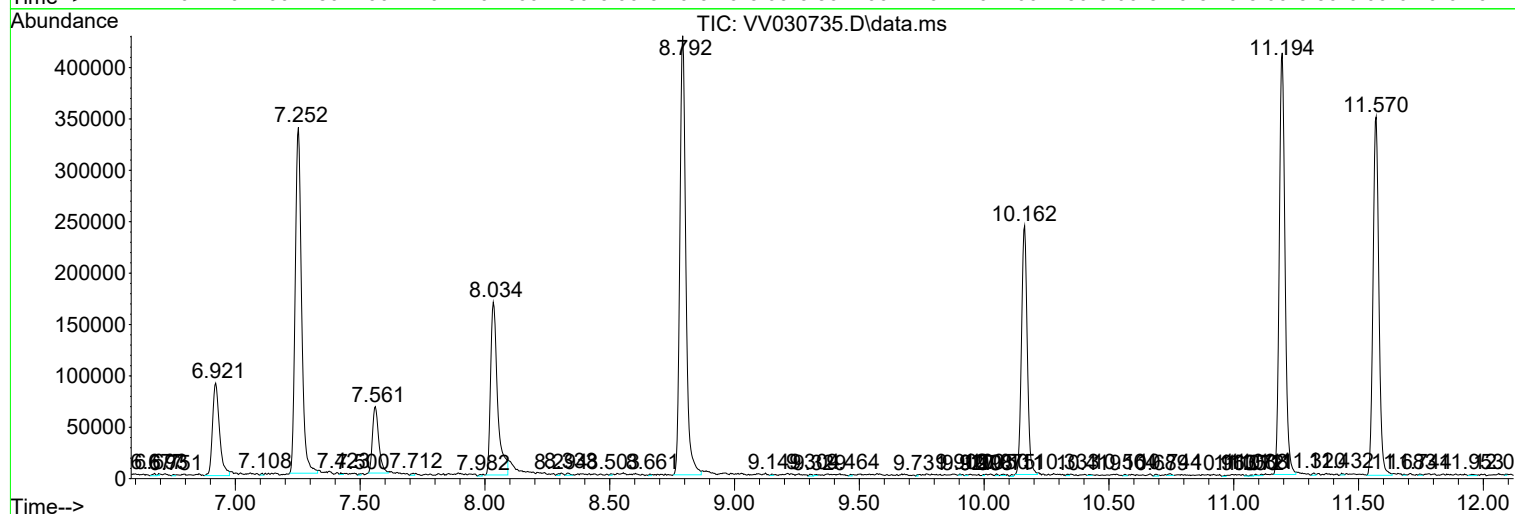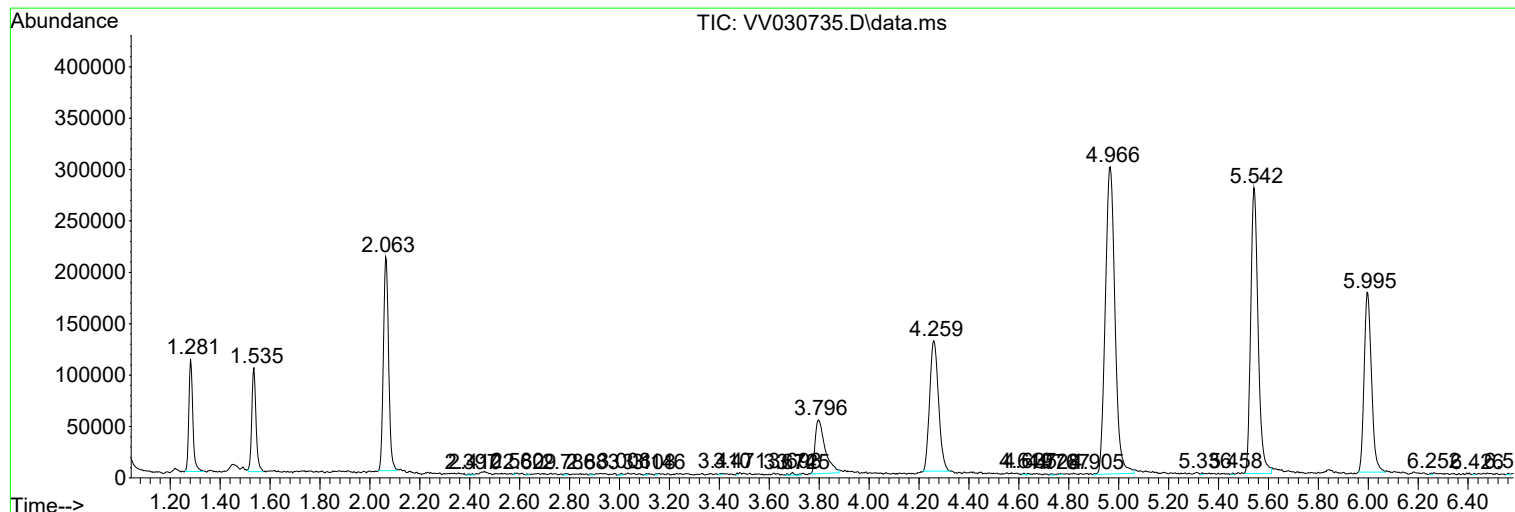

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030735.D
Acq On : 20 Apr 2023 22:52
Operator : SY/MD
Sample : 02440-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030735.D
Acq On : 20 Apr 2023 22:52
Operator : SY/MD
Sample : 02440-04 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc