

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030736.D
 Acq On : 20 Apr 2023 23:16
 Operator : SY/MD
 Sample : 02440-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M

Title : VOC Analysis

Signal : TIC: VV030736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	86	rBV	102039	110085	14.84%	1.836%
2	1.536	148	154	164	rVB	100032	113251	15.26%	1.889%
3	2.063	309	318	331	rBV	187032	273573	36.87%	4.564%
4	2.346	402	406	407	rBV4	1055	806	0.11%	0.013%
5	2.423	427	430	432	rBV3	981	639	0.09%	0.011%
6	2.709	517	519	522	rBV4	1376	817	0.11%	0.014%
7	2.770	537	538	540	rBV2	1394	636	0.09%	0.011%
8	2.851	559	563	566	rBV5	1439	876	0.12%	0.015%
9	2.912	580	582	587	rBV6	1133	1125	0.15%	0.019%
10	3.002	608	610	613	rBV3	1368	828	0.11%	0.014%
11	3.066	626	630	634	rBV7	992	881	0.12%	0.015%
12	3.214	673	676	677	rBV3	1303	649	0.09%	0.011%
13	3.339	714	715	720	rBV4	1449	1034	0.14%	0.017%
14	3.397	731	733	737	rBV4	900	641	0.09%	0.011%
15	3.468	751	755	757	rBV3	2043	1448	0.20%	0.024%
16	3.484	757	760	765	rVB7	1500	1207	0.16%	0.020%
17	3.519	769	771	773	rBV3	1681	1167	0.16%	0.019%
18	3.564	783	785	788	rVB4	1522	802	0.11%	0.013%
19	3.741	837	840	844	rVV6	1286	1172	0.16%	0.020%
20	3.802	850	859	879	rBV	47973	133039	17.93%	2.219%
21	4.182	975	977	982	rBV6	1643	1429	0.19%	0.024%
22	4.262	988	1002	1022	rVB	117280	294086	39.64%	4.906%
23	4.593	1102	1105	1109	rBV5	1608	1504	0.20%	0.025%
24	4.706	1134	1140	1142	rBV7	1366	1210	0.16%	0.020%
25	4.780	1161	1163	1168	rVB5	1430	936	0.13%	0.016%
26	4.806	1168	1171	1174	rBV4	1113	876	0.12%	0.015%
27	4.876	1190	1193	1200	rVB8	2257	2254	0.30%	0.038%
28	4.966	1200	1221	1248	rBV2	272908	741903	100.00%	12.376%
29	5.375	1346	1348	1351	rBV4	1324	830	0.11%	0.014%
30	5.404	1353	1357	1361	rBV6	1524	1495	0.20%	0.025%
31	5.542	1386	1400	1424	rBV	271922	574721	77.47%	9.587%
32	5.998	1530	1542	1560	rBV	159907	330876	44.60%	5.520%
33	6.217	1607	1610	1613	rBV5	1248	647	0.09%	0.011%
34	6.420	1670	1673	1674	rBV3	1292	694	0.09%	0.012%
35	6.548	1711	1713	1716	rBV4	1213	679	0.09%	0.011%
36	6.683	1752	1755	1757	rBV4	1390	905	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030736.D
 Acq On : 20 Apr 2023 23:16
 Operator : SY/MD
 Sample : 02440-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.725	1766	1768	1772	rVB4	2375	1208	0.16%	0.020%
38	6.751	1772	1776	1779	rBV5	1756	1553	0.21%	0.026%
39	6.822	1796	1798	1800	rBV2	1613	672	0.09%	0.011%
40	6.921	1818	1829	1846	rBV	85699	158732	21.40%	2.648%
41	7.191	1910	1913	1918	rBV8	1538	1500	0.20%	0.025%
42	7.252	1920	1932	1952	rBV	303425	537647	72.47%	8.969%
43	7.561	2019	2028	2047	rBV	60114	106213	14.32%	1.772%
44	7.847	2115	2117	2120	rBV4	1330	718	0.10%	0.012%
45	7.911	2134	2137	2139	rBV4	1213	766	0.10%	0.013%
46	7.998	2159	2164	2165	rBV5	2158	1798	0.24%	0.030%
47	8.034	2166	2175	2204	rBV	154571	315097	42.47%	5.256%
48	8.532	2327	2330	2333	rBV5	1533	1101	0.15%	0.018%
49	8.561	2335	2339	2341	rVV5	1234	839	0.11%	0.014%
50	8.574	2341	2343	2347	rVB4	1943	758	0.10%	0.013%
51	8.596	2347	2350	2352	rBV4	1369	912	0.12%	0.015%
52	8.648	2363	2366	2368	rBV3	1663	1049	0.14%	0.017%
53	8.751	2393	2398	2399	rBV5	1563	849	0.11%	0.014%
54	8.792	2400	2411	2431	rVV	419345	720481	97.11%	12.019%
55	9.207	2538	2540	2545	rVB6	2104	1403	0.19%	0.023%
56	9.342	2578	2582	2583	rBV3	1113	832	0.11%	0.014%
57	9.362	2586	2588	2592	rVV4	1117	812	0.11%	0.014%
58	9.477	2621	2624	2627	rBV5	1189	706	0.10%	0.012%
59	9.522	2634	2638	2639	rBV4	1015	694	0.09%	0.012%
60	9.661	2678	2681	2685	rBV3	1325	1043	0.14%	0.017%
61	9.940	2767	2768	2771	rBV3	1190	724	0.10%	0.012%
62	10.159	2826	2836	2853	rVB	222204	353312	47.62%	5.894%
63	10.239	2860	2861	2865	rVB4	1590	694	0.09%	0.012%
64	10.461	2928	2930	2935	rVB6	1428	894	0.12%	0.015%
65	10.490	2935	2939	2942	rBV6	1531	1294	0.17%	0.022%
66	10.677	2995	2997	3002	rBV6	1080	950	0.13%	0.016%
67	10.905	3065	3068	3072	rBV5	1730	1314	0.18%	0.022%
68	10.924	3072	3074	3077	rVV4	1360	658	0.09%	0.011%
69	11.017	3098	3103	3105	rBV5	1327	1092	0.15%	0.018%
70	11.108	3128	3131	3133	rVB4	1268	689	0.09%	0.011%
71	11.194	3147	3158	3180	rBV	396442	634655	85.54%	10.587%
72	11.429	3228	3231	3232	rBV2	1324	712	0.10%	0.012%
73	11.484	3244	3248	3251	rBV5	1288	1154	0.16%	0.019%
74	11.522	3258	3260	3262	rBV3	1576	860	0.12%	0.014%
75	11.571	3264	3275	3295	rVB	309648	512040	69.02%	8.542%
76	11.773	3336	3338	3342	rBV5	964	957	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030736.D
 Acq On : 20 Apr 2023 23:16
 Operator : SY/MD
 Sample : 02440-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.802	3345	3347	3350	rBV3	1466	955	0.13%	0.016%
78	11.853	3361	3363	3366	rBV4	2136	1380	0.19%	0.023%
79	12.066	3425	3429	3430	rBV4	1388	1056	0.14%	0.018%
80	12.252	3484	3487	3488	rBV3	1375	842	0.11%	0.014%
81	12.333	3508	3512	3513	rBV2	1447	941	0.13%	0.016%
82	12.378	3524	3526	3528	rBV3	1403	742	0.10%	0.012%
83	12.590	3588	3592	3595	rBV7	1409	1285	0.17%	0.021%
84	12.744	3636	3640	3643	rVB5	1266	977	0.13%	0.016%
85	12.879	3677	3682	3683	rBV3	1838	860	0.12%	0.014%
86	12.982	3709	3714	3715	rBV4	1474	1169	0.16%	0.020%
87	13.098	3747	3750	3755	rVB7	1806	1264	0.17%	0.021%
88	13.127	3755	3759	3760	rBV4	1679	1082	0.15%	0.018%
89	13.384	3835	3839	3841	rVB5	1547	899	0.12%	0.015%
90	13.490	3870	3872	3877	rVB6	1238	1017	0.14%	0.017%
91	13.509	3877	3878	3883	rBV4	1387	883	0.12%	0.015%
92	13.532	3883	3885	3890	rBV6	1331	1301	0.18%	0.022%
93	13.638	3912	3918	3920	rBV5	1951	1638	0.22%	0.027%
94	13.799	3966	3968	3970	rBV3	1247	686	0.09%	0.011%
95	13.828	3975	3977	3980	rBV2	906	657	0.09%	0.011%
96	14.197	4087	4092	4094	rBV5	1247	1210	0.16%	0.020%
97	14.278	4115	4117	4121	rBV4	1636	1578	0.21%	0.026%
98	14.448	4166	4170	4171	rBV4	1198	774	0.10%	0.013%
99	15.062	4358	4361	4363	rBV4	1884	1213	0.16%	0.020%
100	15.098	4370	4372	4374	rBV3	1895	977	0.13%	0.016%



Sum of corrected areas: 5994489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030736.D
Acq On : 20 Apr 2023 23:16
Operator : SY/MD
Sample : 02440-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

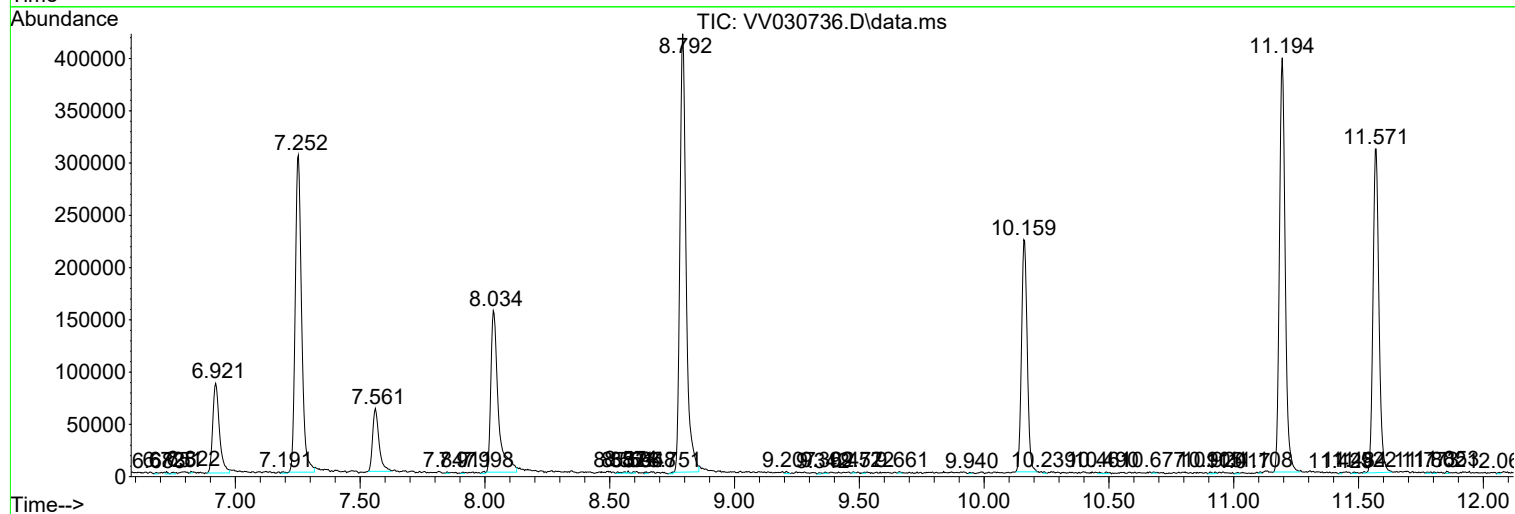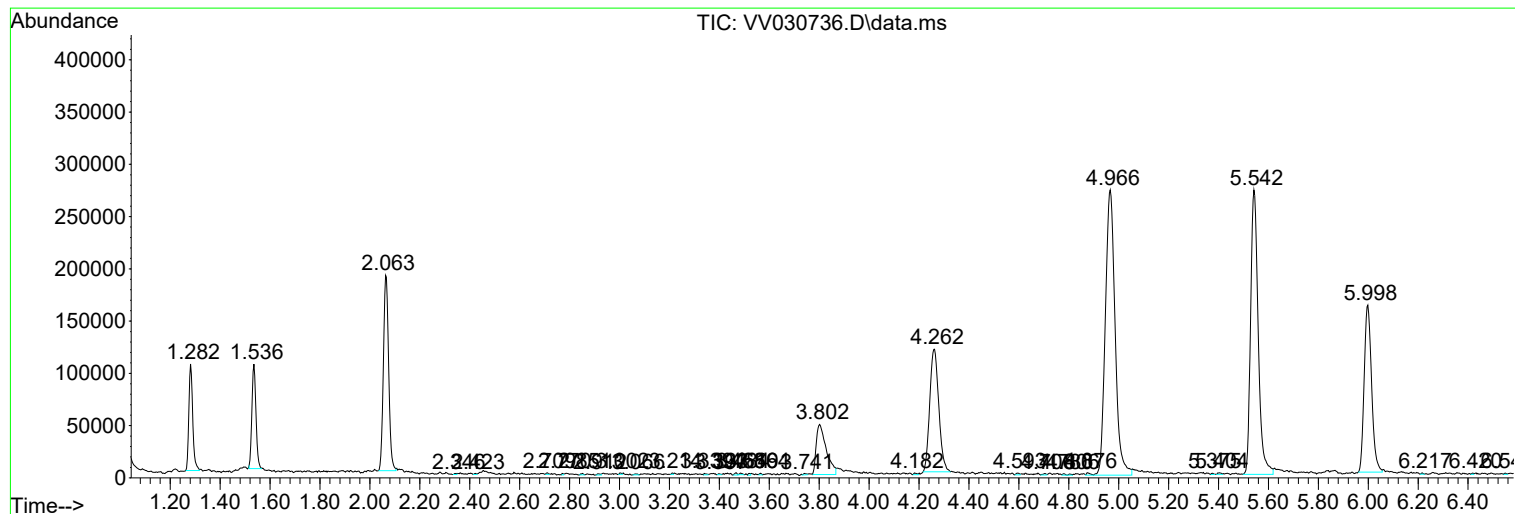

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030736.D
Acq On : 20 Apr 2023 23:16
Operator : SY/MD
Sample : 02440-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030736.D
Acq On : 20 Apr 2023 23:16
Operator : SY/MD
Sample : 02440-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc