

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030739.D
 Acq On : 21 Apr 2023 00:28
 Operator : SY/MD
 Sample : 02440-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rBV	104974	114355	15.30%	1.871%
2	1.536	147	154	168	rVB	93404	109850	14.70%	1.797%
3	2.063	310	318	335	rVB	195000	282747	37.84%	4.625%
4	2.513	455	458	462	rBV5	1477	1237	0.17%	0.020%
5	2.535	462	465	469	rVB6	943	652	0.09%	0.011%
6	2.561	471	473	476	rBV3	1479	832	0.11%	0.014%
7	2.619	487	491	493	rVV5	1159	812	0.11%	0.013%
8	2.770	536	538	542	rBV5	1204	632	0.08%	0.010%
9	2.789	542	544	547	rVB4	1512	682	0.09%	0.011%
10	2.806	547	549	552	rBV4	1324	678	0.09%	0.011%
11	2.892	572	576	578	rBV5	1447	1083	0.14%	0.018%
12	2.976	599	602	603	rBV3	967	604	0.08%	0.010%
13	3.127	647	649	654	rVB6	1667	1208	0.16%	0.020%
14	3.188	666	668	670	rBV3	1821	748	0.10%	0.012%
15	3.252	684	688	689	rBV4	988	712	0.10%	0.012%
16	3.301	699	703	706	rBV6	1647	1227	0.16%	0.020%
17	3.400	731	734	737	rBV5	1036	760	0.10%	0.012%
18	3.426	739	742	747	rVB5	1525	1153	0.15%	0.019%
19	3.452	747	750	756	rBV7	1360	1637	0.22%	0.027%
20	3.490	759	762	763	rBV4	1296	819	0.11%	0.013%
21	3.606	795	798	800	rBV4	1706	1208	0.16%	0.020%
22	3.741	839	840	844	rVB4	1413	917	0.12%	0.015%
23	3.799	849	858	887	rVV	49045	137882	18.45%	2.255%
24	4.188	976	979	980	rBV3	1627	817	0.11%	0.013%
25	4.259	988	1001	1020	rBV	122047	299020	40.01%	4.891%
26	4.555	1091	1093	1094	rBV2	1198	655	0.09%	0.011%
27	4.654	1121	1124	1126	rBV4	1660	1221	0.16%	0.020%
28	4.773	1159	1161	1164	rBV4	1012	789	0.11%	0.013%
29	4.822	1173	1176	1180	rVB5	1240	941	0.13%	0.015%
30	4.966	1205	1221	1247	rBV2	278670	747272	100.00%	12.224%
31	5.429	1363	1365	1367	rBV2	1322	743	0.10%	0.012%
32	5.542	1388	1400	1421	rBV	277656	572333	76.59%	9.362%
33	5.998	1530	1542	1563	rBV2	166095	340523	45.57%	5.570%
34	6.474	1689	1690	1695	rBV5	961	576	0.08%	0.009%
35	6.670	1749	1751	1759	rBV10	1063	1200	0.16%	0.020%
36	6.751	1773	1776	1777	rBV3	1280	679	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030739.D
 Acq On : 21 Apr 2023 00:28
 Operator : SY/MD
 Sample : 02440-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.921	1817	1829	1850	rBV	83942	159724	21.37%	2.613%
38	7.204	1915	1917	1920	rVB4	1400	641	0.09%	0.010%
39	7.252	1920	1932	1949	rBV	314477	566748	75.84%	9.271%
40	7.481	1998	2003	2007	rBV7	1741	2222	0.30%	0.036%
41	7.561	2019	2028	2047	rBV	61465	112754	15.09%	1.844%
42	7.860	2118	2121	2125	rBV6	1775	1458	0.20%	0.024%
43	7.915	2134	2138	2141	rBV6	1554	1032	0.14%	0.017%
44	7.963	2150	2153	2155	rBV4	1476	1077	0.14%	0.018%
45	8.034	2165	2175	2205	rBV	160430	325784	43.60%	5.329%
46	8.519	2324	2326	2329	rBV3	951	776	0.10%	0.013%
47	8.735	2390	2393	2395	rBV4	1725	926	0.12%	0.015%
48	8.792	2399	2411	2431	rBV	429418	714864	95.66%	11.694%
49	9.095	2503	2505	2511	rVB8	1255	1189	0.16%	0.019%
50	9.124	2511	2514	2516	rBV4	2056	1414	0.19%	0.023%
51	9.513	2633	2635	2638	rBV4	1288	686	0.09%	0.011%
52	9.641	2671	2675	2677	rBV4	1170	983	0.13%	0.016%
53	9.728	2700	2702	2706	rVB5	1532	995	0.13%	0.016%
54	9.873	2743	2747	2749	rBV6	1023	817	0.11%	0.013%
55	10.014	2789	2791	2794	rBV4	1457	979	0.13%	0.016%
56	10.069	2805	2808	2809	rBV2	1373	784	0.10%	0.013%
57	10.162	2826	2837	2849	rBV	227467	358844	48.02%	5.870%
58	10.452	2923	2927	2928	rBV4	1613	1039	0.14%	0.017%
59	10.580	2961	2967	2969	rBV7	2225	2130	0.29%	0.035%
60	10.596	2970	2972	2975	rVV5	1319	829	0.11%	0.014%
61	10.628	2980	2982	2986	rVV5	1050	777	0.10%	0.013%
62	10.709	3004	3007	3010	rBV5	1276	798	0.11%	0.013%
63	10.728	3010	3013	3015	rBV4	1419	998	0.13%	0.016%
64	10.915	3068	3071	3074	rBV5	1292	950	0.13%	0.016%
65	11.034	3105	3108	3110	rVB3	1547	936	0.13%	0.015%
66	11.050	3110	3113	3118	rBV6	1713	1329	0.18%	0.022%
67	11.194	3147	3158	3176	rBV	405526	654708	87.61%	10.710%
68	11.477	3244	3246	3250	rBV4	1161	713	0.10%	0.012%
69	11.516	3254	3258	3262	rBV7	1761	1503	0.20%	0.025%
70	11.570	3263	3275	3291	rBV	328954	533364	71.37%	8.725%
71	11.792	3340	3344	3345	rBV4	1062	771	0.10%	0.013%
72	11.982	3401	3403	3405	rBV3	1622	816	0.11%	0.013%
73	12.117	3443	3445	3448	rBV4	1062	669	0.09%	0.011%
74	12.210	3471	3474	3479	rVB6	1416	951	0.13%	0.016%
75	12.365	3519	3522	3524	rBV3	1668	1039	0.14%	0.017%
76	12.413	3535	3537	3538	rVV2	1512	684	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
 Data File : VV030739.D
 Acq On : 21 Apr 2023 00:28
 Operator : SY/MD
 Sample : 02440-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.435	3542	3544	3546	rVB3	1985	840	0.11%	0.014%
78	12.455	3546	3550	3552	rBV5	1351	850	0.11%	0.014%
79	12.471	3552	3555	3558	rBV5	1549	1066	0.14%	0.017%
80	12.516	3566	3569	3572	rBV4	1869	1109	0.15%	0.018%
81	12.583	3586	3590	3593	rBV5	1183	953	0.13%	0.016%
82	12.612	3597	3599	3600	rBV	1240	609	0.08%	0.010%
83	12.722	3631	3633	3637	rBV4	1357	1175	0.16%	0.019%
84	12.747	3639	3641	3645	rVB4	1726	1223	0.16%	0.020%
85	12.976	3706	3712	3716	rBV6	1952	1953	0.26%	0.032%
86	13.014	3720	3724	3726	rBV5	1419	1058	0.14%	0.017%
87	13.040	3730	3732	3738	rBV4	1031	852	0.11%	0.014%
88	13.136	3760	3762	3765	rBV3	1569	765	0.10%	0.013%
89	13.185	3775	3777	3780	rBV3	1149	779	0.10%	0.013%
90	13.355	3828	3830	3832	rBV3	1270	644	0.09%	0.011%
91	13.519	3877	3881	3884	rBV4	1323	1297	0.17%	0.021%
92	13.541	3887	3888	3895	rVB7	1267	1038	0.14%	0.017%
93	13.651	3918	3922	3925	rBV4	1509	1203	0.16%	0.020%
94	13.722	3940	3944	3948	rBV8	1266	1498	0.20%	0.025%
95	13.857	3982	3986	3988	rBV4	800	581	0.08%	0.010%
96	13.869	3988	3990	3991	rBV2	1391	594	0.08%	0.010%
97	14.474	4173	4178	4180	rBV6	1857	1452	0.19%	0.024%
98	14.721	4251	4255	4256	rBV3	2027	1025	0.14%	0.017%
99	14.908	4310	4313	4314	rBV2	1607	853	0.11%	0.014%
100	15.120	4377	4379	4382	rBV4	1868	901	0.12%	0.015%




Sum of corrected areas: 6113223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030739.D
Acq On : 21 Apr 2023 00:28
Operator : SY/MD
Sample : 02440-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

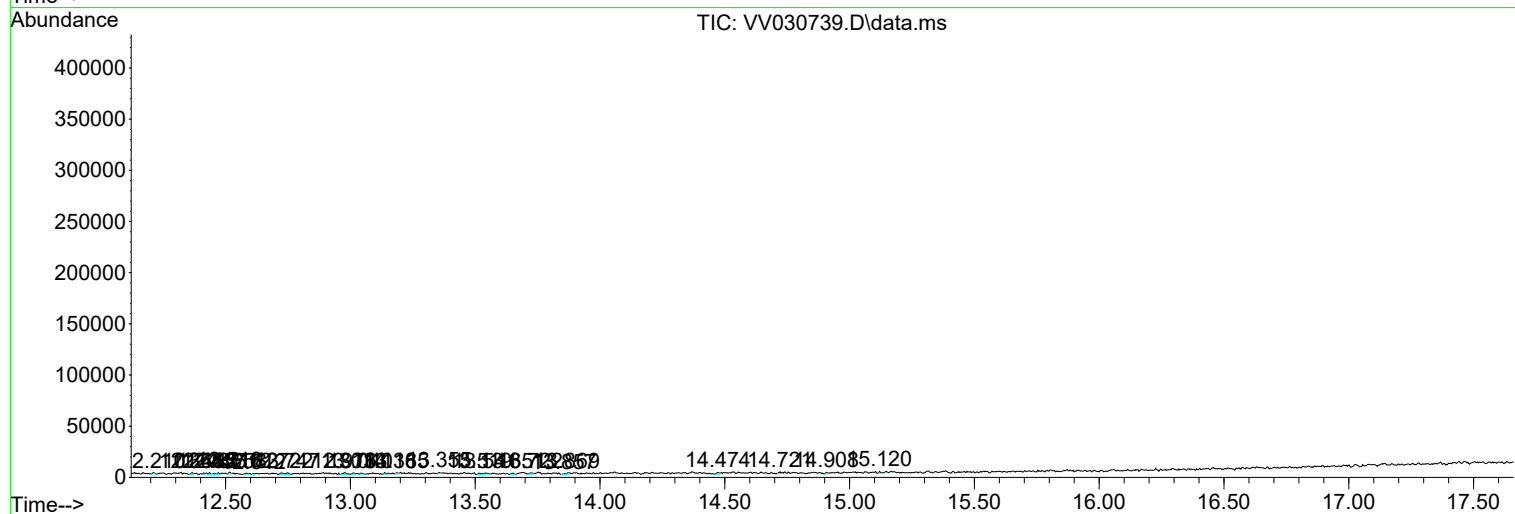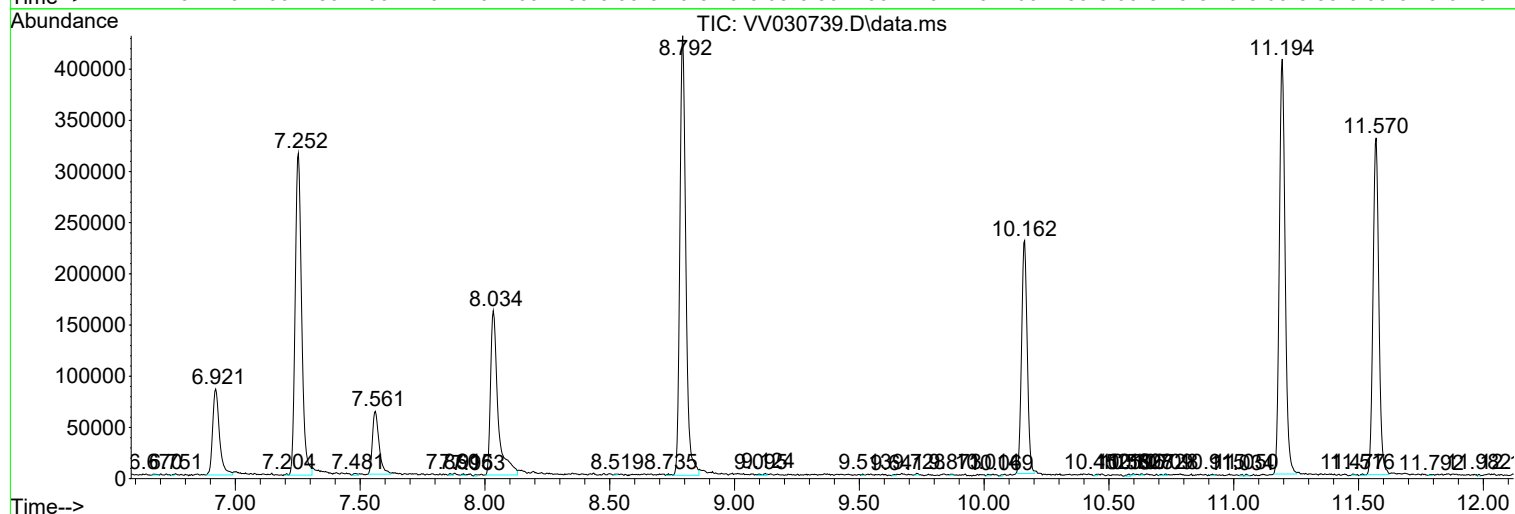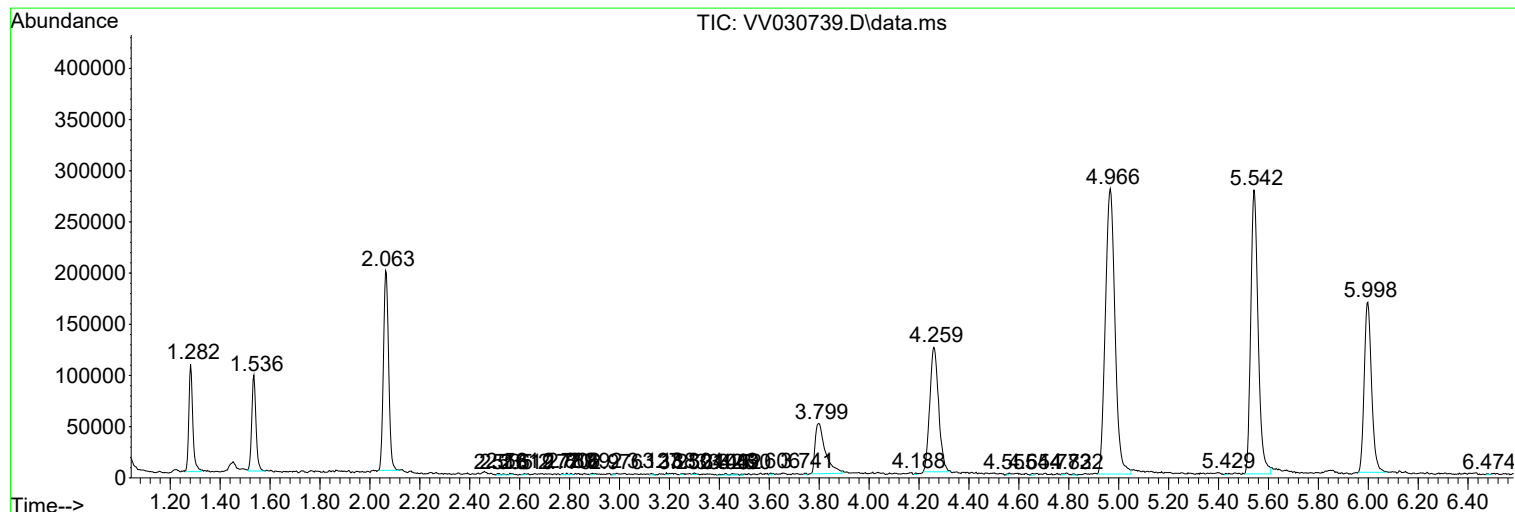

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030739.D
Acq On : 21 Apr 2023 00:28
Operator : SY/MD
Sample : 02440-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COMQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042023\
Data File : VV030739.D
Acq On : 21 Apr 2023 00:28
Operator : SY/MD
Sample : 02440-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------